

Data Path : S:\HPCHEM1\HPLC_L\Data\HL022713\
Data File : HL005089.D
Signal(s) : VWD1A.CH
Acq On : 27-Feb-2013, 19:57
Operator : QM
Sample : HSTDICV0500
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 01 00:29:05 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.480	2024637	464.716 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 154.91%#
Target Compounds			
2) L1 3,5-Dinitroaniline	4.412	6168498	438.216 ug/L
3) L2 PETN	21.723	4086641	447.839 ug/L m


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL022713\
Data File : HL005089.D
Signal(s) : VWD1A.CH
Acq On : 27-Feb-2013, 19:57
Operator : QM
Sample : HSTDICV0500
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 01 00:29:05 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. :
Signal Phase :
Signal Info :

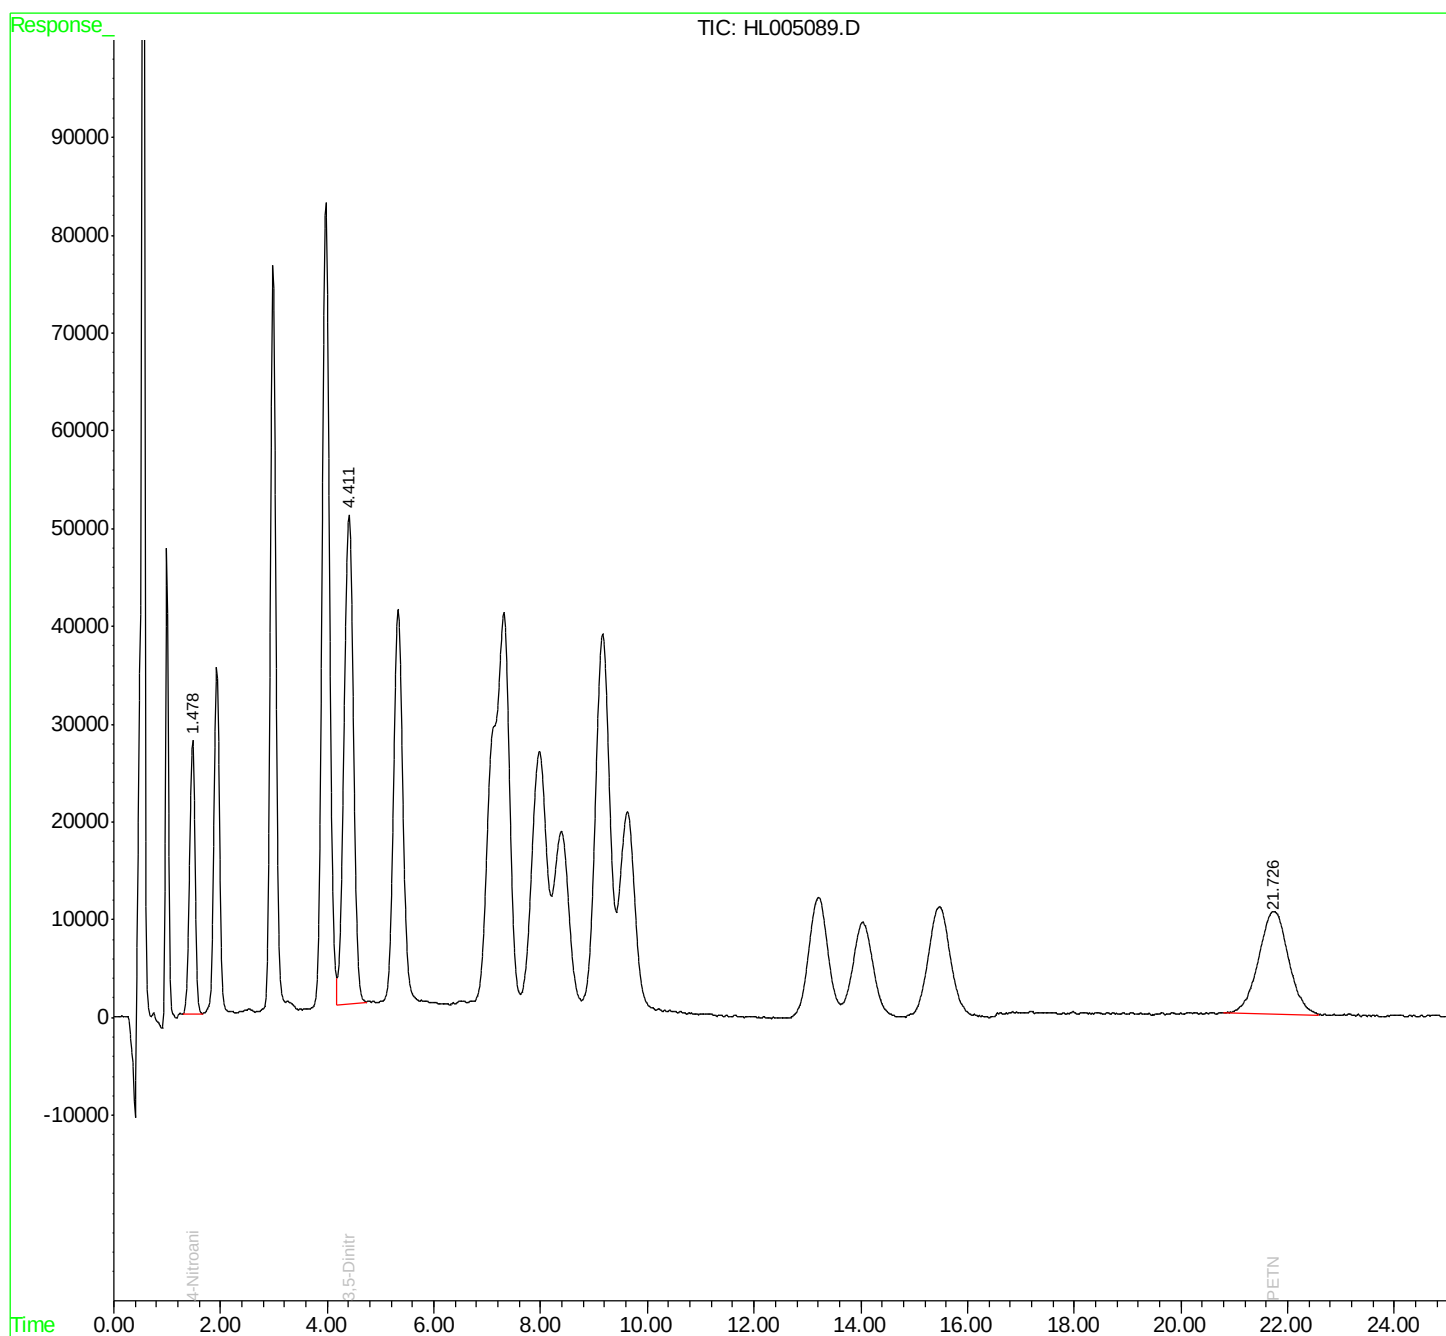

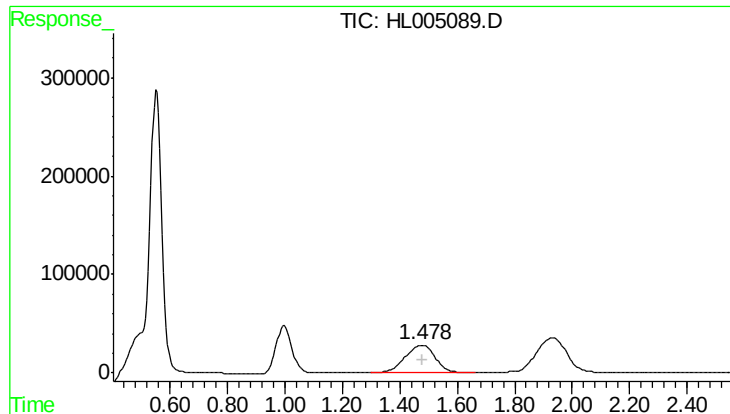


#1 4-Nitroaniline

R.T.: 1.480 min
Delta R.T.: 0.000 min
Response: 2024637
Conc: 464.72 ug/L

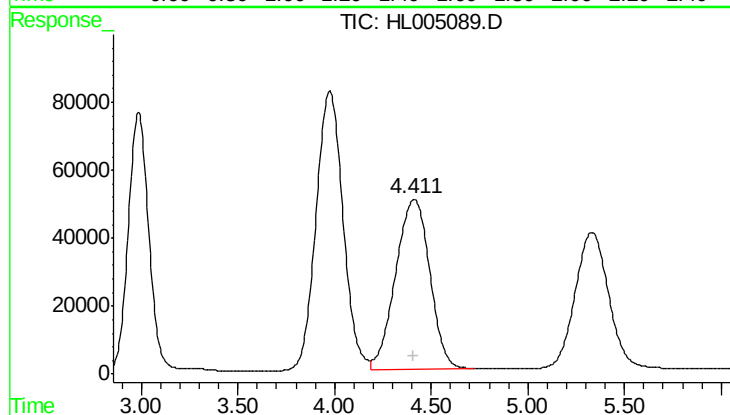

#2 3,5-Dinitroaniline

R.T.: 4.412 min
Delta R.T.: 0.002 min
Response: 6168498
Conc: 438.22 ug/L

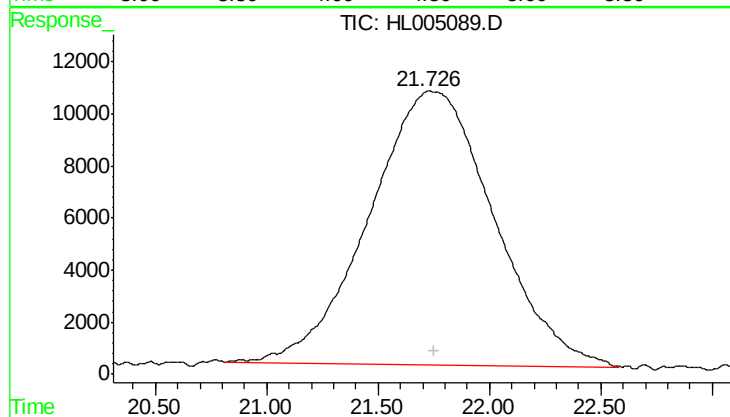

#3 PETN

R.T.: 21.723 min
Delta R.T.: -0.027 min
Response: 4086641
Conc: 447.84 ug/L m