

Data Path : S:\HPCHEM1\HPLC_L\Data\HL022713\
Data File : HL005100.D
Signal(s) : VWD1A.CH
Acq On : 28-Feb-2013, 00:54
Operator : QM
Sample : HSTDCCC0500
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 01 00:32:25 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.477	2180960	500.597 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 166.87%#
Target Compounds			
2) L1 3,5-Dinitroaniline	4.401	7074874	502.606 ug/L
3) L2 PETN	21.704	4736578	519.063 ug/L m


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL022713\
Data File : HL005100.D
Signal(s) : VWD1A.CH
Acq On : 28-Feb-2013, 00:54
Operator : QM
Sample : HSTDCCC0500
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 01 00:32:25 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. :
Signal Phase :
Signal Info :

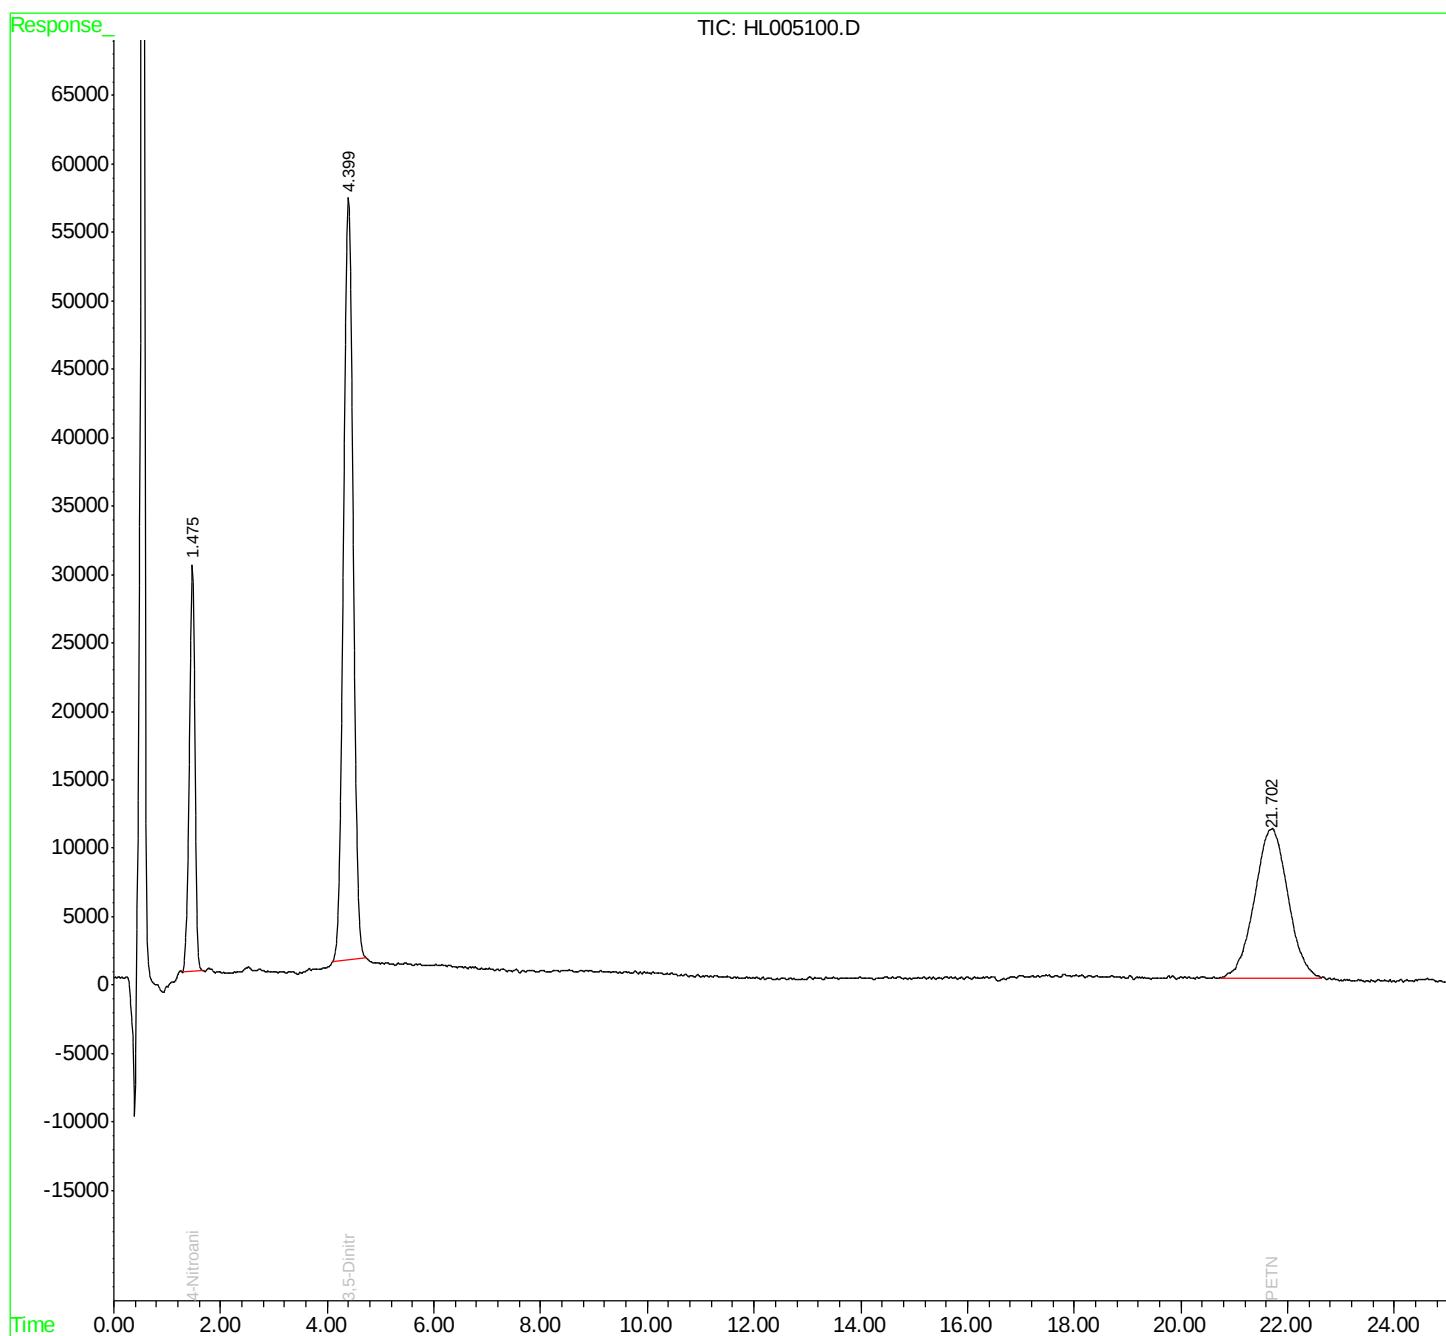

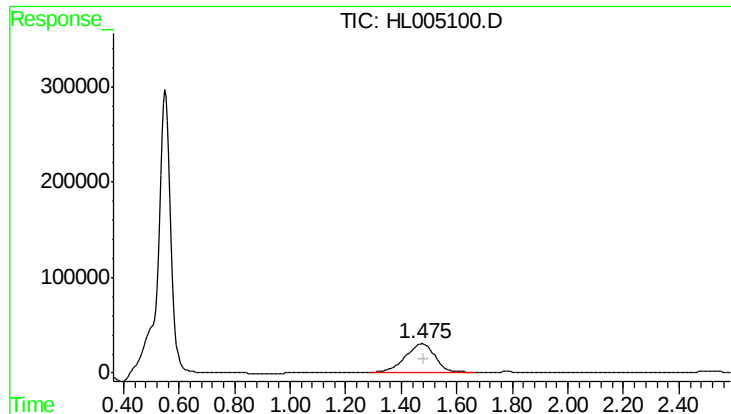


#1 4-Nitroaniline

R.T.: 1.477 min
Delta R.T.: -0.003 min
Response: 2180960
Conc: 500.60 ug/L

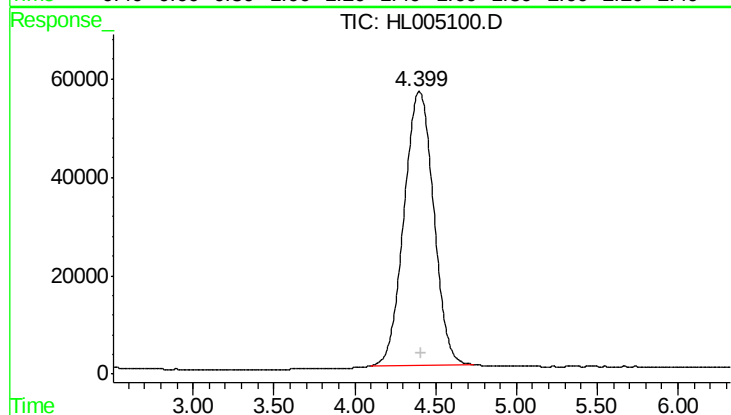

#2 3,5-Dinitroaniline

R.T.: 4.401 min
Delta R.T.: -0.009 min
Response: 7074874
Conc: 502.61 ug/L

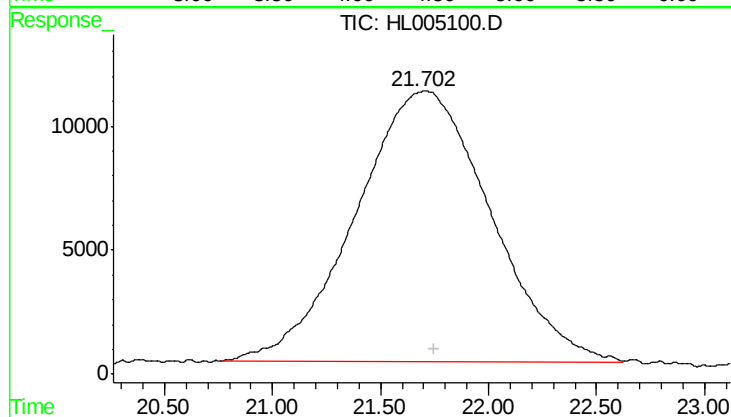

#3 PETN

R.T.: 21.704 min
Delta R.T.: -0.046 min
Response: 4736578
Conc: 519.06 ug/L m