

Data Path : S:\HPCHEM1\HPLC_L\Data\HL022713\
Data File : HL005108.D
Signal(s) : VWD1A.CH
Acq On : 28-Feb-2013, 04:30
Operator : QM
Sample : E1390-16
Misc :
ALS Vial : 75 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 01 00:33:54 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.472	1138667	261.359 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 87.12%
Target Compounds			
2) L1 3,5-Dinitroaniline	4.409	89701	6.372 ug/L m
3) L2 PETN	21.713	160606	17.600 ug/L m


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL022713\
Data File : HL005108.D
Signal(s) : VWD1A.CH
Acq On : 28-Feb-2013, 04:30
Operator : QM
Sample : E1390-16
Misc :
ALS Vial : 75 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 01 00:33:54 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. :
Signal Phase :
Signal Info :

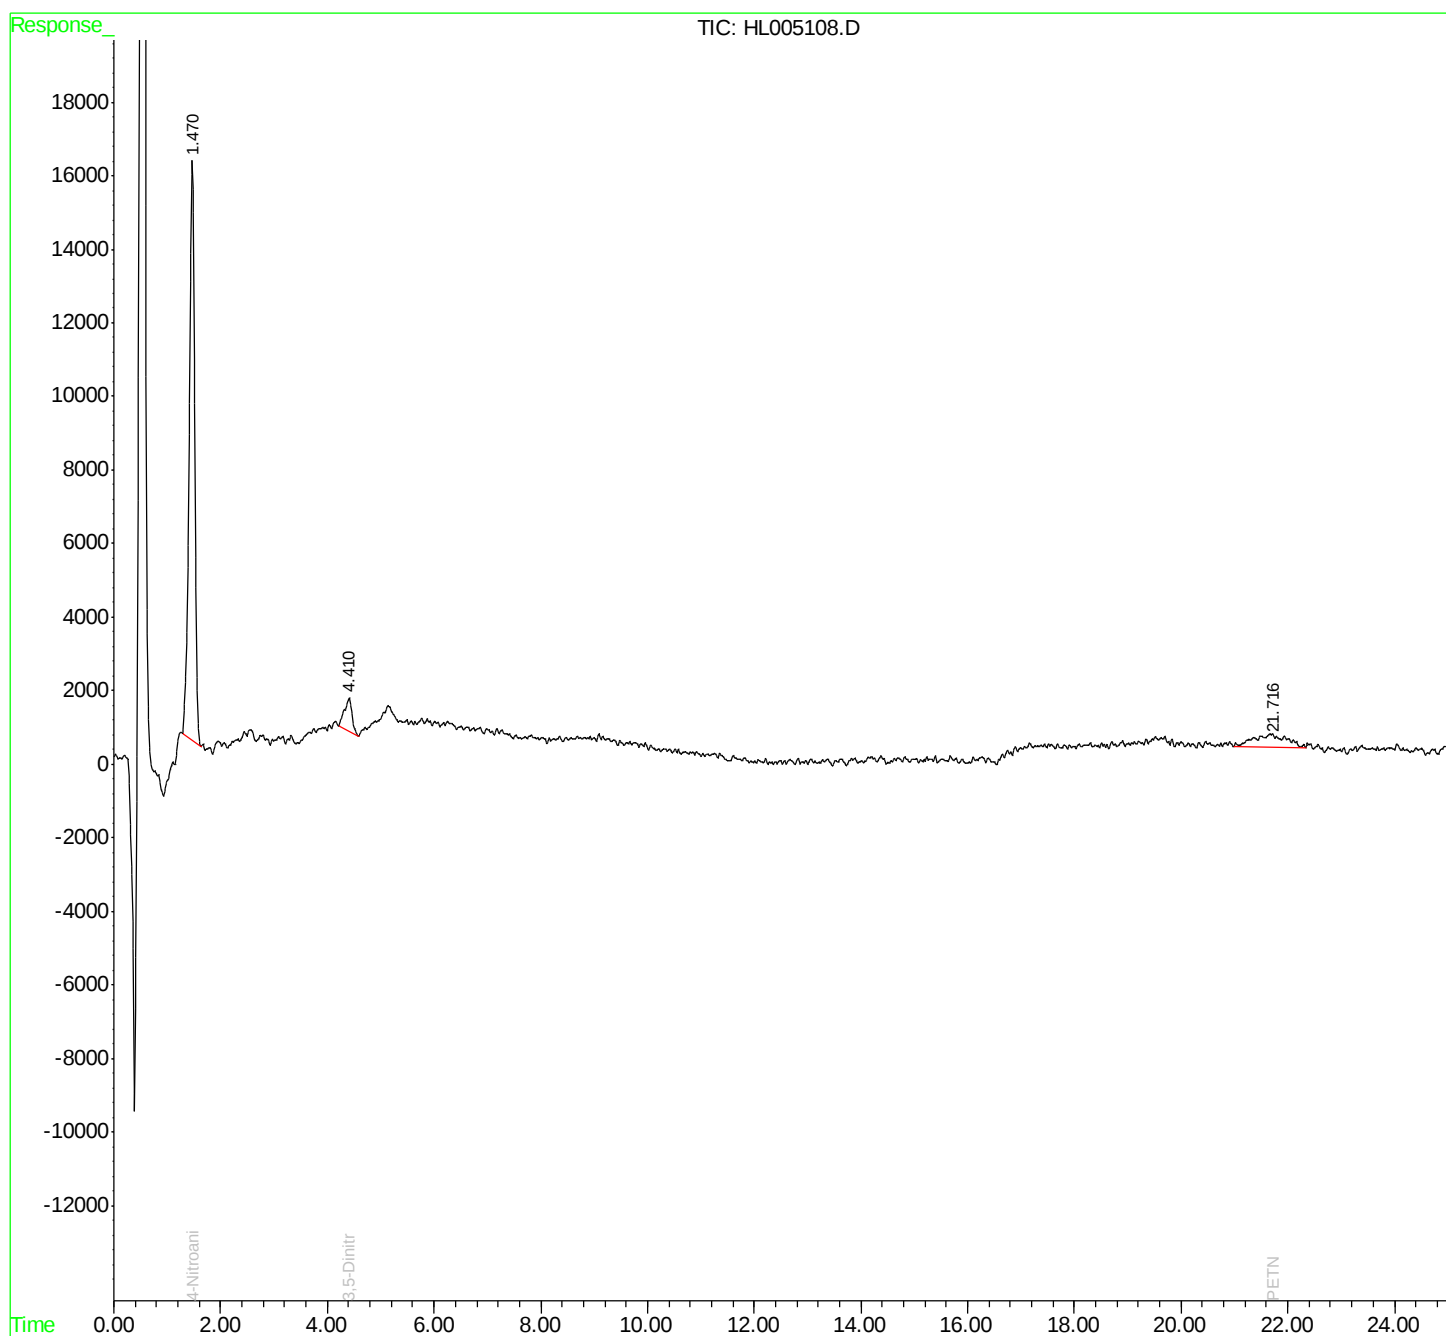

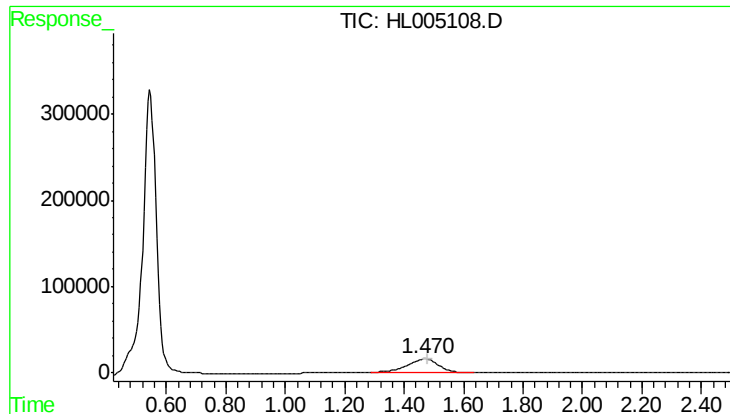


#1 4-Nitroaniline

R.T.: 1.472 min
 Delta R.T.: -0.008 min
 Response: 1138667
 Conc: 261.36 ug/L

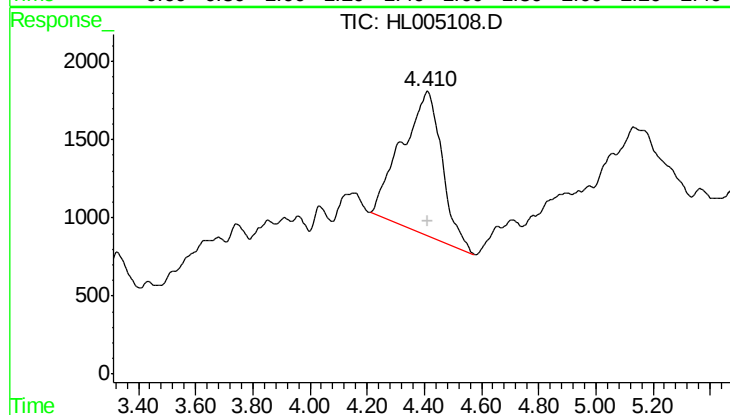

#2 3,5-Dinitroaniline

R.T.: 4.409 min
 Delta R.T.: -0.001 min
 Response: 89701
 Conc: 6.37 ug/L m

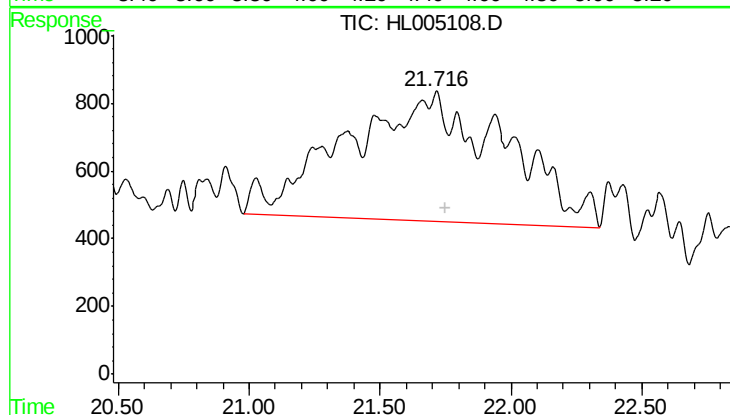

#3 PETN

R.T.: 21.713 min
 Delta R.T.: -0.037 min
 Response: 160606
 Conc: 17.60 ug/L m