

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL031016\  
Data File : HL006306.D  
Signal(s) : vwd1A.ch  
Acq On : 10-Mar-2016, 11:24  
Operator : UM/MA  
Sample : G4825-05  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
LOD-WATER2016-01

Manual Integrations  
APPROVED

Sohil  
3/10/2016 3:39:43 PM

Integration File: AUTOINT1.E  
Quant Time: Mar 10 12:14:14 2016  
Quant Method : Z:\HPCHEM1\HPLC\_L\Methods\HL0308NG.M  
Quant Title :  
QLast Update : Tue Mar 08 16:18:46 2016  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 1) S 4-Nitroaniline         | 2.175 | 2623490  | 0.518 ng/ulm |
| Target Compounds            |       |          |              |
| 2) T Nitroglycerin          | 6.617 | 3343438  | 0.312 ng/ul  |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL031016\  
Data File : HL006306.D  
Signal(s) : vwd1A.ch  
Acq On : 10-Mar-2016, 11:24  
Operator : UM/MA  
Sample : G4825-05  
Misc :  
ALS Vial : 3 Sample Multiplier: 1


Instrument :  
HPLC\_L  
ClientSampleId :  
LOD-WATER2016-01


Manual Integrations  
APPROVED

Sohil  
3/10/2016 3:39:43 PM

Integration File: AUTOINT1.E  
Quant Time: Mar 10 12:14:14 2016  
Quant Method : Z:\HPCHEM1\HPLC\_L\Methods\HL0308NG.M  
Quant Title :  
QLast Update : Tue Mar 08 16:18:46 2016  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

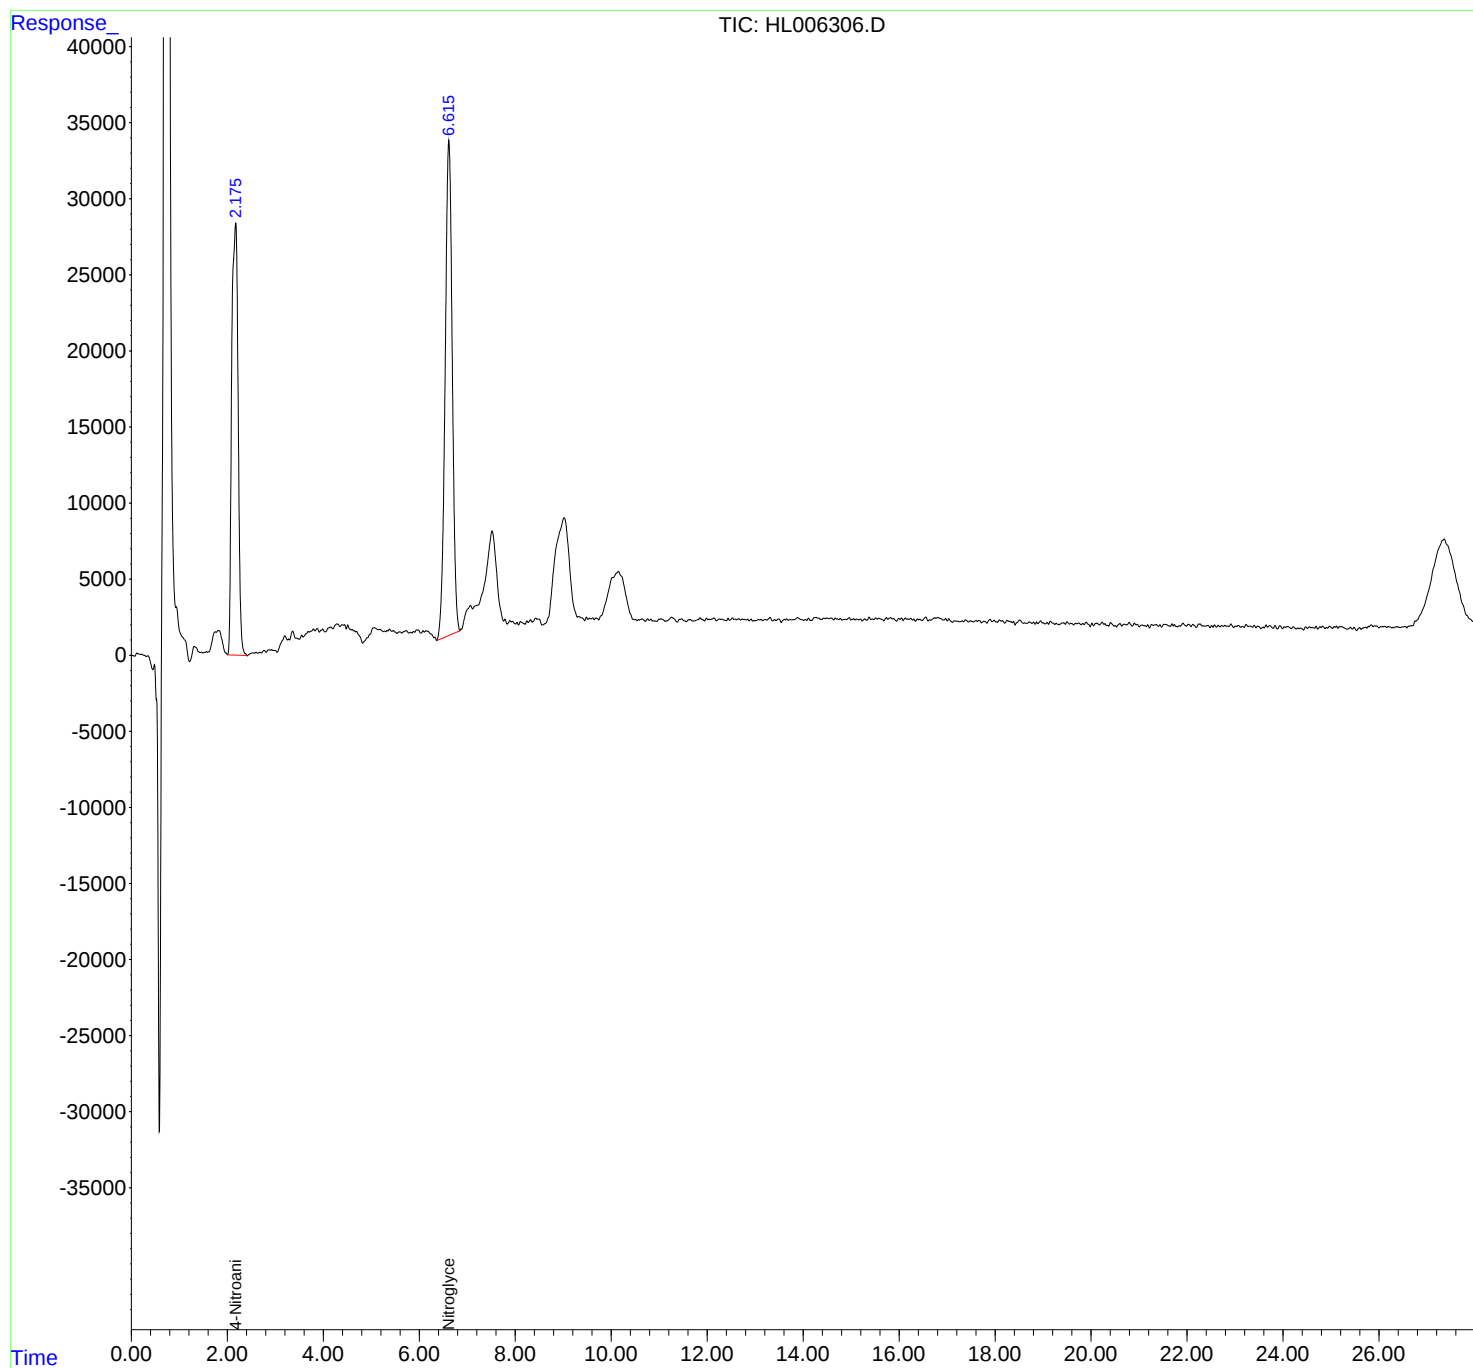

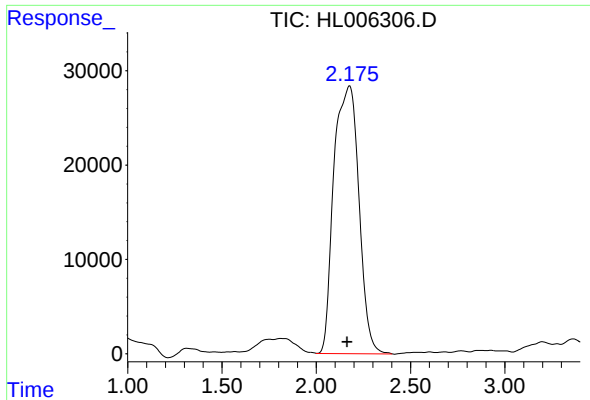


#1 4-Nitroaniline

R.T.: 2.175 min  
Delta R.T.: 0.011 min  
Response: 2623490  
Conc: 0.52 ng/ul m

Instrument :  
HPLC\_L  
ClientSampleId :  
LOD-WATER2016-01

Manual Integrations  
APPROVED

Sohil  
3/10/2016 3:39:43 PM

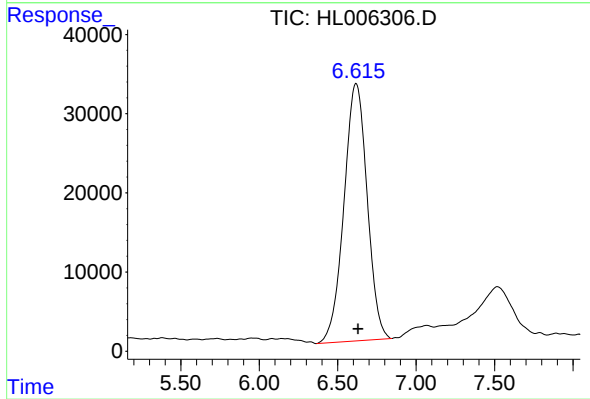

#2 Nitroglycerin

R.T.: 6.617 min  
Delta R.T.: -0.013 min  
Response: 3343438  
Conc: 0.31 ng/ul