

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL031315\
 Data File : HL006119.D
 Signal(s) : vwd1A.ch
 Acq On : 13-Mar-2015, 15:57
 Operator : TP/IZ
 Sample : HSTDICCC0500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICCC0500

Integration File: AUTOINT1.E
 Quant Time: Mar 16 07:19:37 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL031315.M
 Quant Title :
 QLast Update : Mon Mar 16 07:19:22 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.586	6135113	500.000 ug/L
Target Compounds			
2) T HMX	1.474	2803347	500.000 ug/L
3) T RDX	2.586	6135113	500.000 ug/L
4) T 1,3,5-Trinitrobenzene	4.125	7094192	500.000 ug/L
5) T 1,3-Dinitrobenzene	5.473	10628144	500.000 ng/ml
6) T 3,5-Dinitroaniline	6.426	8215962	500.000 ug/L
7) T Nitrobenzene	7.057	6263117	500.000 ug/L
8) T Tetryl	9.558	3962001	500.000 ug/L
9) T 2,4,6-Trinitrotoluene	9.980	6590745	500.000 ug/L
10) T 2-Amino-4,6-dinitroto...	11.575	6962939	500.000 ug/L
11) T 4-Amino-2,6-dinitroto...	12.173	4492422	500.000 ug/L
12) T 2,4-Dinitrotoluene	12.824	9593023	500.000 ug/L
13) T 2,6-Dinitrotoluene	13.256	5307412	500.000 ug/L
14) T 2-Nitrotoluene	17.871	12277667	533.590 ug/L
15) T 4-Nitrotoluene	19.434	8014236	492.906 ug/L
16) T 3-Nitrotoluene	21.036	12612079	495.126 ug/L
17) T PETN	21.843	4761544	501.354 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL031315\
Data File : HL006119.D
Signal(s) : vwd1A.ch
Acq On : 13-Mar-2015, 15:57
Operator : TP/IZ
Sample : HSTDICCC0500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500

Integration File: AUTOINT1.E
Quant Time: Mar 16 07:19:37 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL031315.M
Quant Title :
QLast Update : Mon Mar 16 07:19:22 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

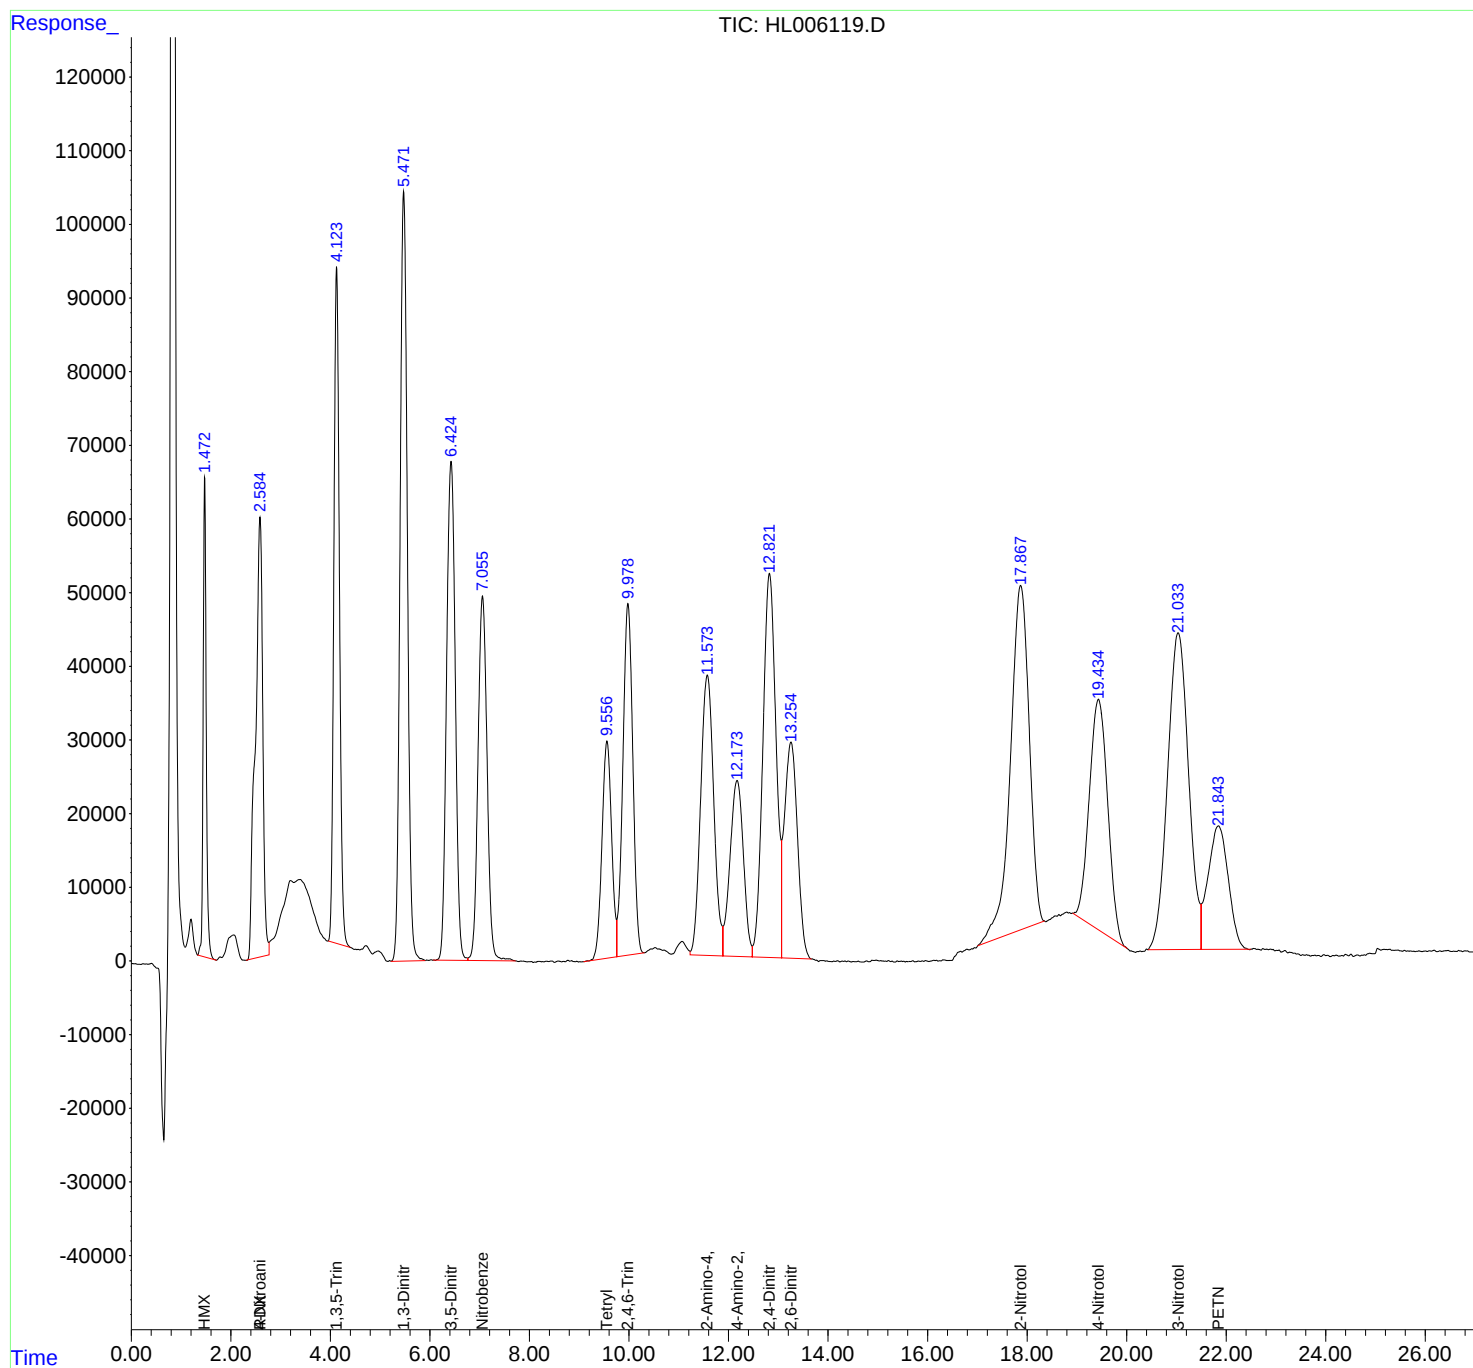


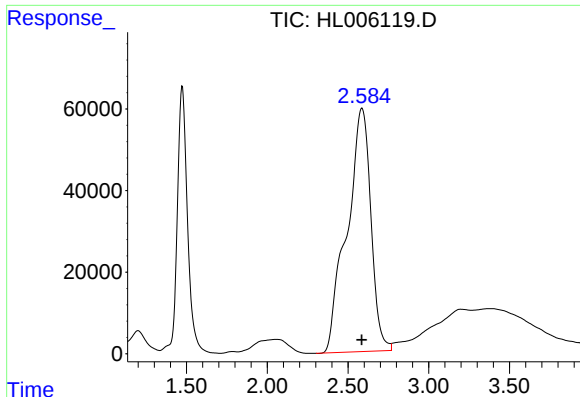

#1 4-Nitroaniline


R.T.: 2.586 min
Delta R.T.: 0.000 min
Response: 6135113
Conc: 500.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500

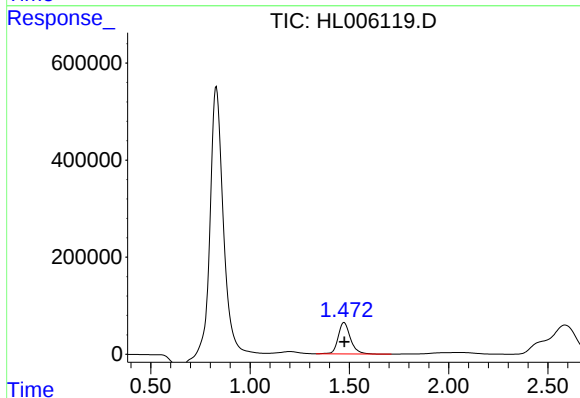


#2 HMX

R.T.: 1.474 min
Delta R.T.: 0.000 min
Response: 2803347
Conc: 500.00 ug/L

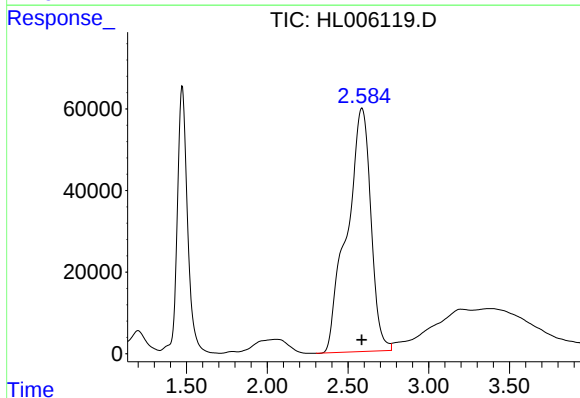


#3 RDX

R.T.: 2.586 min
Delta R.T.: 0.000 min
Response: 6135113
Conc: 500.00 ug/L

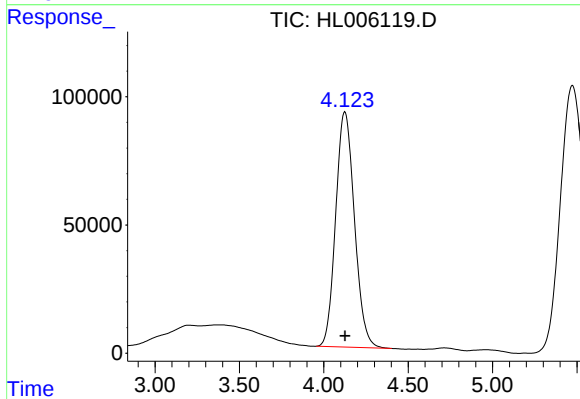

#4 1,3,5-Trinitrobenzene


R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 7094192
Conc: 500.00 ug/L

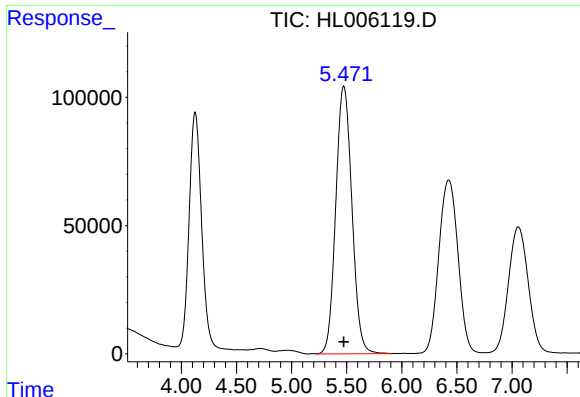

#5 1,3-Dinitrobenzene


R.T.: 5.473 min
Delta R.T.: 0.000 min
Response: 10628144
Conc: 500.00 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500

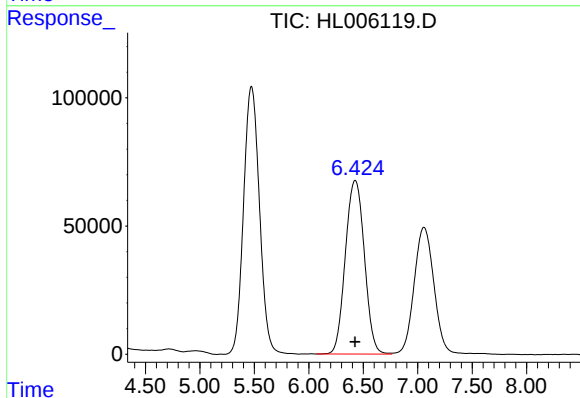


#6 3,5-Dinitroaniline

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 8215962
Conc: 500.00 ug/L

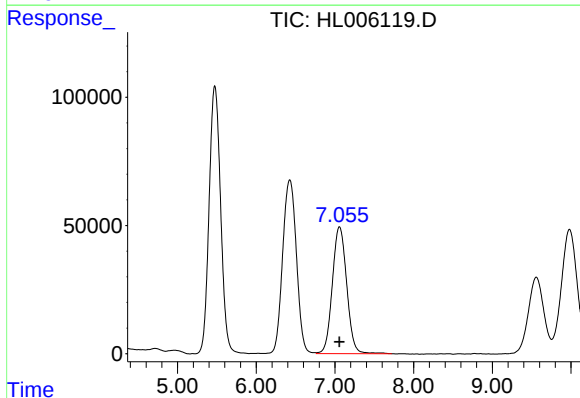


#7 Nitrobenzene

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 6263117
Conc: 500.00 ug/L

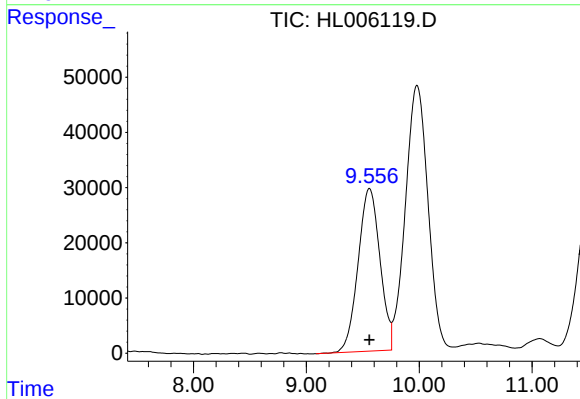

#8 Tetryl


R.T.: 9.558 min
Delta R.T.: 0.000 min
Response: 3962001
Conc: 500.00 ug/L

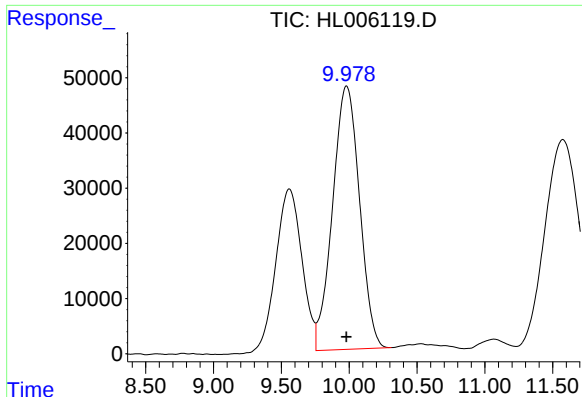

#9 2,4,6-Trinitrotoluene


R.T.: 9.980 min
Delta R.T.: 0.000 min
Response: 6590745
Conc: 500.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500

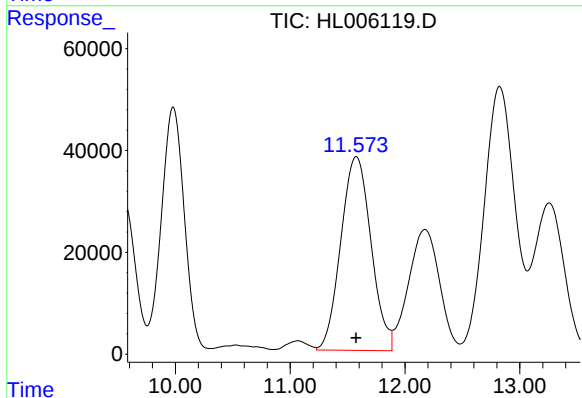


#10 2-Amino-4,6-dinitrotoluene

R.T.: 11.575 min
Delta R.T.: 0.000 min
Response: 6962939
Conc: 500.00 ug/L

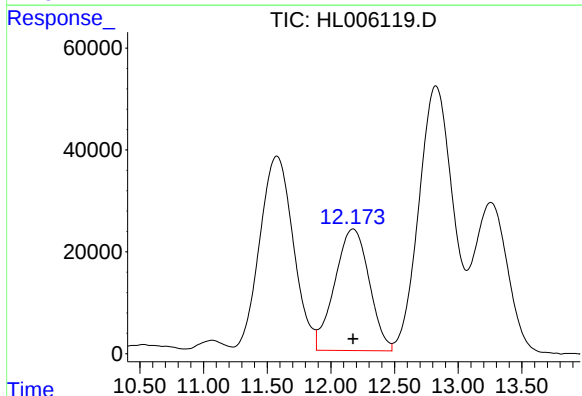


#11 4-Amino-2,6-dinitrotoluene

R.T.: 12.173 min
Delta R.T.: 0.000 min
Response: 4492422
Conc: 500.00 ug/L

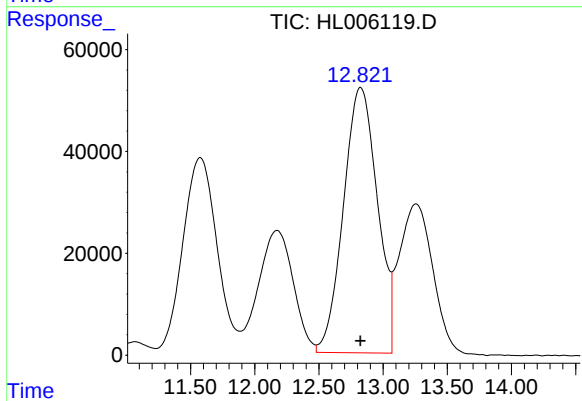

#12 2,4-Dinitrotoluene

R.T.: 12.824 min
Delta R.T.: 0.000 min
Response: 9593023
Conc: 500.00 ug/L

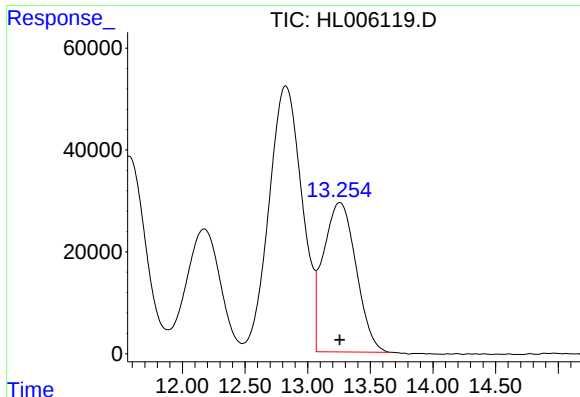

#13 2,6-Dinitrotoluene


R.T.: 13.256 min

Delta R.T.: 0.000 min

Response: 5307412

Conc: 500.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500

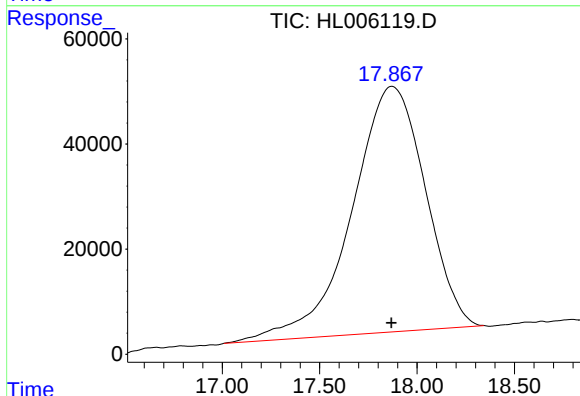


#14 2-Nitrotoluene

R.T.: 17.871 min

Delta R.T.: 0.002 min

Response: 12277667

Conc: 533.59 ug/L

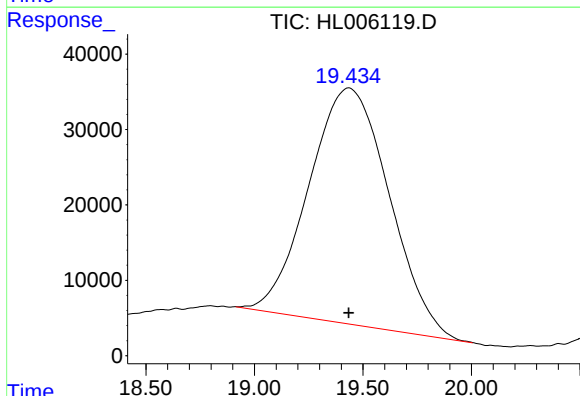


#15 4-Nitrotoluene

R.T.: 19.434 min

Delta R.T.: 0.000 min

Response: 8014236

Conc: 492.91 ug/L

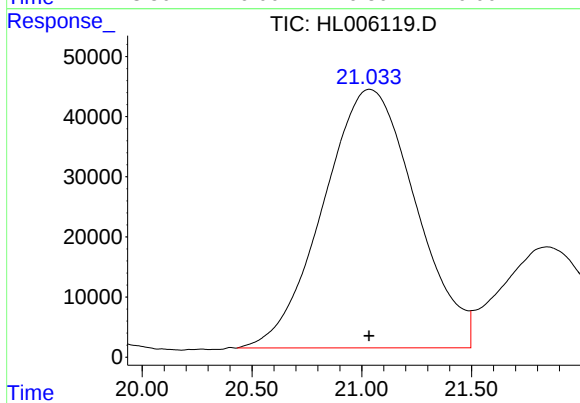


#16 3-Nitrotoluene

R.T.: 21.036 min

Delta R.T.: 0.003 min

Response: 12612079

Conc: 495.13 ug/L

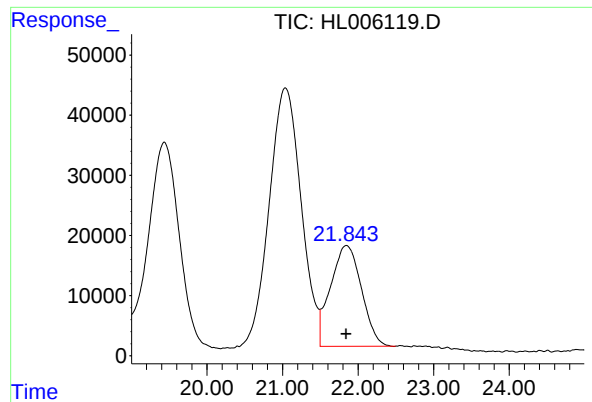

#17 PETN

R.T.: 21.843 min
Delta R.T.: 0.000 min
Response: 4761544
Conc: 501.35 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500