

Data File : H:\VOL1\HPLC\HPLC L\120316\HL002129.D Vial: 13
Acq On : 16-Mar-2012, 18:18 Operator: HLM
Sample : PB61713BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Mar 19 11:15 2012 Quant Results File: HL022712.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL022712.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Mar 19 11:16:51 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.40	1164270	307.917 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 102.64%


Target Compounds


11) T	1,3-Dinitrobenzene	3.72	36676	2.176 ug/L
16) T	3,5-Dinitroaniline	4.05	4882	0.303 ug/L
17) T	Nitroglycerin	6.28	286561	5088.347 ug/L

Data File : H:\VOL1\HPLC\HPLC L\120316\HL002129.D Vial: 13
Acq On : 16-Mar-2012, 18:18 Operator: HLM
Sample : PB61713BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Mar 19 11:15 2012 Quant Results File: HL022712.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL022712.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Mar 19 11:16:51 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M


Volume Inj. :
Signal Phase :
Signal Info :

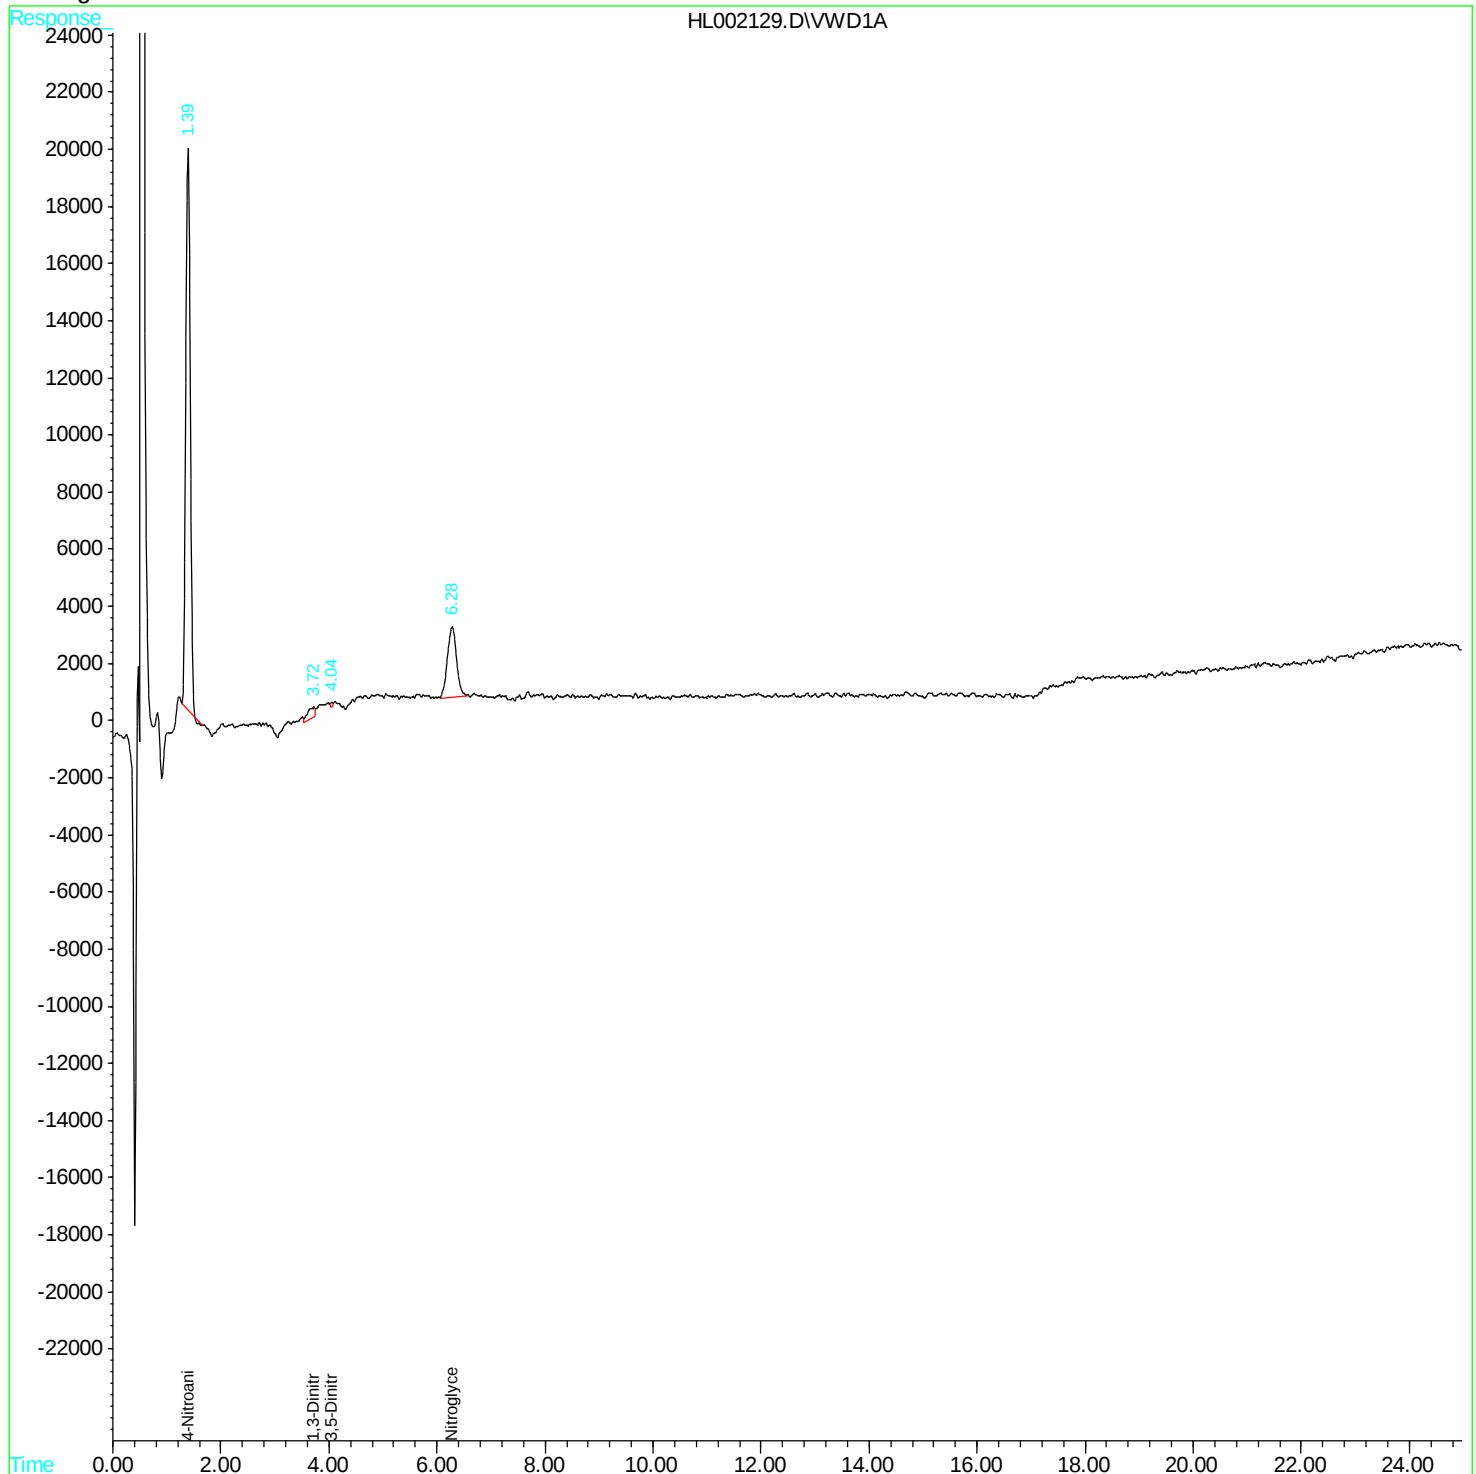

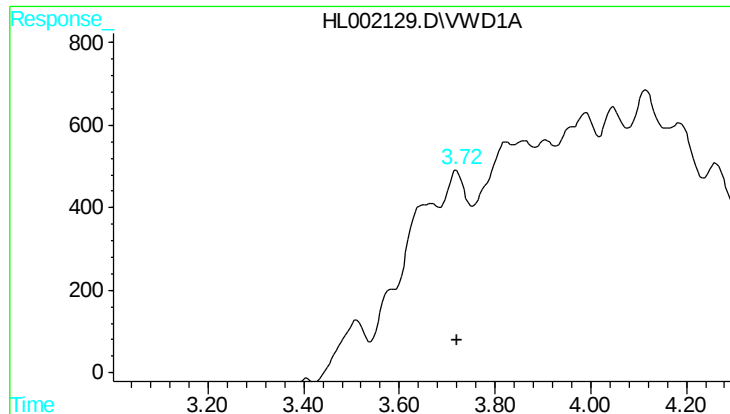


#11 1,3-Dinitrobenzene

R.T.: 3.720 min
Delta R.T.: -0.002 min
Response: 36676
Conc: 2.18 ug/L

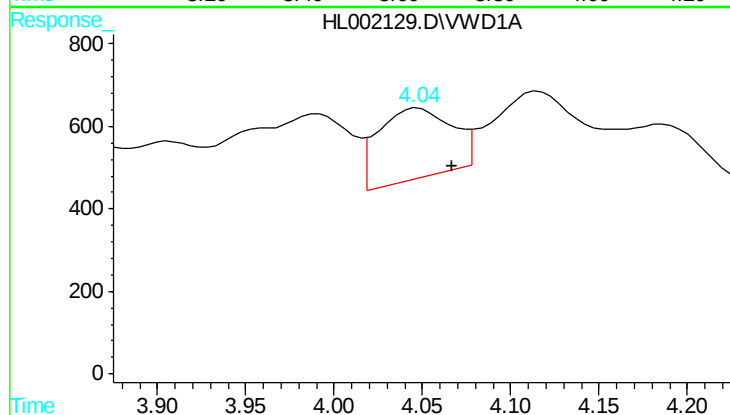

#16 3,5-Dinitroaniline

R.T.: 4.047 min
Delta R.T.: -0.019 min
Response: 4882
Conc: 0.30 ug/L

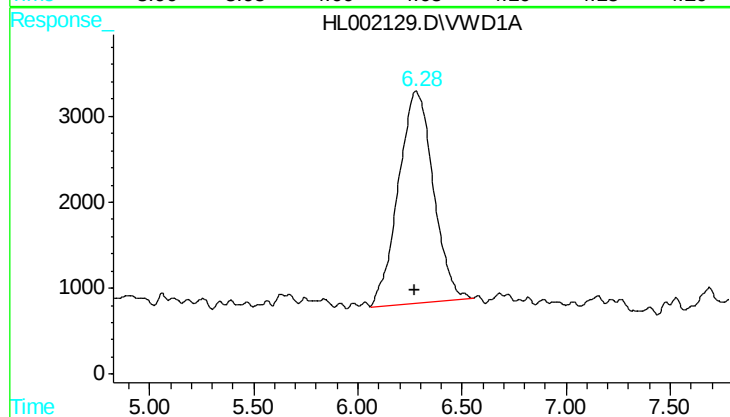

#17 Nitroglycerin

R.T.: 6.279 min
Delta R.T.: 0.006 min
Response: 286561
Conc: 5088.35 ug/L