

Data File : H:\VOL1\HPLC\HPLC L\120316\HL002132.D Vial: 16
Acq On : 16-Mar-2012, 19:41 Operator: HLM
Sample : D1801-19 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Mar 19 11:15 2012 Quant Results File: HL022712.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL022712.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Mar 19 11:16:51 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.40	1996904	528.126 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 176.04%#

Target Compounds


2) T	HMX	0.92f	42300	10.703 ug/L
16) T	3,5-Dinitroaniline	4.04f	83783	5.206 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120316\HL002132.D Vial: 16
 Acq On : 16-Mar-2012, 19:41 Operator: HLM
 Sample : D1801-19 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Mar 19 11:15 2012 Quant Results File: HL022712.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL022712.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Mar 19 11:16:51 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M


Volume Inj. :
 Signal Phase :
 Signal Info :

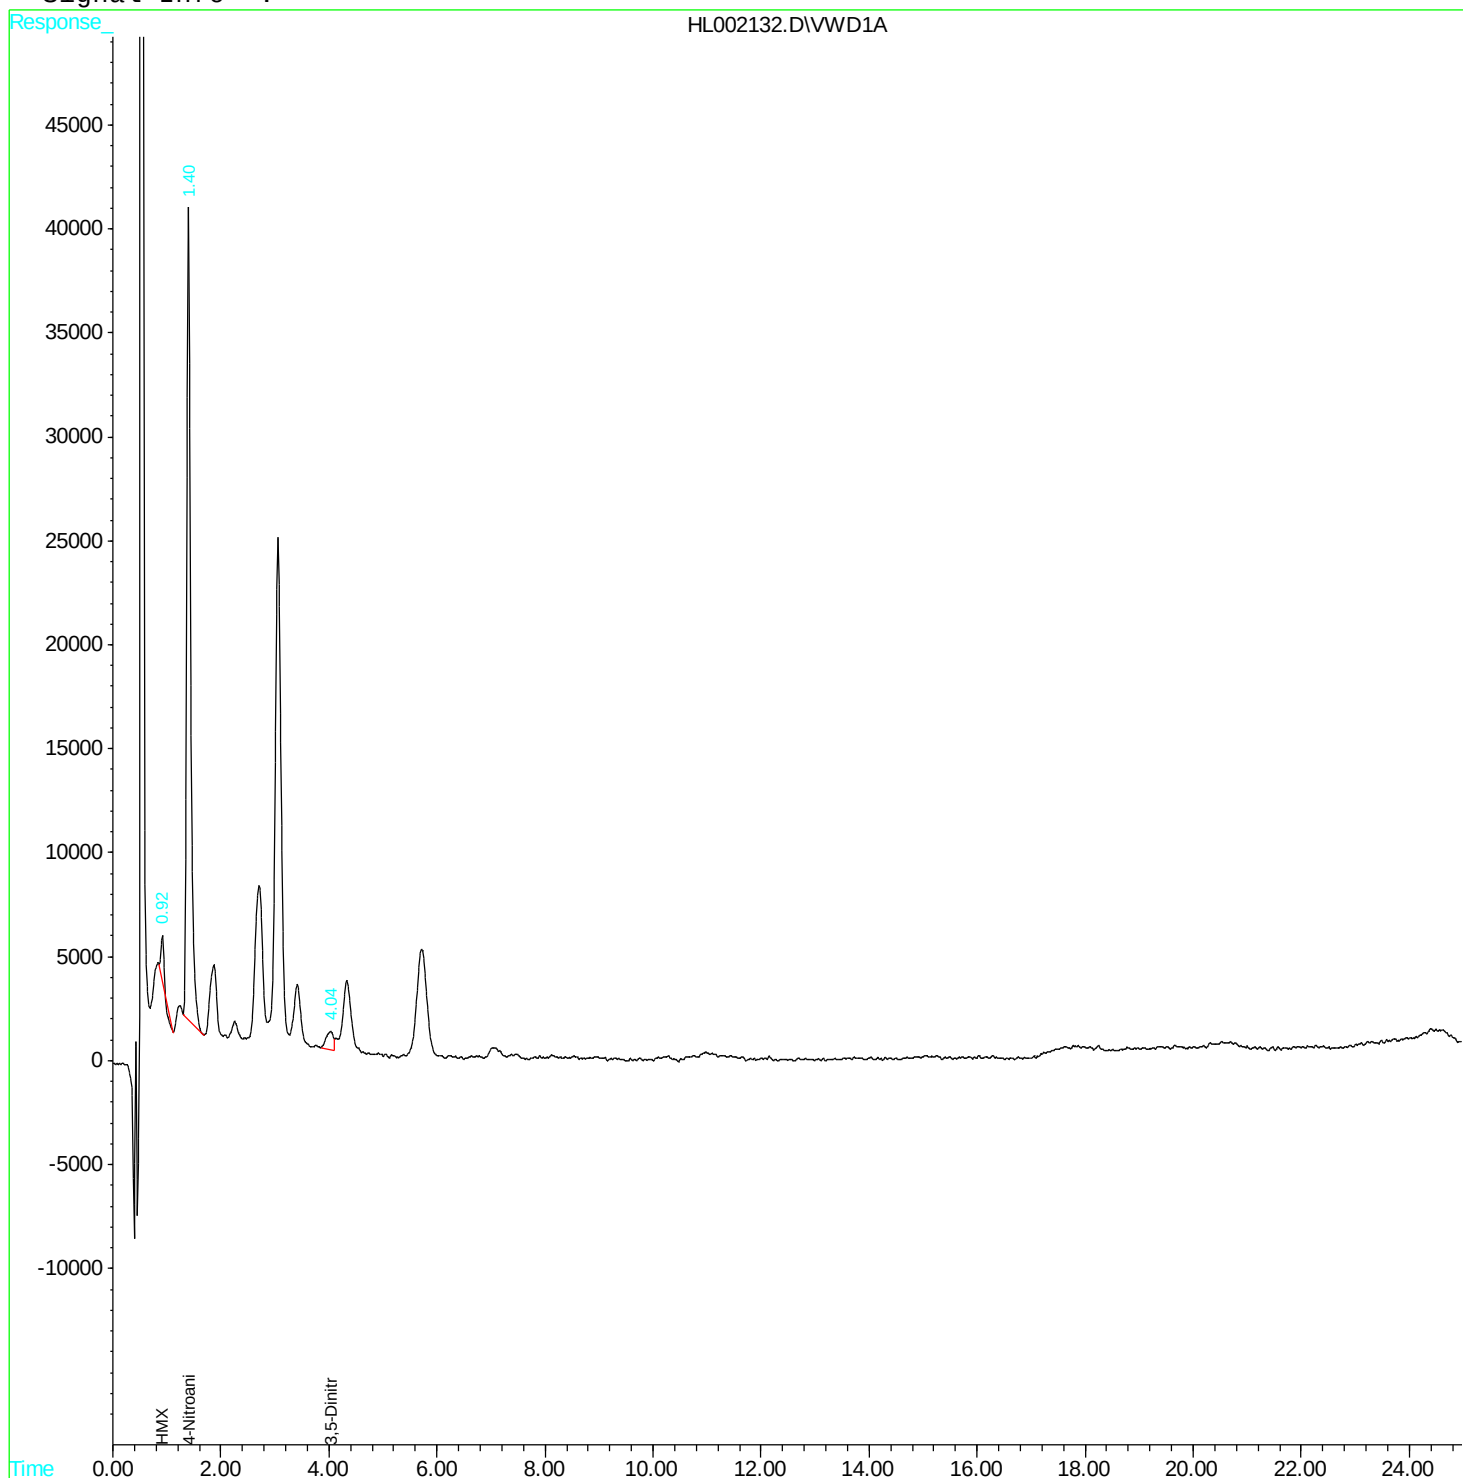

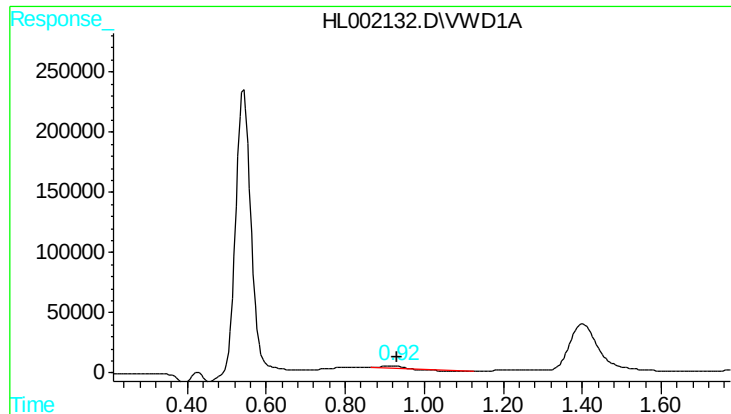

#2 HMX

R.T.: 0.919 min
Delta R.T.: -0.013 min
Response: 42300
Conc: 10.70 ug/L

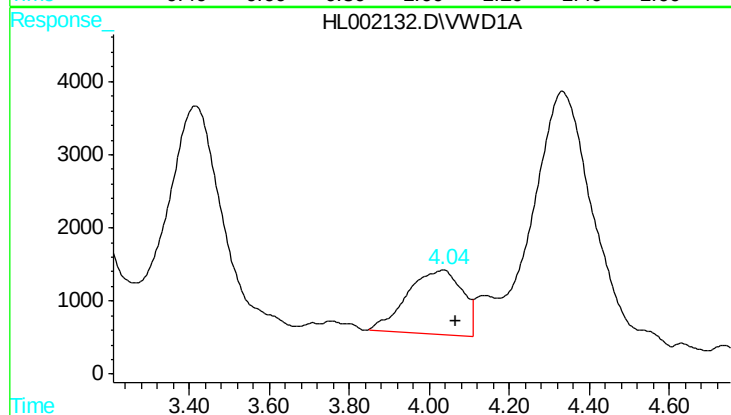

#16 3,5-Dinitroaniline

R.T.: 4.036 min
Delta R.T.: -0.031 min
Response: 83783
Conc: 5.21 ug/L