

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL031715\
 Data File : HL006154.D
 Signal(s) : vwd1A.ch
 Acq On : 17-Mar-2015, 18:33
 Operator : TP/IZ
 Sample : G1001-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 LOD-WATER2015-01

Integration File: AUTOINT1.E
 Quant Time: Mar 18 10:58:07 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL031615.M
 Quant Title :
 QLast Update : Tue Mar 17 09:09:29 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
9) T	2,4,6-Trinitrotoluene	10.327	598521	41.313 ug/L
10) T	2-Amino-4,6-dinitroto...	11.978	692891	42.686 ug/L
11) T	4-Amino-2,6-dinitroto...	12.586	486215	48.651 ug/L
12) T	2,4-Dinitrotoluene	13.258	1028828	49.157 ug/L
13) T	2,6-Dinitrotoluene	13.685	564130	52.005 ug/L
14) T	2-Nitrotoluene	18.353	2345002	86.835 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL031715\
Data File : HL006154.D
Signal(s) : vwd1A.ch
Acq On : 17-Mar-2015, 18:33
Operator : TP/IZ
Sample : G1001-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

Integration File: AUTOINT1.E
Quant Time: Mar 18 10:58:07 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL031615.M
Quant Title :
QLast Update : Tue Mar 17 09:09:29 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

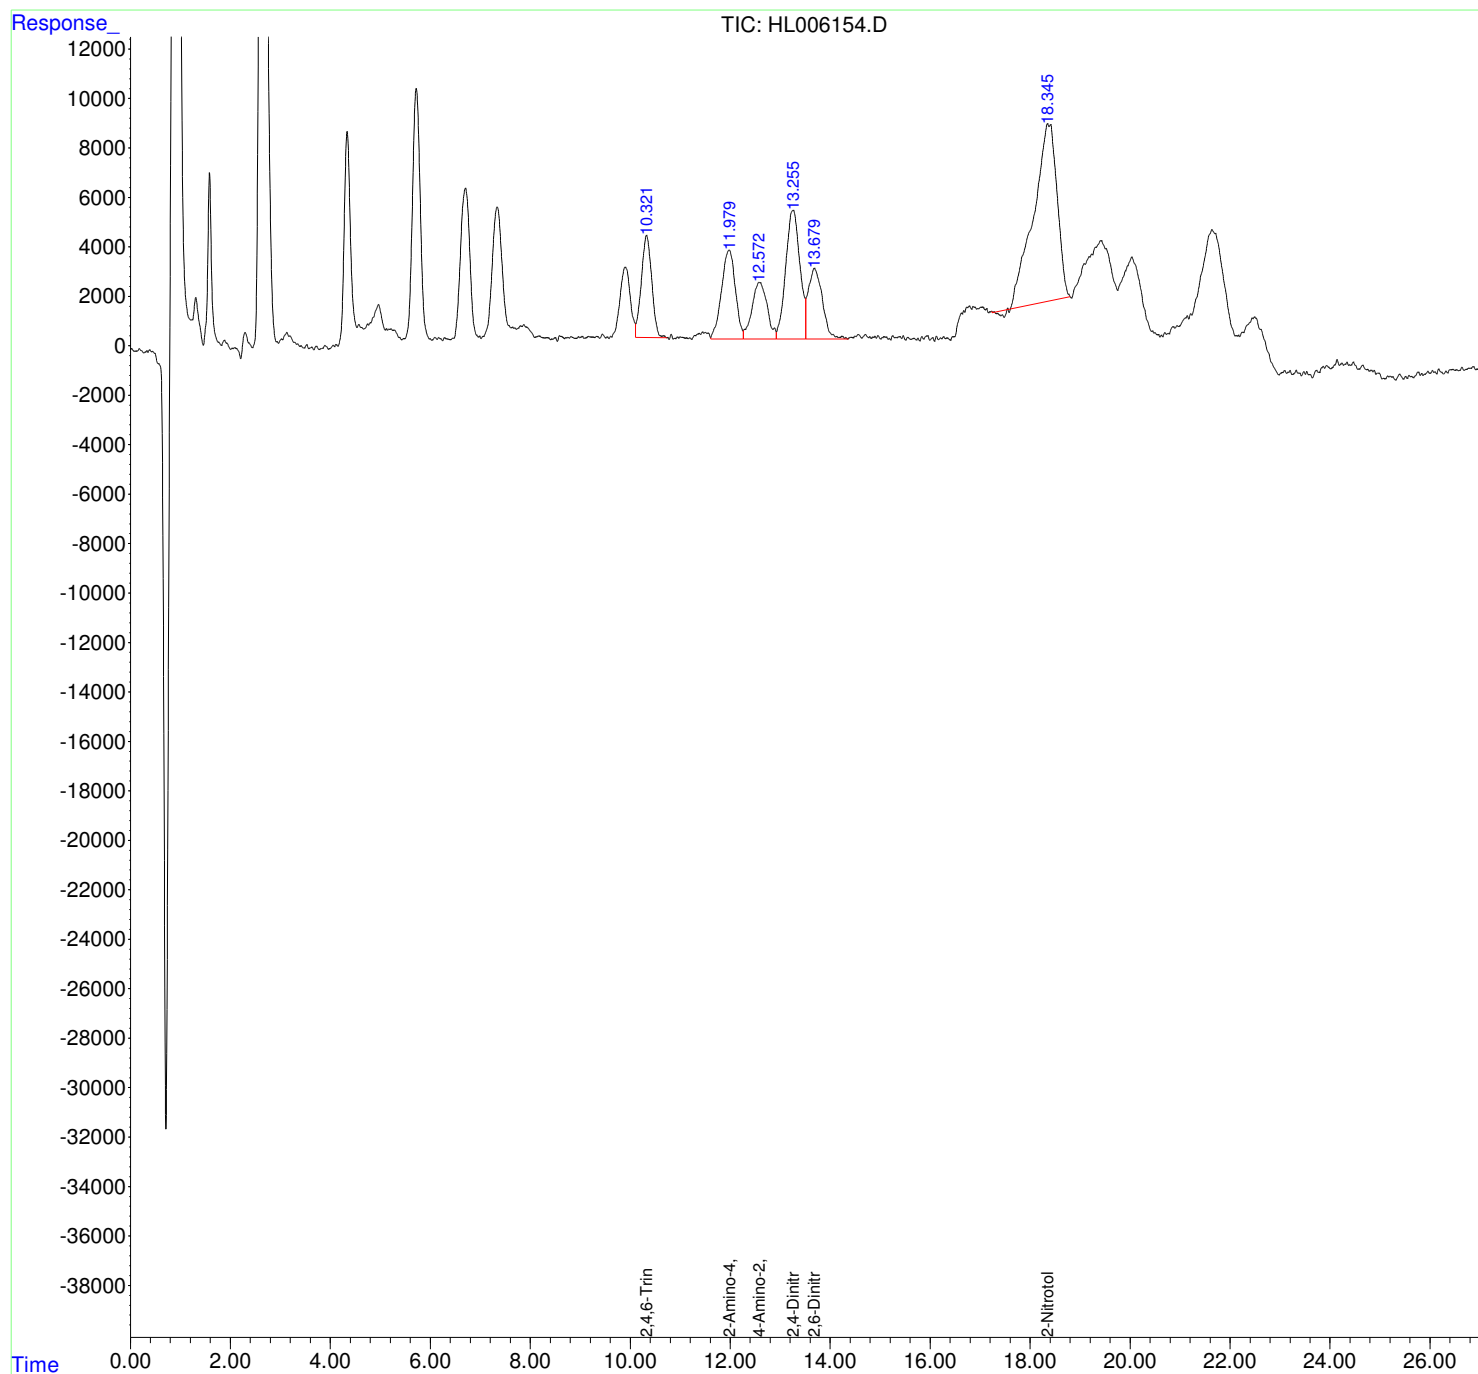


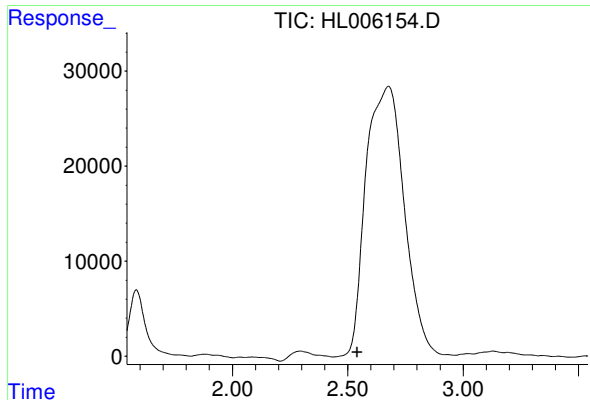

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.541 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

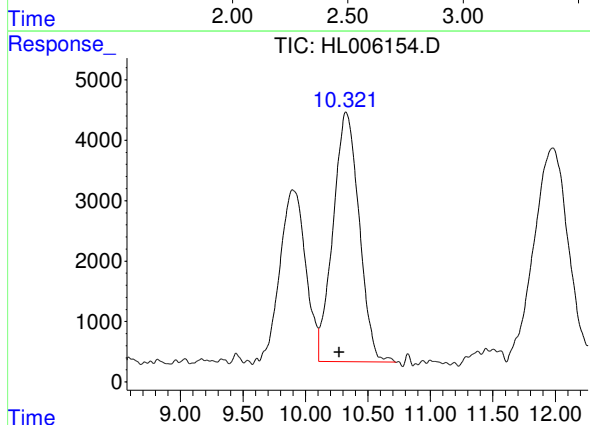


#9 2,4,6-Trinitrotoluene

R.T.: 10.327 min
Delta R.T.: 0.057 min
Response: 598521
Conc: 41.31 ug/L

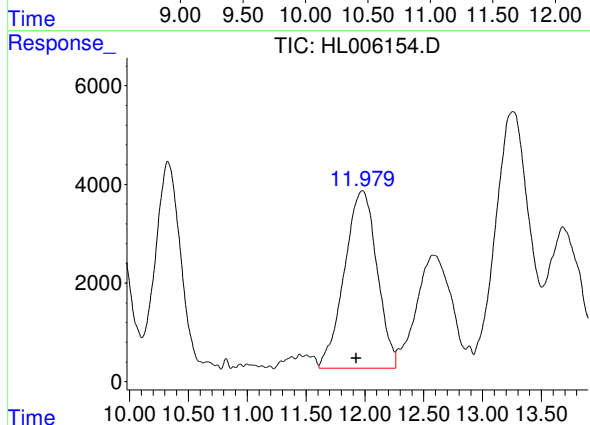


#10 2-Amino-4,6-dinitrotoluene

R.T.: 11.978 min
Delta R.T.: 0.052 min
Response: 692891
Conc: 42.69 ug/L

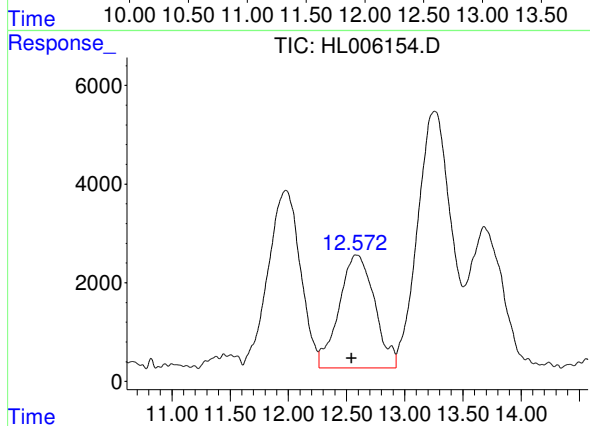

#11 4-Amino-2,6-dinitrotoluene


R.T.: 12.586 min
Delta R.T.: 0.042 min
Response: 486215
Conc: 48.65 ug/L

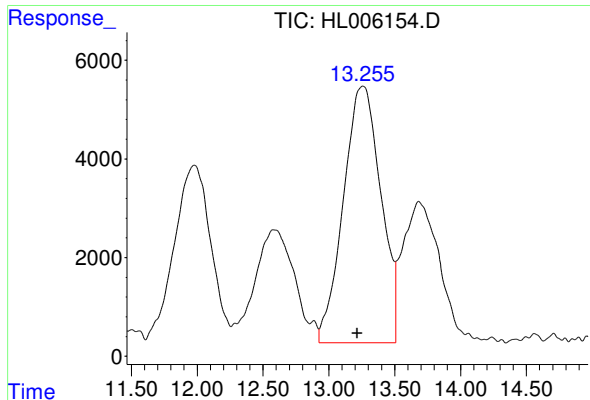

#12 2,4-Dinitrotoluene


R.T.: 13.258 min
Delta R.T.: 0.045 min
Response: 1028828
Conc: 49.16 ug/L

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

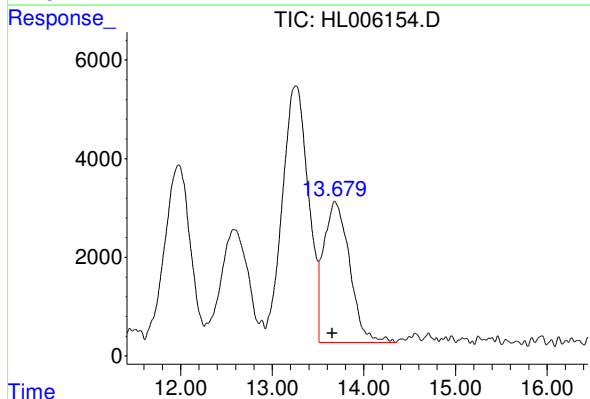

#13 2,6-Dinitrotoluene

R.T.: 13.685 min
Delta R.T.: 0.032 min
Response: 564130
Conc: 52.01 ug/L

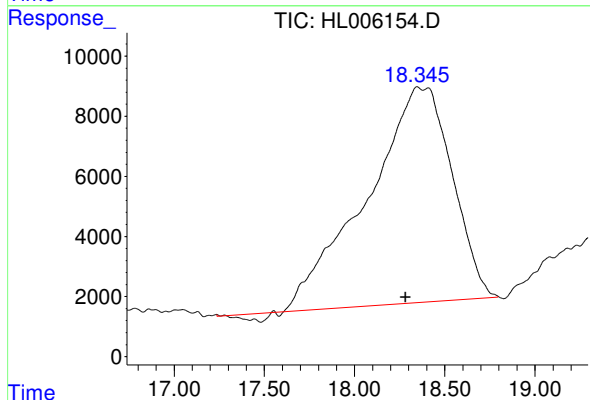

#14 2-Nitrotoluene

R.T.: 18.353 min
Delta R.T.: 0.069 min
Response: 2345002
Conc: 86.83 ug/L