

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL031715\
 Data File : HL006156.D
 Signal(s) : vwd1A.ch
 Acq On : 17-Mar-2015, 19:29
 Operator : TP/IZ
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 LOQ-WATER2015-02

Integration File: AUTOINT1.E
 Quant Time: Mar 18 10:58:13 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL031615.M
 Quant Title :
 QLast Update : Tue Mar 17 09:09:29 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	1.513	3139536	535.917 ug/L
8) T Tetryl	9.800	5366160	532.991 ug/L
9) T 2,4,6-Trinitrotoluene	10.224	7648057	527.902 ug/L
10) T 2-Amino-4,6-dinitroto...	11.873	8615017	530.733 ug/L
11) T 4-Amino-2,6-dinitroto...	12.486	5386603	538.984 ug/L
12) T 2,4-Dinitrotoluene	13.143	11112174	530.932 ug/L
13) T 2,6-Dinitrotoluene	13.587	5917654	545.530 ug/L
14) T 2-Nitrotoluene	18.331	13559011	502.088 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL031715\
Data File : HL006156.D
Signal(s) : vwd1A.ch
Acq On : 17-Mar-2015, 19:29
Operator : TP/IZ
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
LOQ-WATER2015-02

Integration File: AUTOINT1.E
Quant Time: Mar 18 10:58:13 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL031615.M
Quant Title :
QLast Update : Tue Mar 17 09:09:29 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

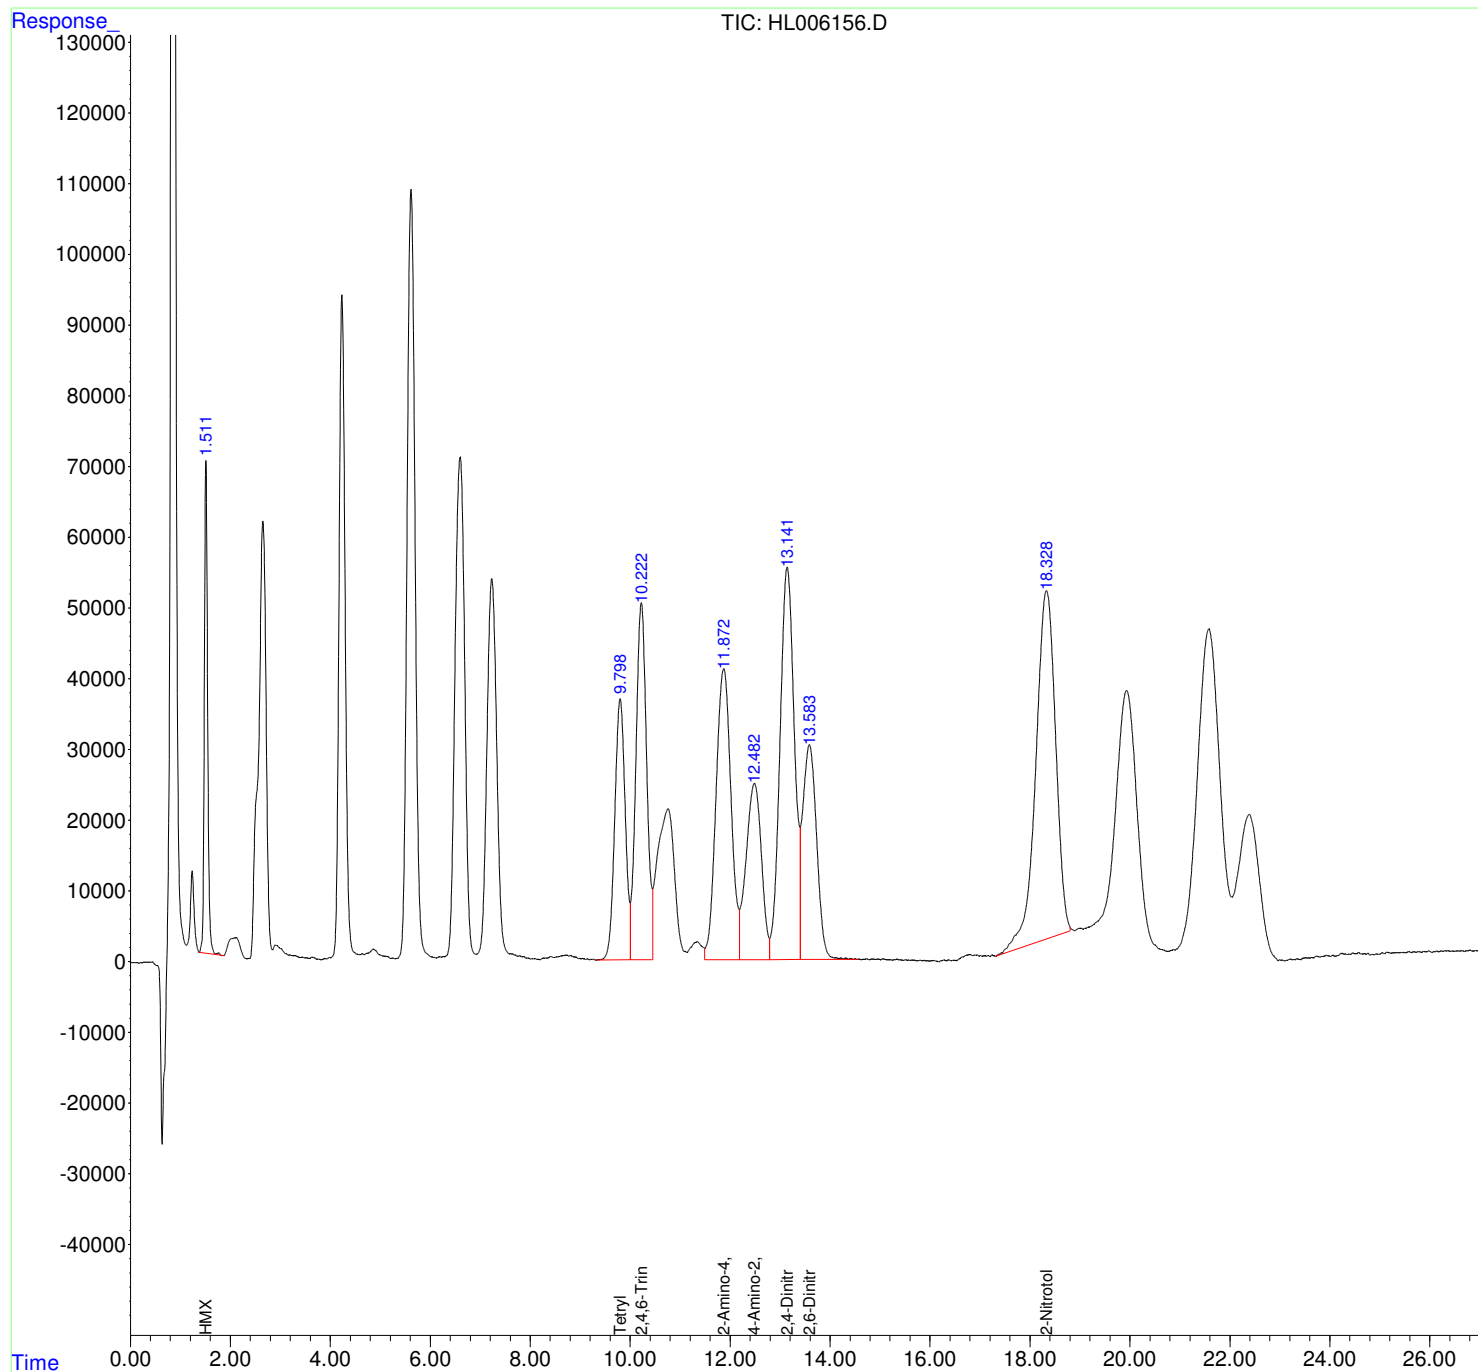


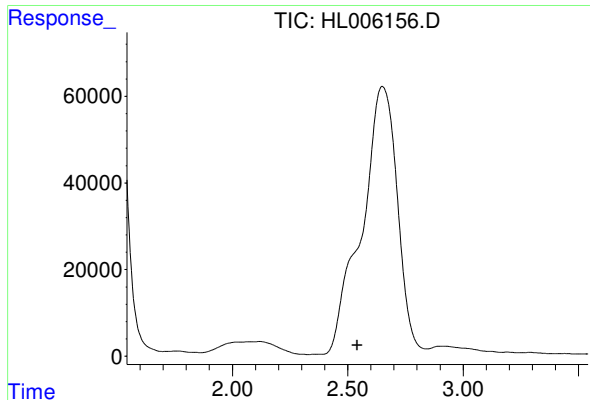

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.541 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
LOQ-WATER2015-02

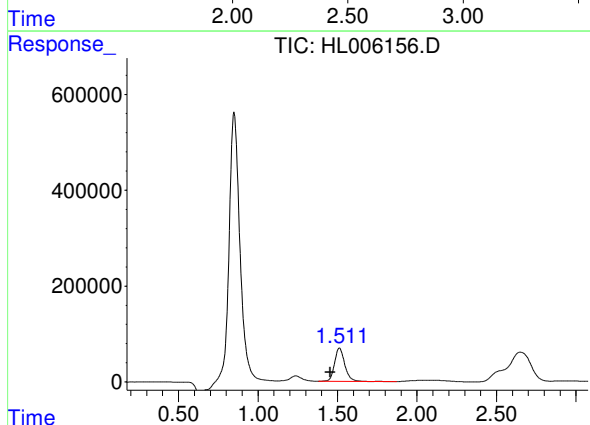


#2 HMX

R.T.: 1.513 min
Delta R.T.: 0.060 min
Response: 3139536
Conc: 535.92 ug/L

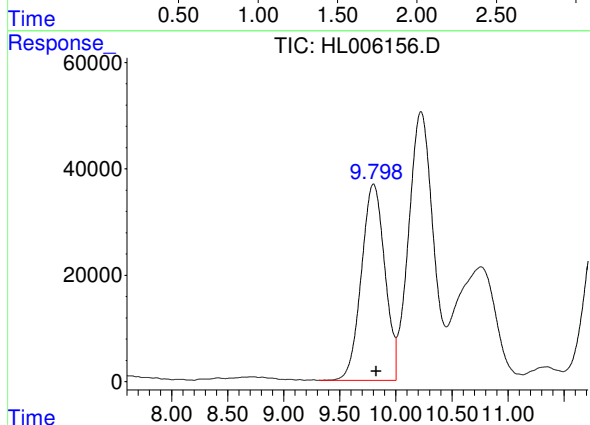


#8 Tetryl

R.T.: 9.800 min
Delta R.T.: -0.026 min
Response: 5366160
Conc: 532.99 ug/L

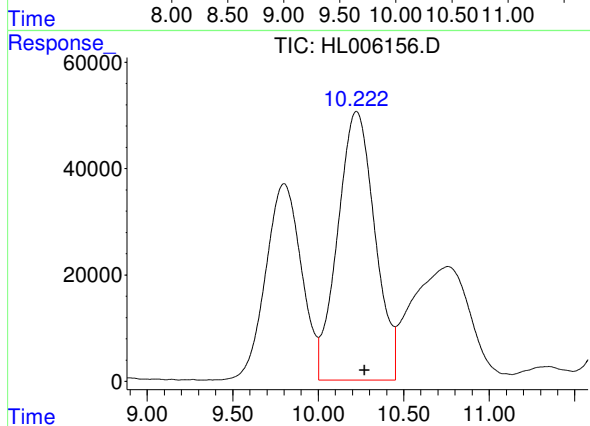

#9 2,4,6-Trinitrotoluene


R.T.: 10.224 min
Delta R.T.: -0.045 min
Response: 7648057
Conc: 527.90 ug/L

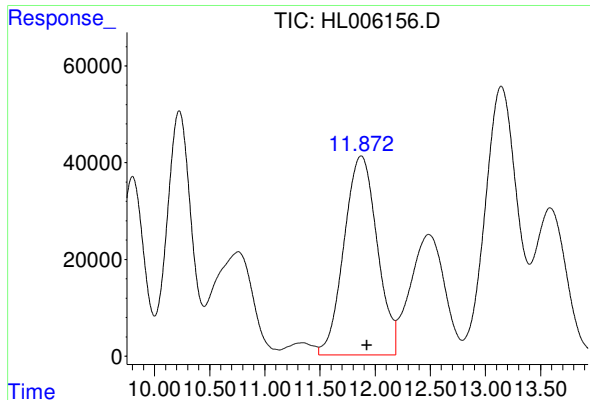

#10 2-Amino-4,6-dinitrotoluene


R.T.: 11.873 min
Delta R.T.: -0.052 min
Response: 8615017
Conc: 530.73 ug/L

Instrument :
HPLC_L
ClientSampleId :
LOQ-WATER2015-02

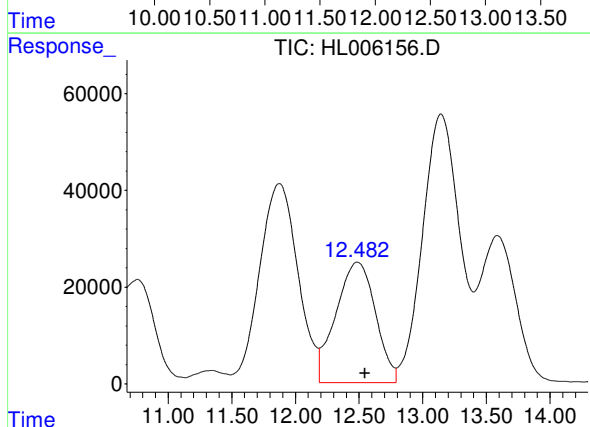


#11 4-Amino-2,6-dinitrotoluene

R.T.: 12.486 min
Delta R.T.: -0.058 min
Response: 5386603
Conc: 538.98 ug/L

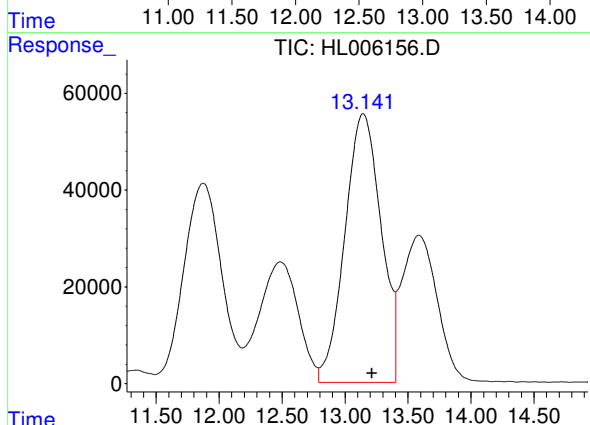


#12 2,4-Dinitrotoluene

R.T.: 13.143 min
Delta R.T.: -0.070 min
Response: 11112174
Conc: 530.93 ug/L

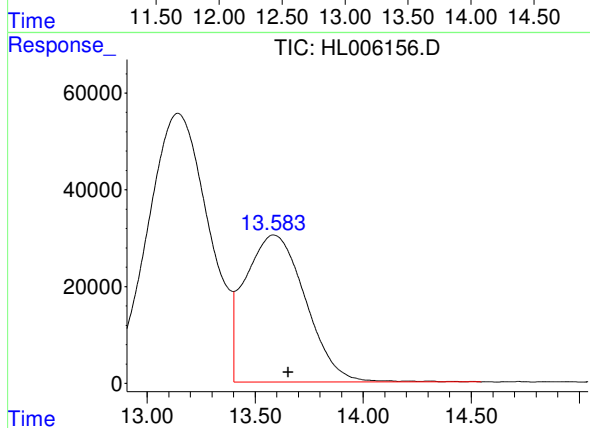

#13 2,6-Dinitrotoluene

R.T.: 13.587 min
Delta R.T.: -0.066 min
Response: 5917654
Conc: 545.53 ug/L

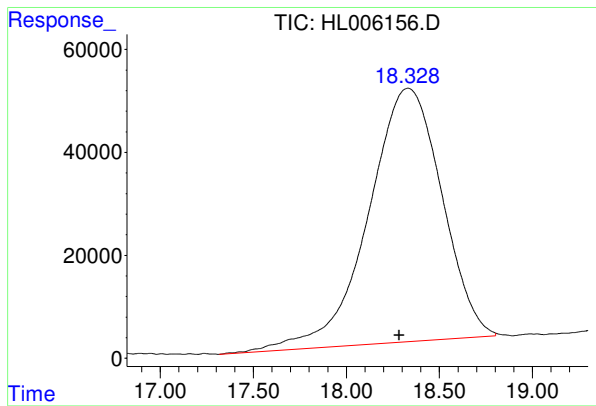

#14 2-Nitrotoluene

R.T.: 18.331 min
Delta R.T.: 0.047 min
Response: 13559011
Conc: 502.09 ug/L

Instrument :
HPLC_L
ClientSampleId :
LOQ-WATER2015-02