

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL031715\
Data File : HL006163.D
Signal(s) : vwd1A.ch
Acq On : 17-Mar-2015, 21:06
Operator : TP/IZ
Sample : G1001-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
LOQ-WATER2015-02

Integration File: AUTOINT1.E
Quant Time: Mar 18 13:53:12 2015
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL0313NG.M
Quant Title :
QLast Update : Sat Mar 14 06:54:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL031715\
Data File : HL006163.D
Signal(s) : vwd1A.ch
Acq On : 17-Mar-2015, 21:06
Operator : TP/IZ
Sample : G1001-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
LOQ-WATER2015-02

Integration File: AUTOINT1.E
Quant Time: Mar 18 13:53:12 2015
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL0313NG.M
Quant Title :
QLast Update : Sat Mar 14 06:54:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

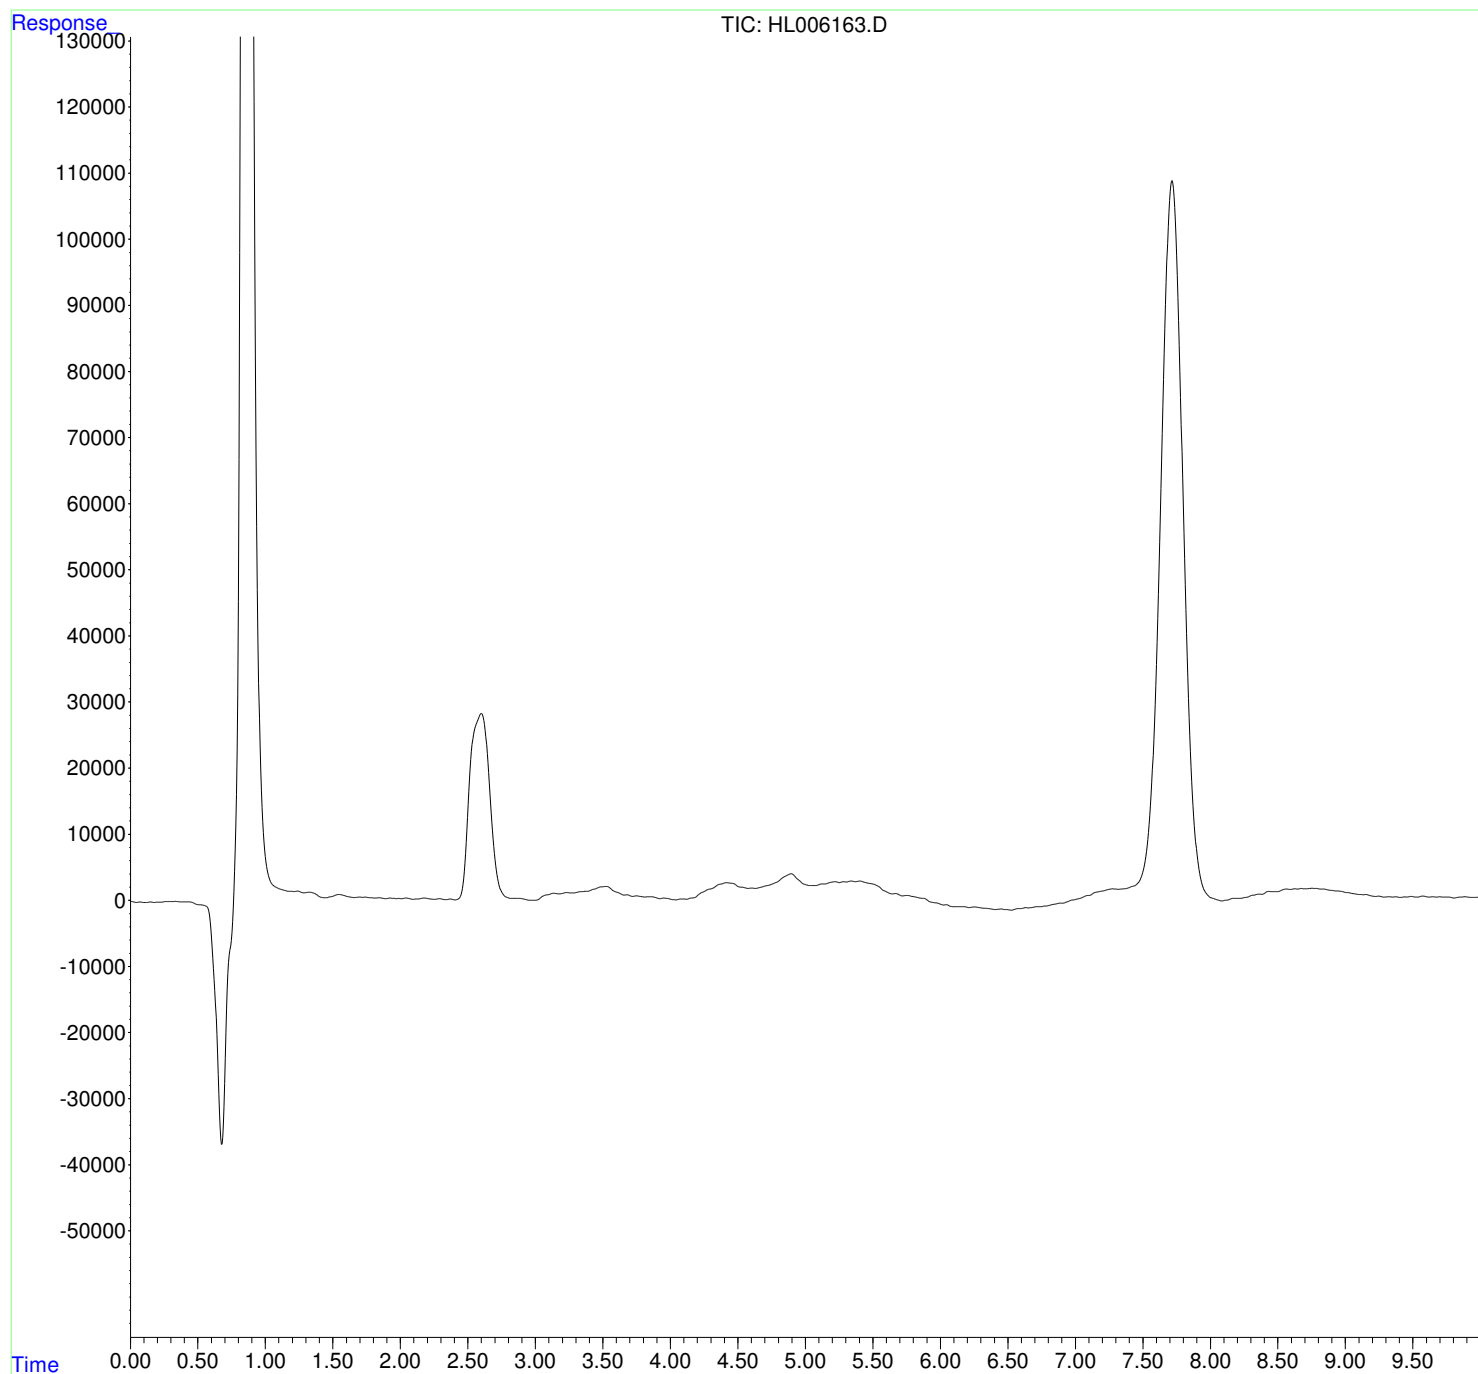

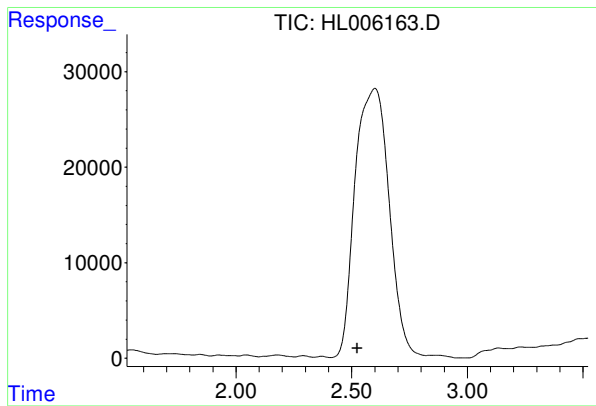

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 2.523 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
LOQ-WATER2015-02