

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL032515\
Data File : HL006181.D
Signal(s) : vwd1A.ch
Acq On : 25-Mar-2015, 20:29
Operator : TP/IZ
Sample : G1614-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

Integration File: AUTOINT1.E
Quant Time: Mar 27 08:46:31 2015
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL0313NG.M
Quant Title :
QLast Update : Fri Mar 27 08:41:14 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 u1
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.743	2968686	0.497 ng/u1
Target Compounds			
2) T Nitroglycerin	8.201	3753041	0.303 ng/u1

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL032515\
Data File : HL006181.D
Signal(s) : vwd1A.ch
Acq On : 25-Mar-2015, 20:29
Operator : TP/IZ
Sample : G1614-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

Integration File: AUTOINT1.E
Quant Time: Mar 27 08:46:31 2015
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL0313NG.M
Quant Title :
QLast Update : Fri Mar 27 08:41:14 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

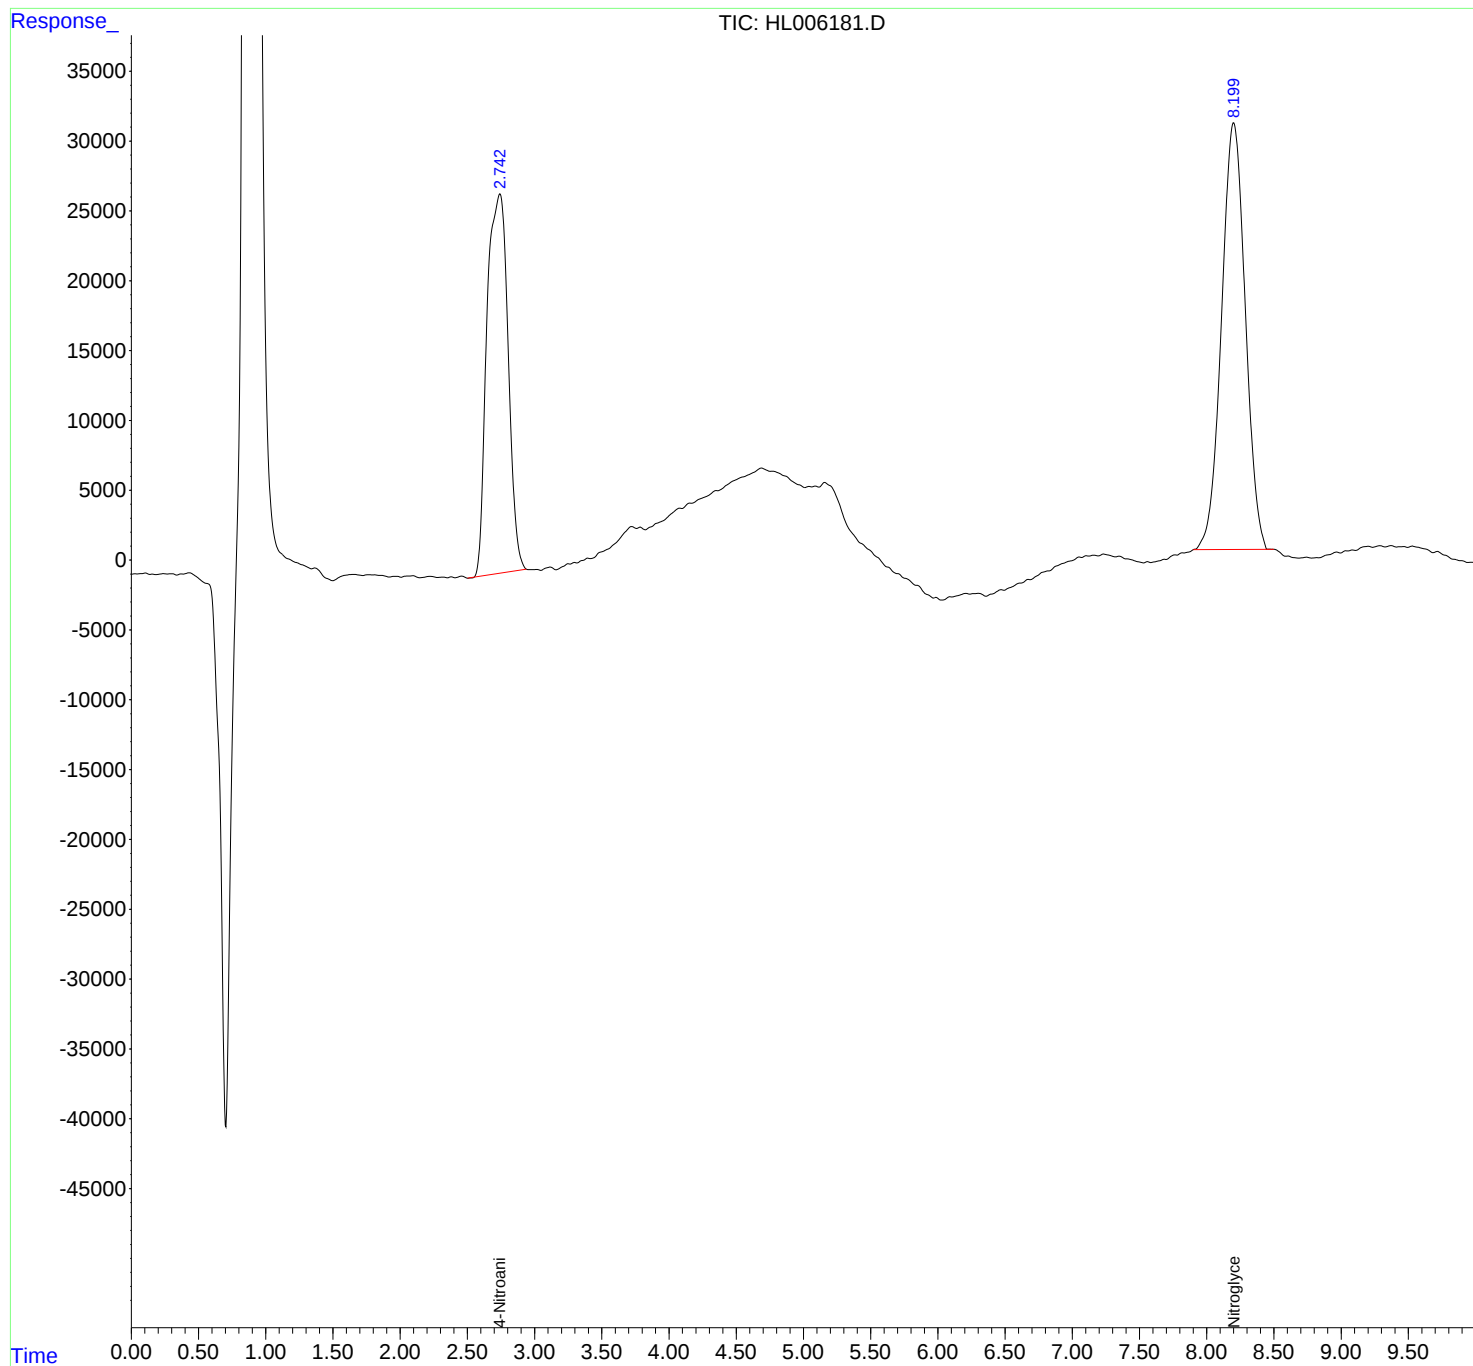


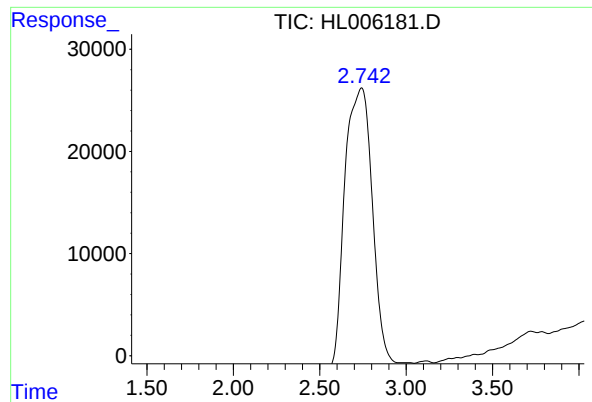

#1 4-Nitroaniline

R.T.: 2.743 min
Delta R.T.: -0.013 min
Response: 2968686
Conc: 0.50 ng/ul

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

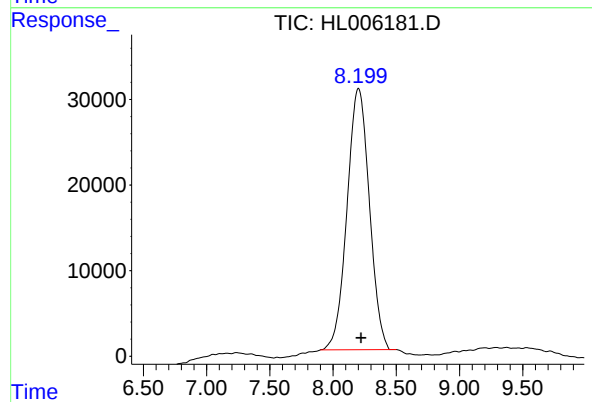

#2 Nitroglycerin

R.T.: 8.201 min
Delta R.T.: -0.019 min
Response: 3753041
Conc: 0.30 ng/ul