

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL040315\
Data File : HL006187.D
Signal(s) : vwd1A.ch
Acq On : 03-Apr-2015, 19:02
Operator : TP/IZ
Sample : PB82292BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
PB82292BL

Integration File: AUTOINT1.E
Quant Time: Apr 06 08:41:37 2015
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL031615.M
Quant Title :
QLast Update : Mon Apr 06 08:22:23 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10) T	2-Amino-4,6-dinitroto...	10.498	1042347	64.214 ug/L
17) T	PETN	23.950	726241	60.980 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL040315\
Data File : HL006187.D
Signal(s) : vwd1A.ch
Acq On : 03-Apr-2015, 19:02
Operator : TP/IZ
Sample : PB82292BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
PB82292BL

Integration File: AUTOINT1.E
Quant Time: Apr 06 08:41:37 2015
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL031615.M
Quant Title :
QLast Update : Mon Apr 06 08:22:23 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

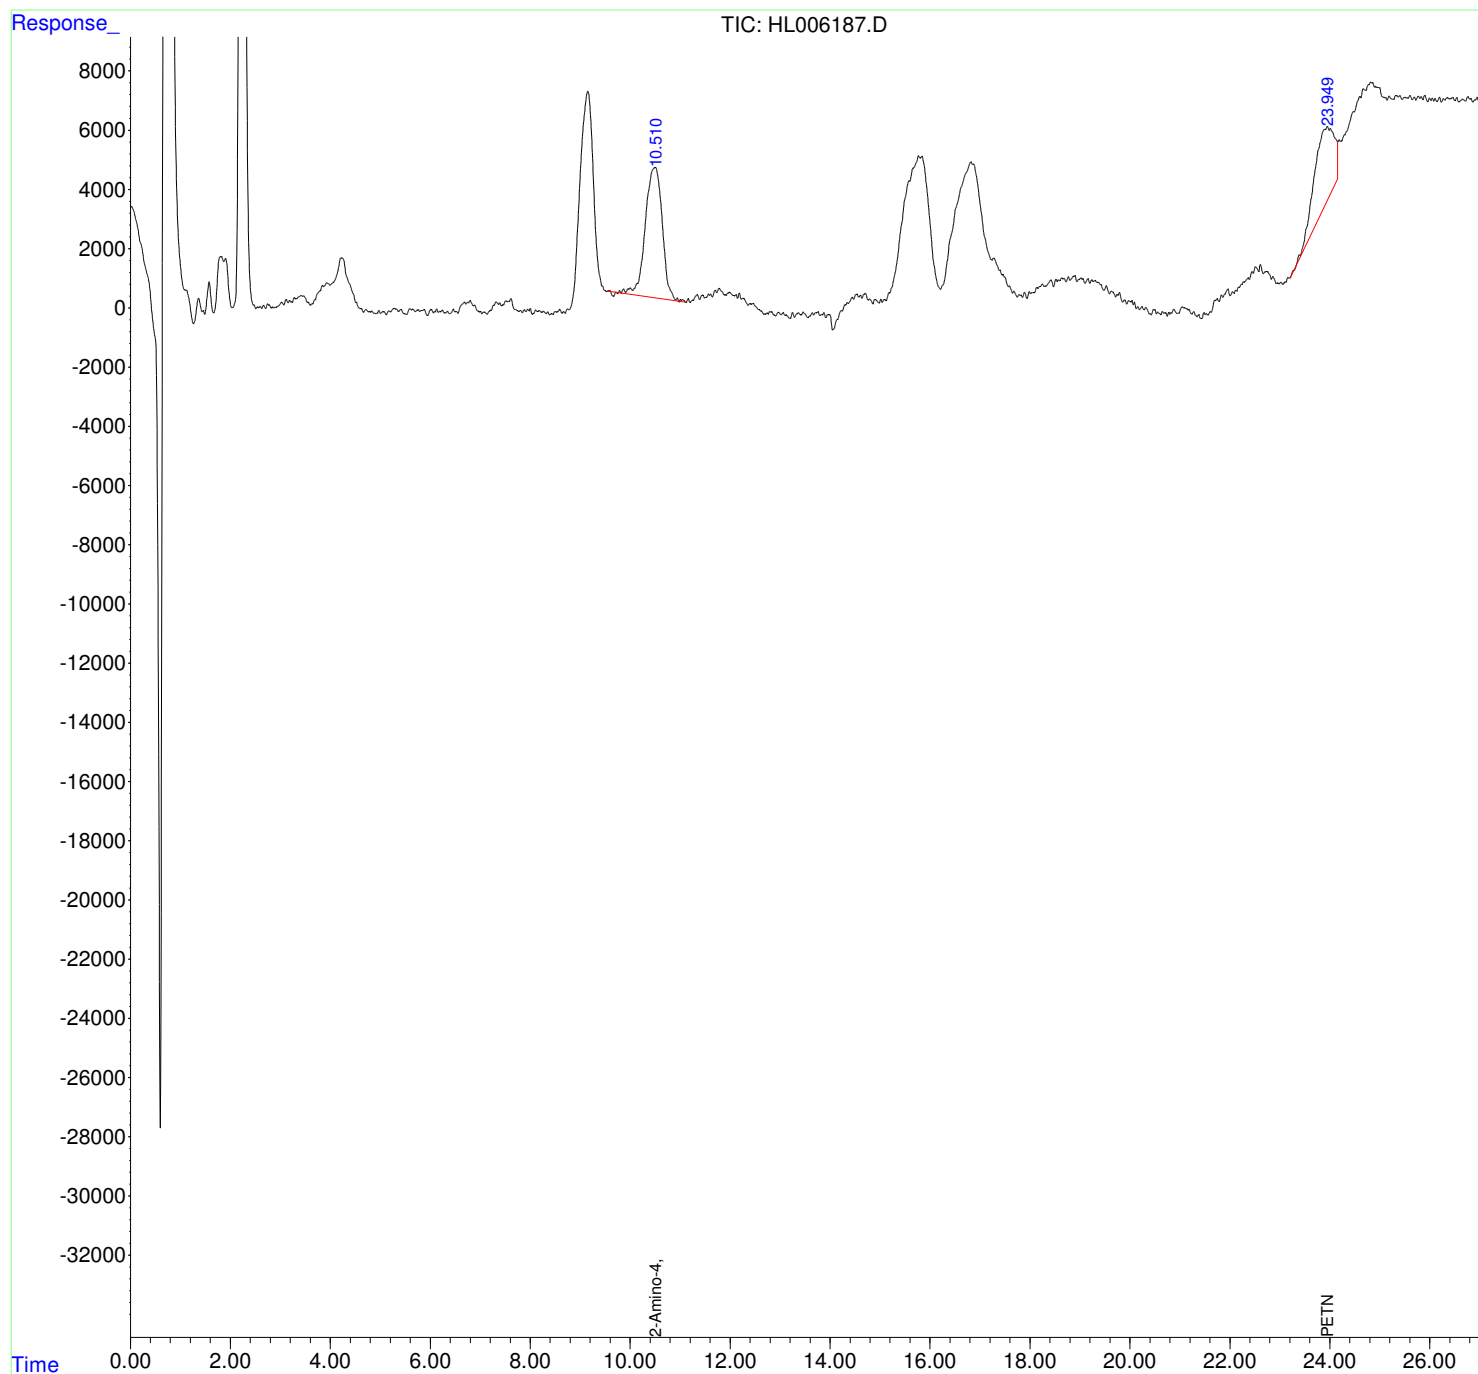


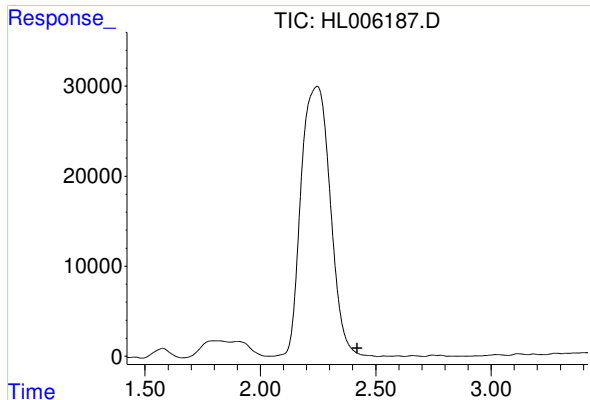

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.420 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
PB82292BL

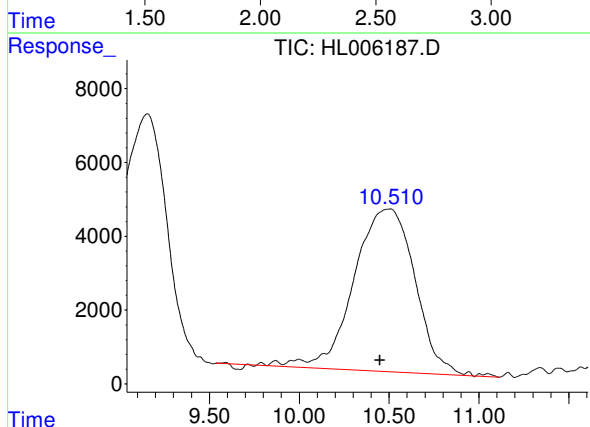

#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.498 min
Delta R.T.: 0.051 min
Response: 1042347
Conc: 64.21 ug/L

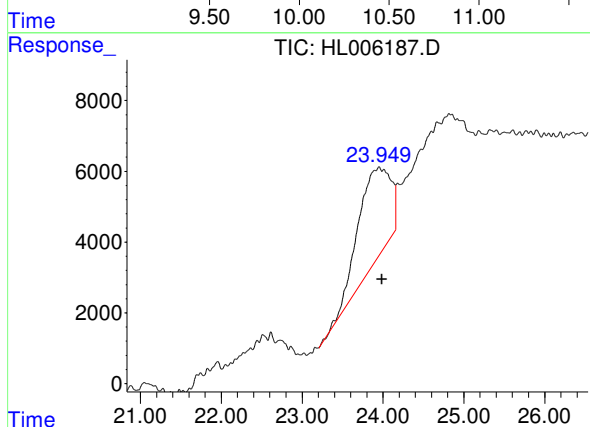

#17 PETN

R.T.: 23.950 min
Delta R.T.: -0.038 min
Response: 726241
Conc: 60.98 ug/L