

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL040315\
Data File : HL006188.D
Signal(s) : vwd1A.ch
Acq On : 03-Apr-2015, 19:31
Operator : TP/IZ
Sample : G1614-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

Integration File: AUTOINT1.E
Quant Time: Apr 06 08:41:41 2015
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL031615.M
Quant Title :
QLast Update : Mon Apr 06 08:22:23 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	1.331	361900	61.776 ug/L
9) T 2,4,6-Trinitrotoluene	9.135	736244	50.819 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL040315\
Data File : HL006188.D
Signal(s) : vwd1A.ch
Acq On : 03-Apr-2015, 19:31
Operator : TP/IZ
Sample : G1614-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

Integration File: AUTOINT1.E
Quant Time: Apr 06 08:41:41 2015
Quant Method : Z:\HPCHEM1\HPLC_L\methods\HL031615.M
Quant Title :
QLast Update : Mon Apr 06 08:22:23 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

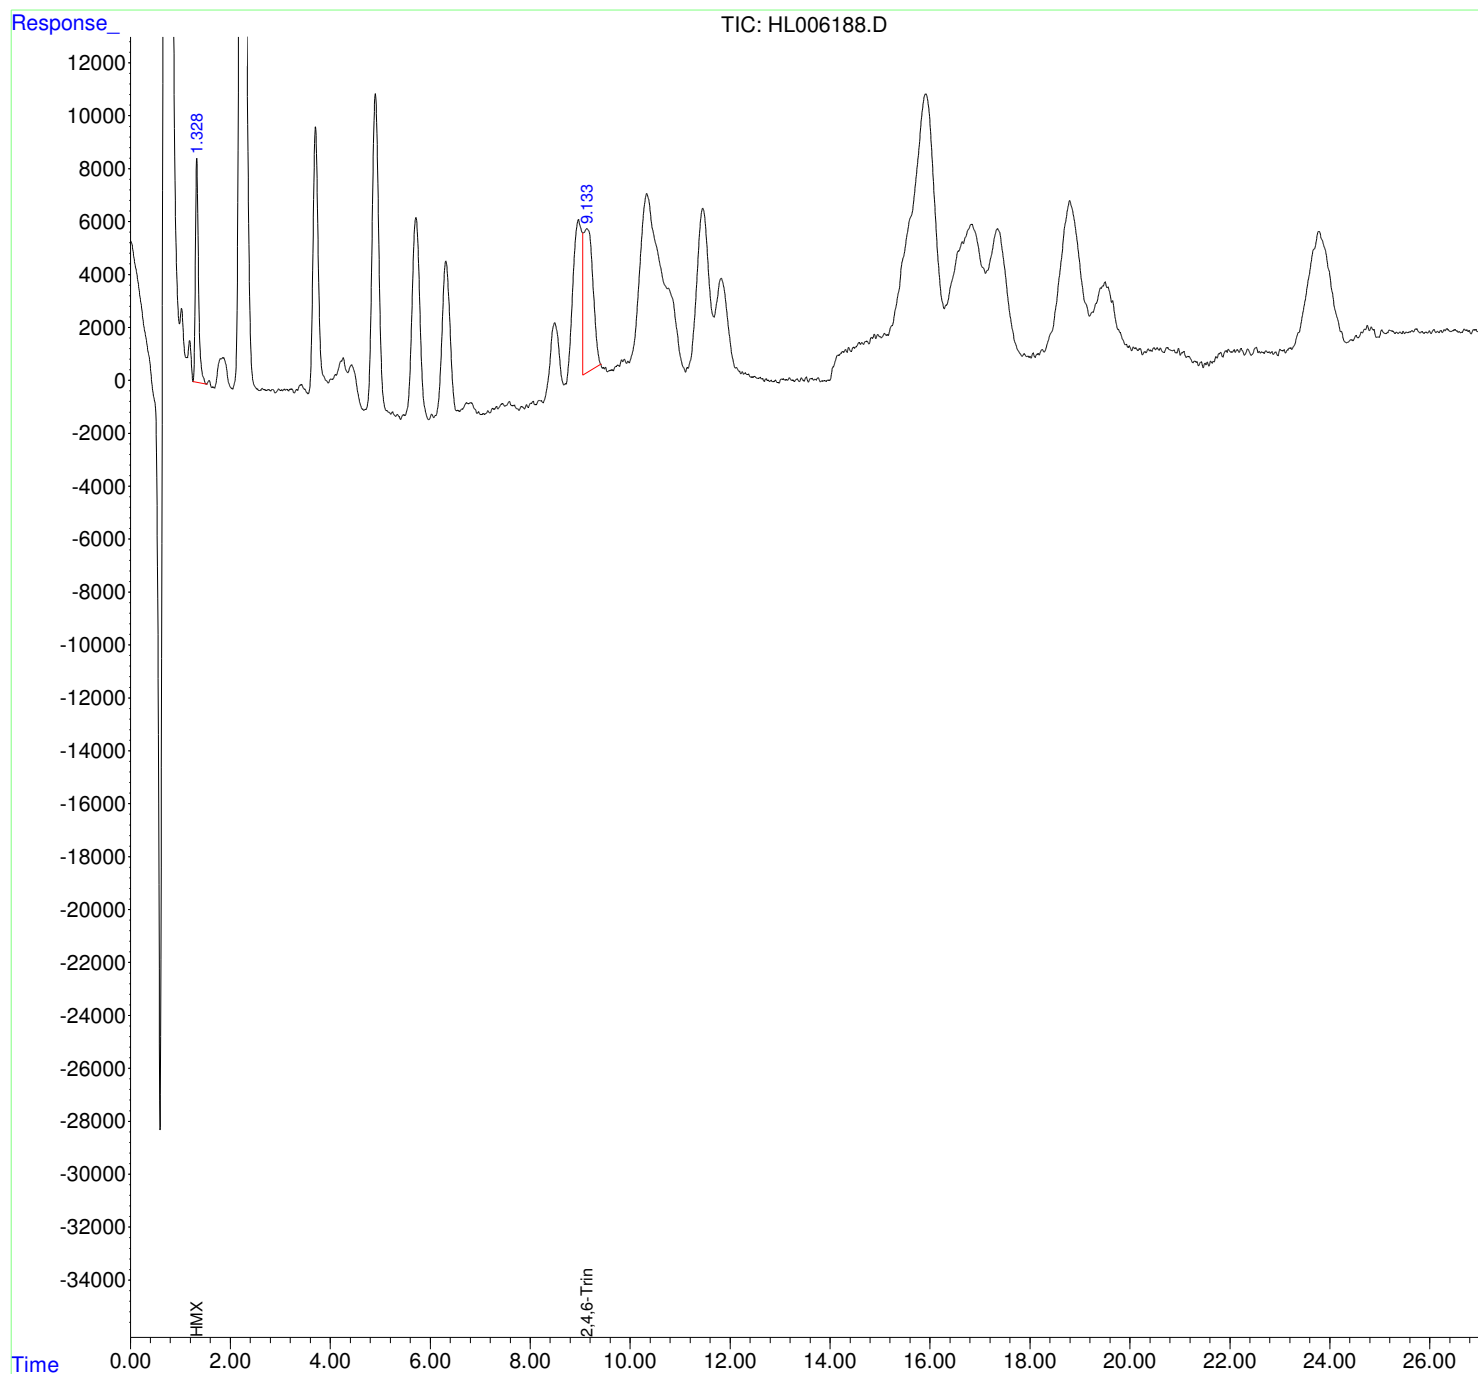


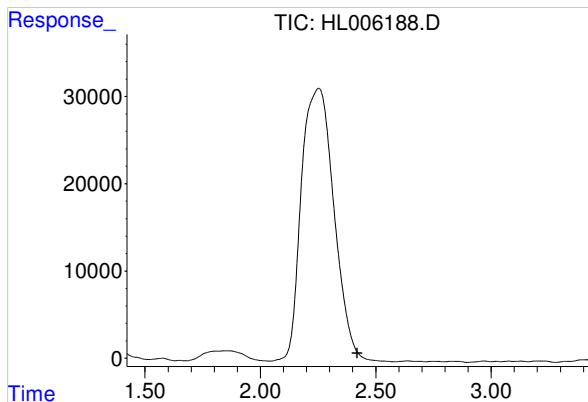

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.420 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
LOD-WATER2015-01

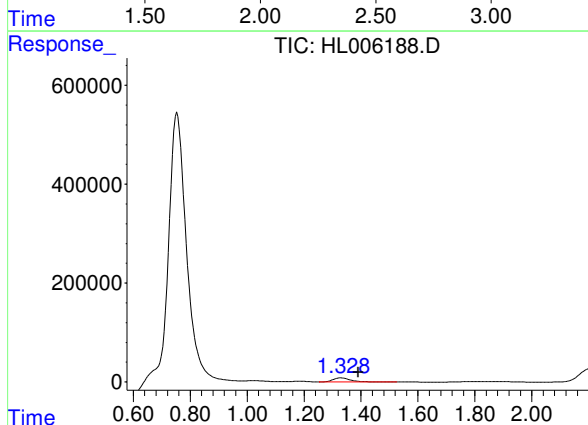

#2 HMX

R.T.: 1.331 min
Delta R.T.: -0.060 min
Response: 361900
Conc: 61.78 ug/L

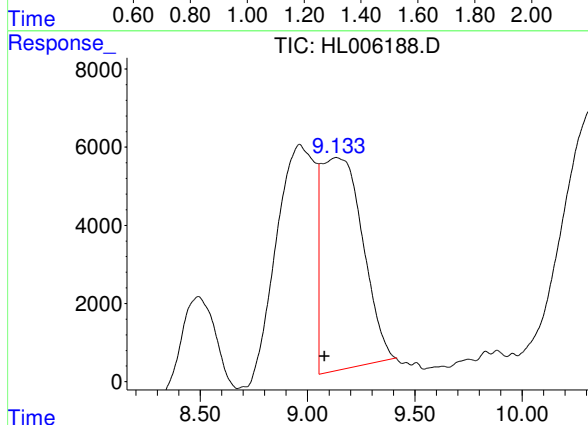

#9 2,4,6-Trinitrotoluene

R.T.: 9.135 min
Delta R.T.: 0.056 min
Response: 736244
Conc: 50.82 ug/L