

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL040315\  
 Data File : HL006190.D  
 Signal(s) : vwd1A.ch  
 Acq On : 03-Apr-2015, 20:27  
 Operator : TP/IZ  
 Sample : HSTDCCC0500  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 HPLC\_L  
 ClientSampleId :  
 HSTDCCC0500

Integration File: AUTOINT1.E  
 Quant Time: Apr 06 08:41:49 2015  
 Quant Method : Z:\HPCHEM1\HPLC\_L\methods\HL031615.M  
 Quant Title :  
 QLast Update : Mon Apr 06 08:22:23 2015  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 50 ul  
 Signal Phase : ZORBAX Extend-C18  
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 2) T HMX                    | 1.329  | 3392061  | 579.023 ug/L |
| 13) T 2,6-Dinitrotoluene    | 11.916 | 6414178  | 591.303 ug/L |
| 14) T 2-Nitrotoluene        | 16.102 | 14840206 | 549.530 ug/L |
| 15) T 4-Nitrotoluene        | 17.502 | 10707830 | 639.981 ug/L |
| 16) T 3-Nitrotoluene        | 18.940 | 15654215 | 562.455 ug/L |
| 17) T PETN                  | 23.926 | 1595342  | 133.955 ug/L |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL040315\  
Data File : HL006190.D  
Signal(s) : vwd1A.ch  
Acq On : 03-Apr-2015, 20:27  
Operator : TP/IZ  
Sample : HSTDCCC0500  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
HSTDCCC0500

Integration File: AUTOINT1.E  
Quant Time: Apr 06 08:41:49 2015  
Quant Method : Z:\HPCHEM1\HPLC\_L\methods\HL031615.M  
Quant Title :  
QLast Update : Mon Apr 06 08:22:23 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

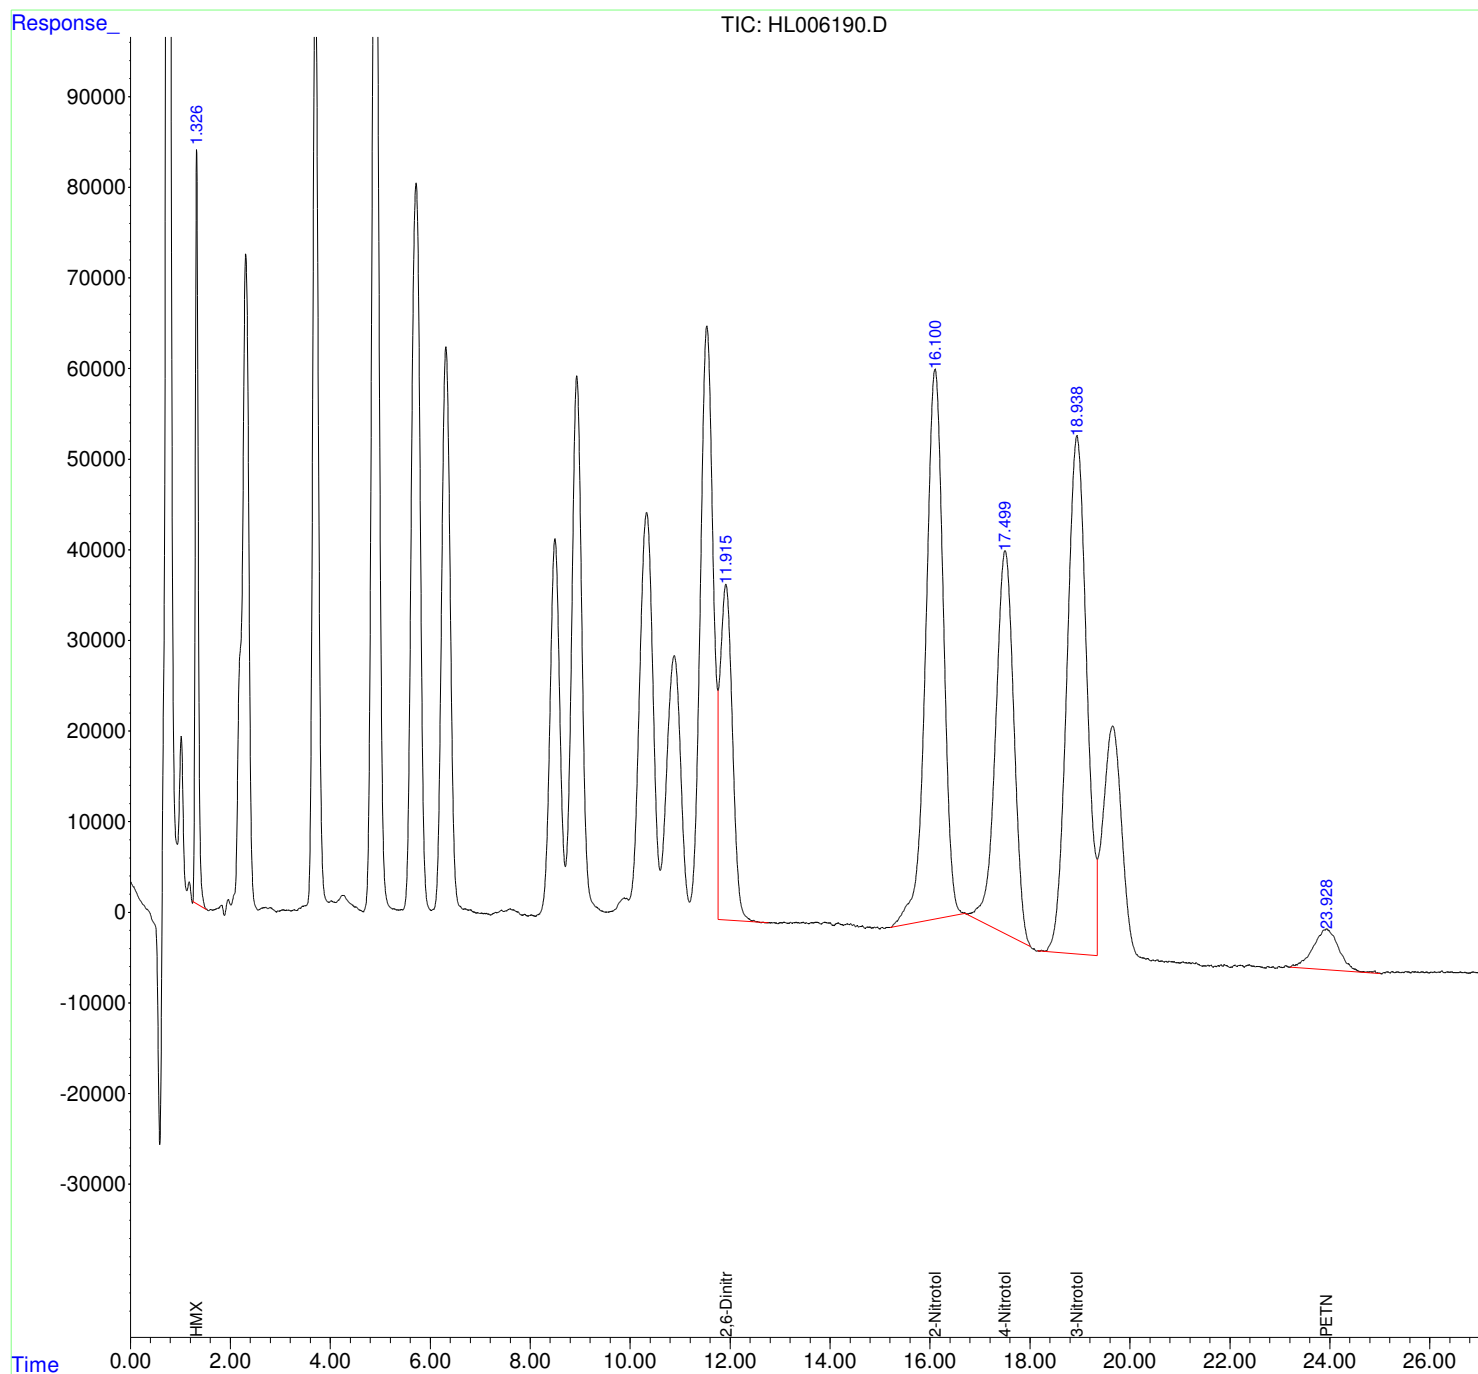


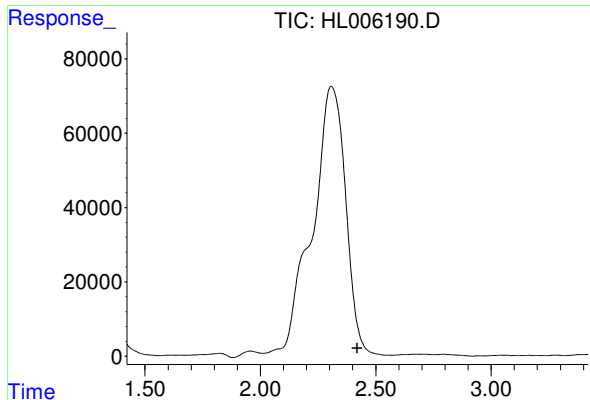

#1 4-Nitroaniline


R.T.: 0.000 min  
Exp R.T.: 2.420 min  
Response: 0  
Conc: N.D.

Instrument :  
HPLC\_L  
ClientSampleId :  
HSTDCCC0500

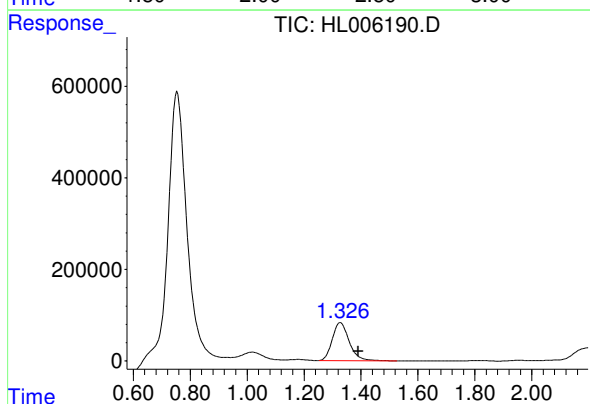


#2 HMX

R.T.: 1.329 min  
Delta R.T.: -0.062 min  
Response: 3392061  
Conc: 579.02 ug/L

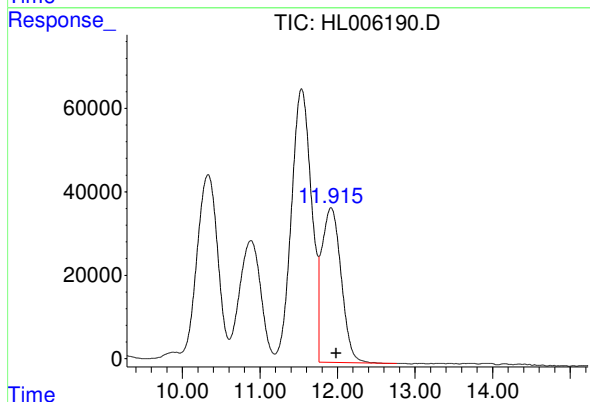


#13 2,6-Dinitrotoluene

R.T.: 11.916 min  
Delta R.T.: -0.069 min  
Response: 6414178  
Conc: 591.30 ug/L

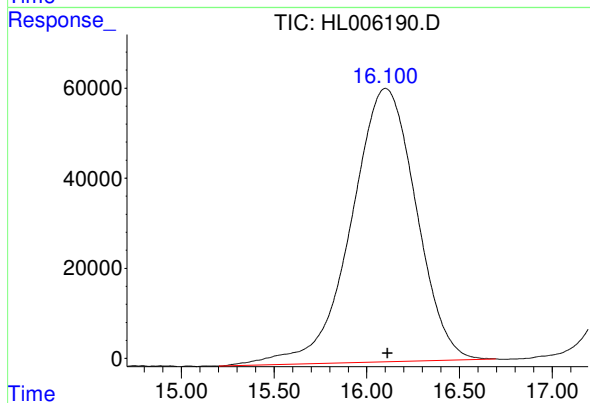

#14 2-Nitrotoluene


R.T.: 16.102 min  
Delta R.T.: -0.009 min  
Response: 14840206  
Conc: 549.53 ug/L

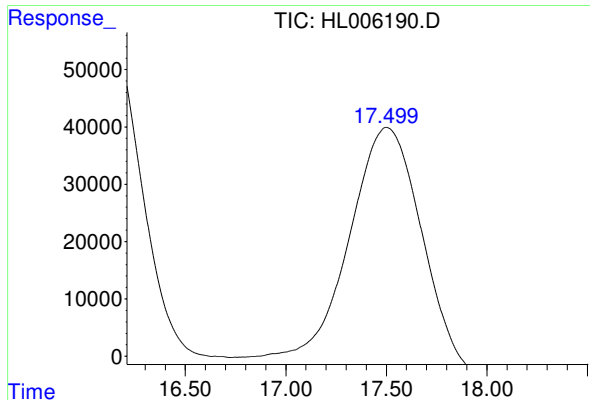

#15 4-Nitrotoluene


R.T.: 17.502 min  
Delta R.T.: -0.052 min  
Response: 10707830  
Conc: 639.98 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
HSTDCCC0500

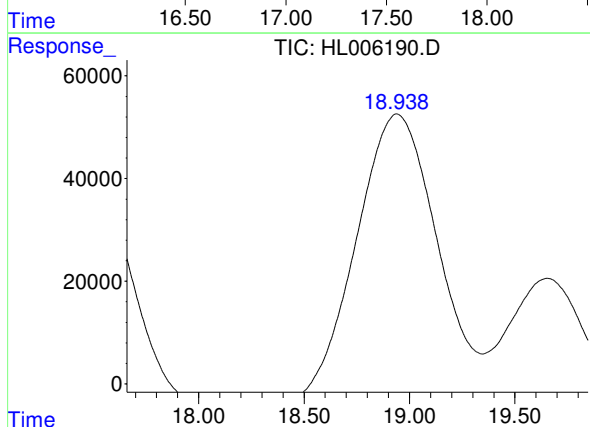

#16 3-Nitrotoluene

R.T.: 18.940 min  
Delta R.T.: -0.034 min  
Response: 15654215  
Conc: 562.45 ug/L

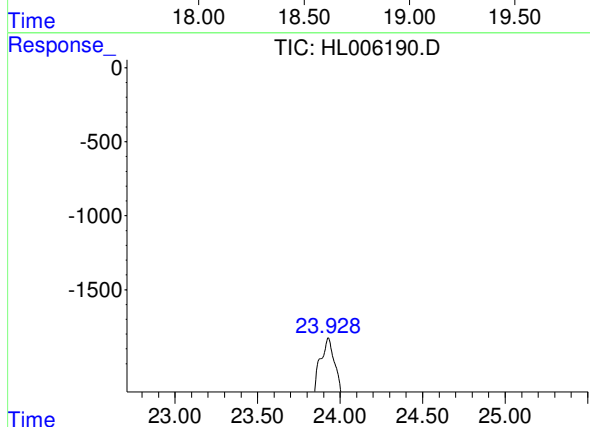

#17 PETN

R.T.: 23.926 min  
Delta R.T.: -0.062 min  
Response: 1595342  
Conc: 133.95 ug/L