

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002776.D Vial: 1
Acq On : 27-Apr-2012, 17:12 Operator: HLM
Sample : I.BLK Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 30 14:05 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Apr 30 14:06:15 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.41	272225	71.475 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 23.83%#

Target Compounds


5) T	Tetryl	6.44f	370586	40.950 ug/L
11) T	1,3-Dinitrobenzene	3.74	23188	1.291 ug/L
18) T	PETN	19.43f	1250112	126.246 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002776.D Vial: 1
 Acq On : 27-Apr-2012, 17:12 Operator: HLM
 Sample : I.BLK Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Apr 30 14:05 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Apr 30 14:06:15 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M


Volume Inj. :
 Signal Phase :
 Signal Info :

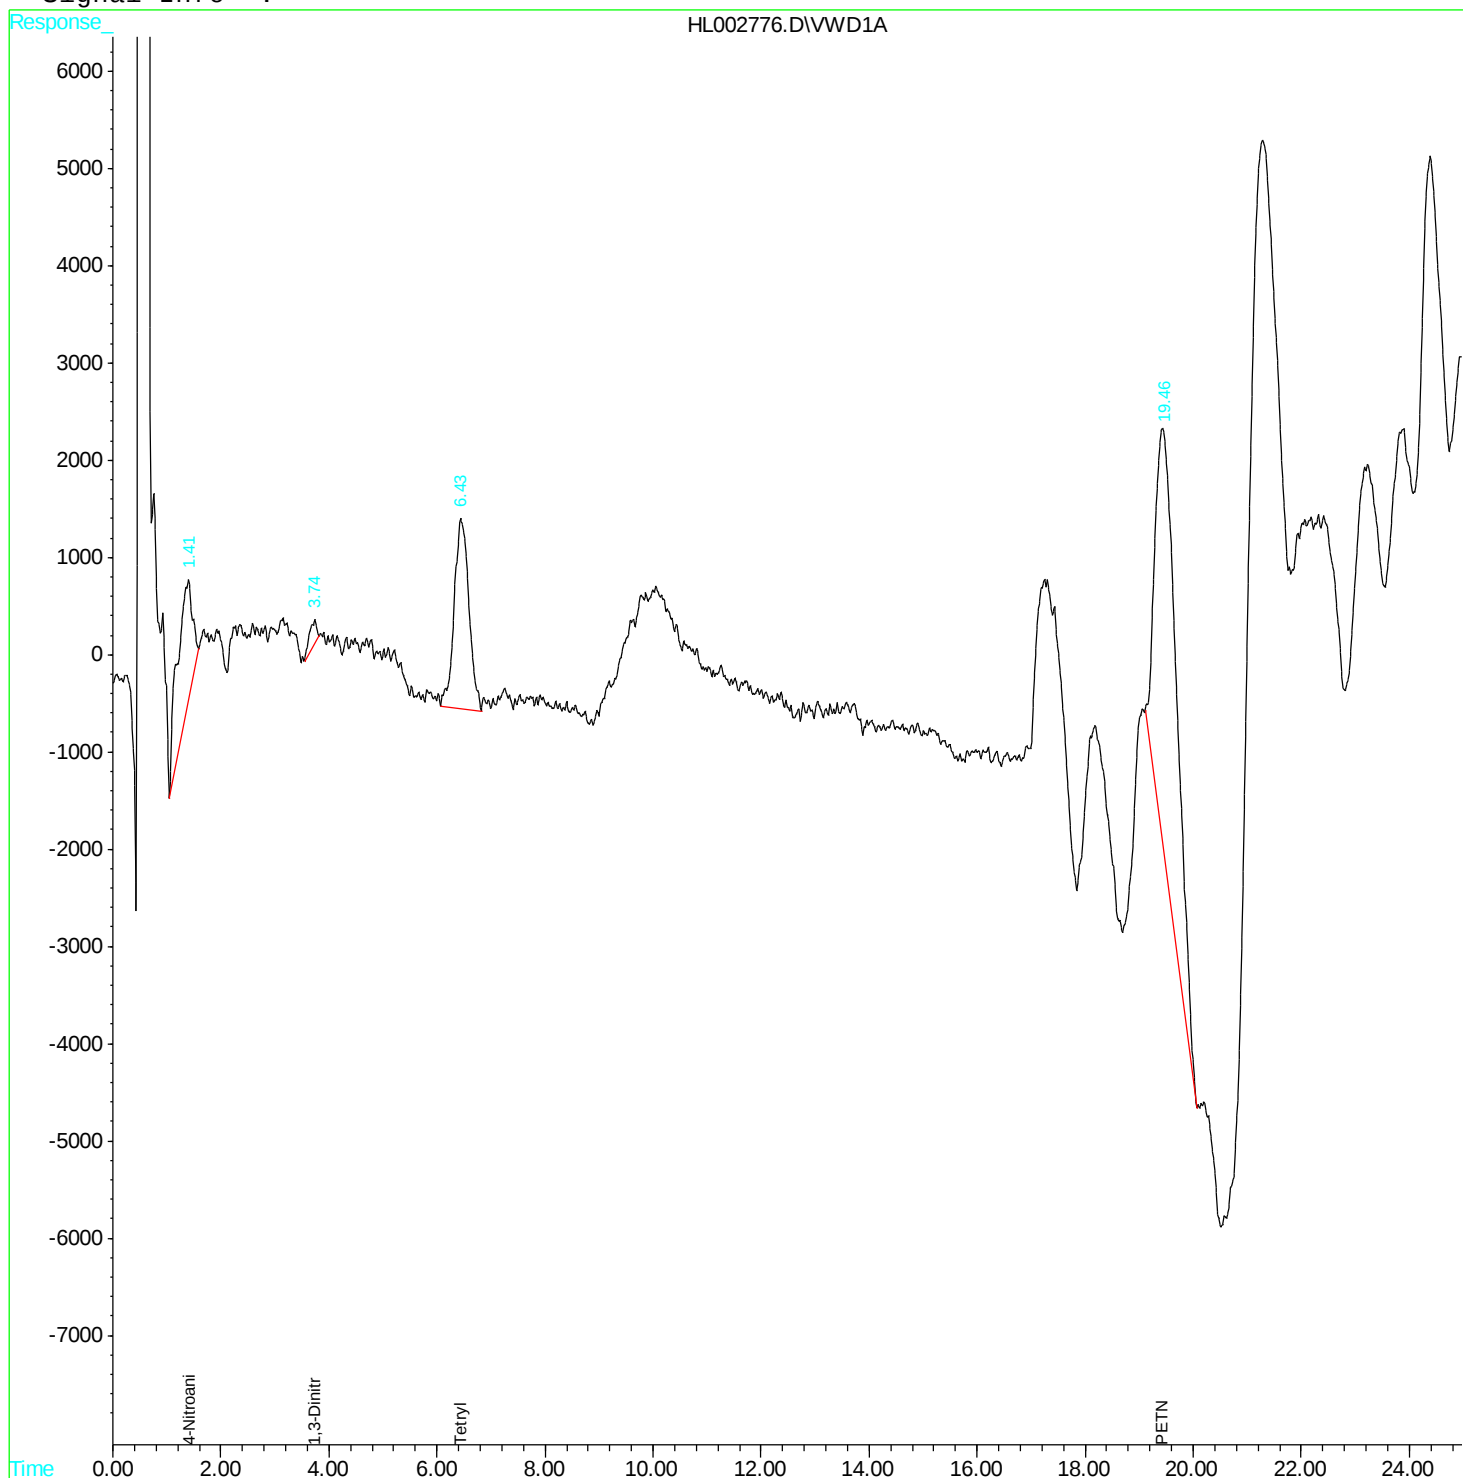

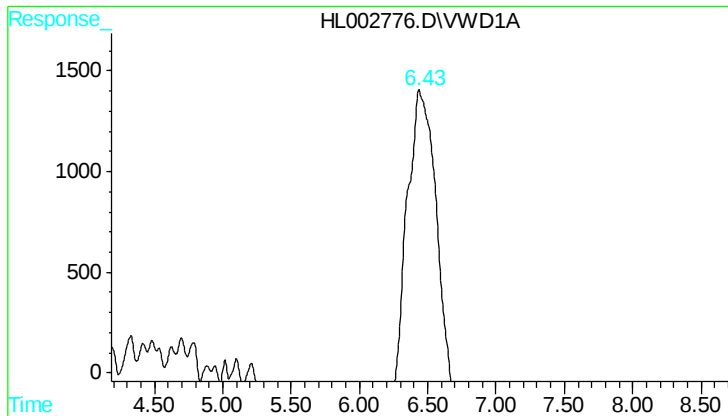


#5 Tetryl

R.T.: 6.436 min
Delta R.T.: 0.045 min
Response: 370586
Conc: 40.95 ug/L

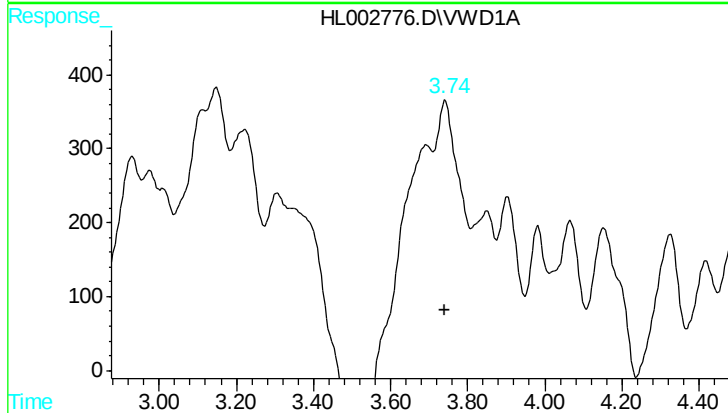

#11 1,3-Dinitrobenzene

R.T.: 3.743 min
Delta R.T.: 0.002 min
Response: 23188
Conc: 1.29 ug/L

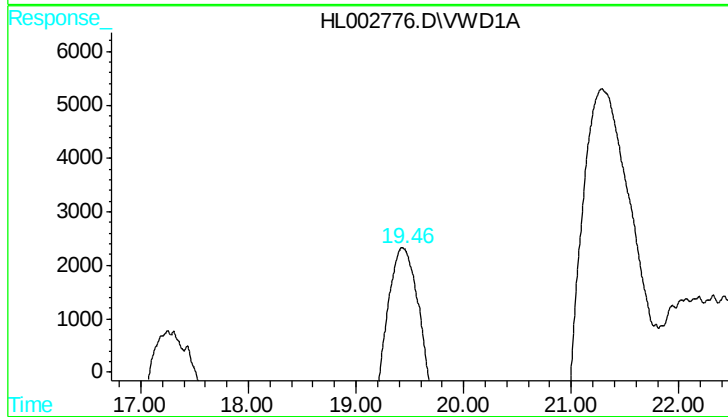

#18 PETN

R.T.: 19.430 min
Delta R.T.: 0.105 min
Response: 1250112
Conc: 126.25 ug/L