

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002787.D Vial: 46
Acq On : 27-Apr-2012, 22:38 Operator: HLM
Sample : D2332-06 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 30 14:06 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Apr 30 14:06:15 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.41	1685585	442.567 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 147.52%

Target Compounds


16) T	3,5-Dinitroaniline	4.13f	26884	1.601 ug/L
-------	--------------------	-------	-------	------------


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002787.D Vial: 46
 Acq On : 27-Apr-2012, 22:38 Operator: HLM
 Sample : D2332-06 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Apr 30 14:06 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Apr 30 14:06:15 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

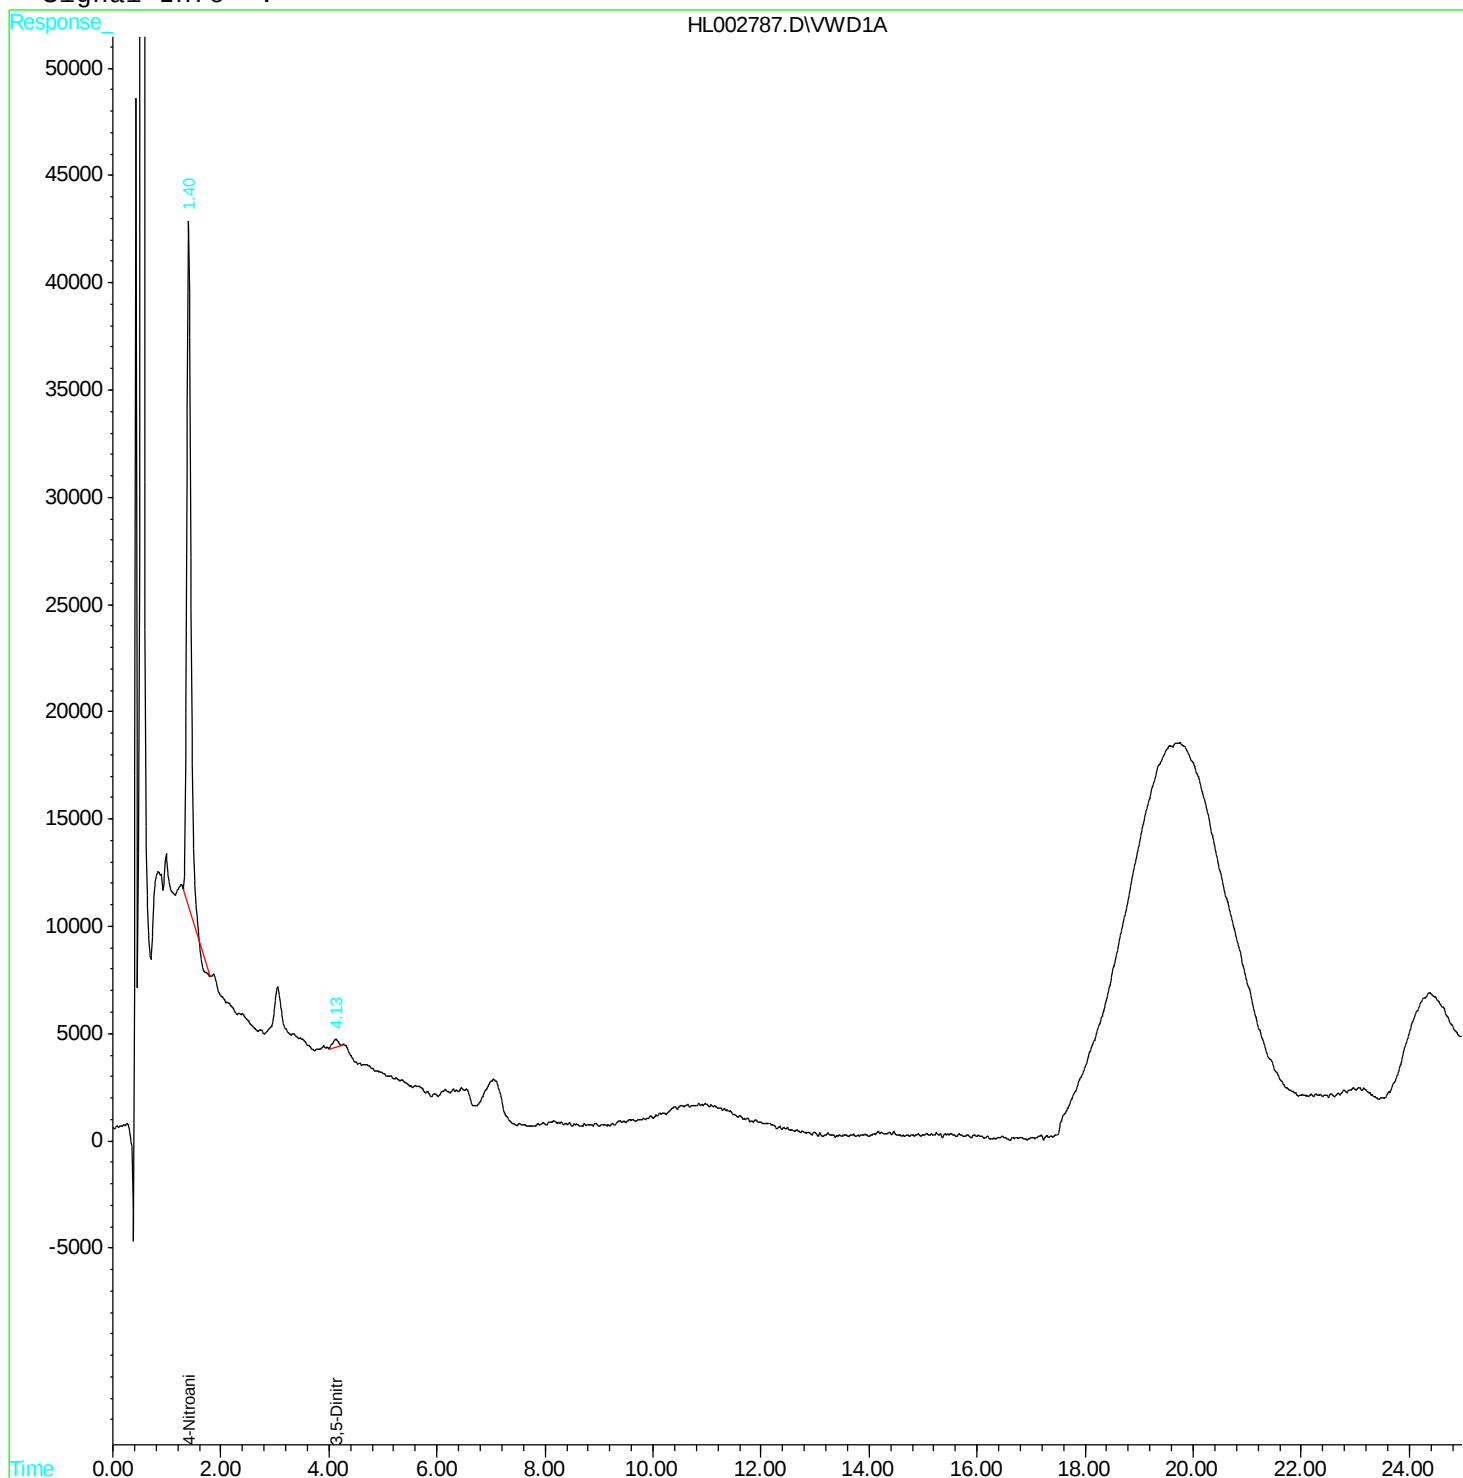

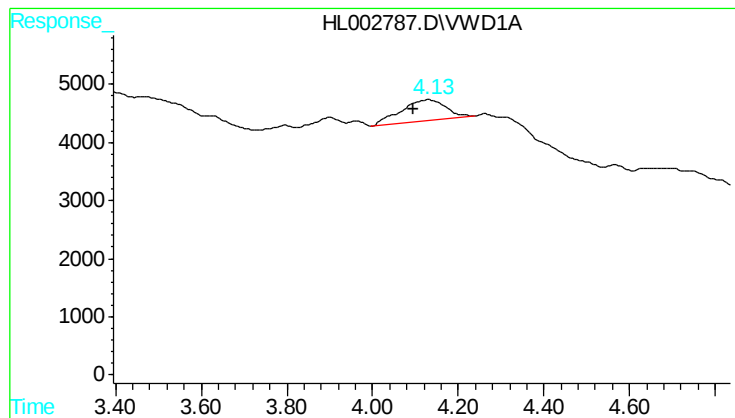

#16 3,5-Dinitroaniline

R.T.: 4.131 min
Delta R.T.: 0.034 min
Response: 26884
Conc: 1.60 ug/L