

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002789.D Vial: 48
Acq On : 27-Apr-2012, 23:32 Operator: HLM
Sample : D2332-07MS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 30 14:06 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Apr 30 14:06:15 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.40	1789262	469.788 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 156.60%#

Target Compounds


7) T	2-Amino-4,6-dinitrotoluene	7.34f	80111	7.143 ug/L
14) T	3-Nitrotoluene	14.17f	7976	1.116 ug/L
17) T	Nitroallycerin	6.29	395028	6918.192 ug/L
18) T	PETN	19.39	61127	6.173 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002789.D Vial: 48
 Acq On : 27-Apr-2012, 23:32 Operator: HLM
 Sample : D2332-07MS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Apr 30 14:06 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Apr 30 14:06:15 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M


Volume Inj. :
 Signal Phase :
 Signal Info :

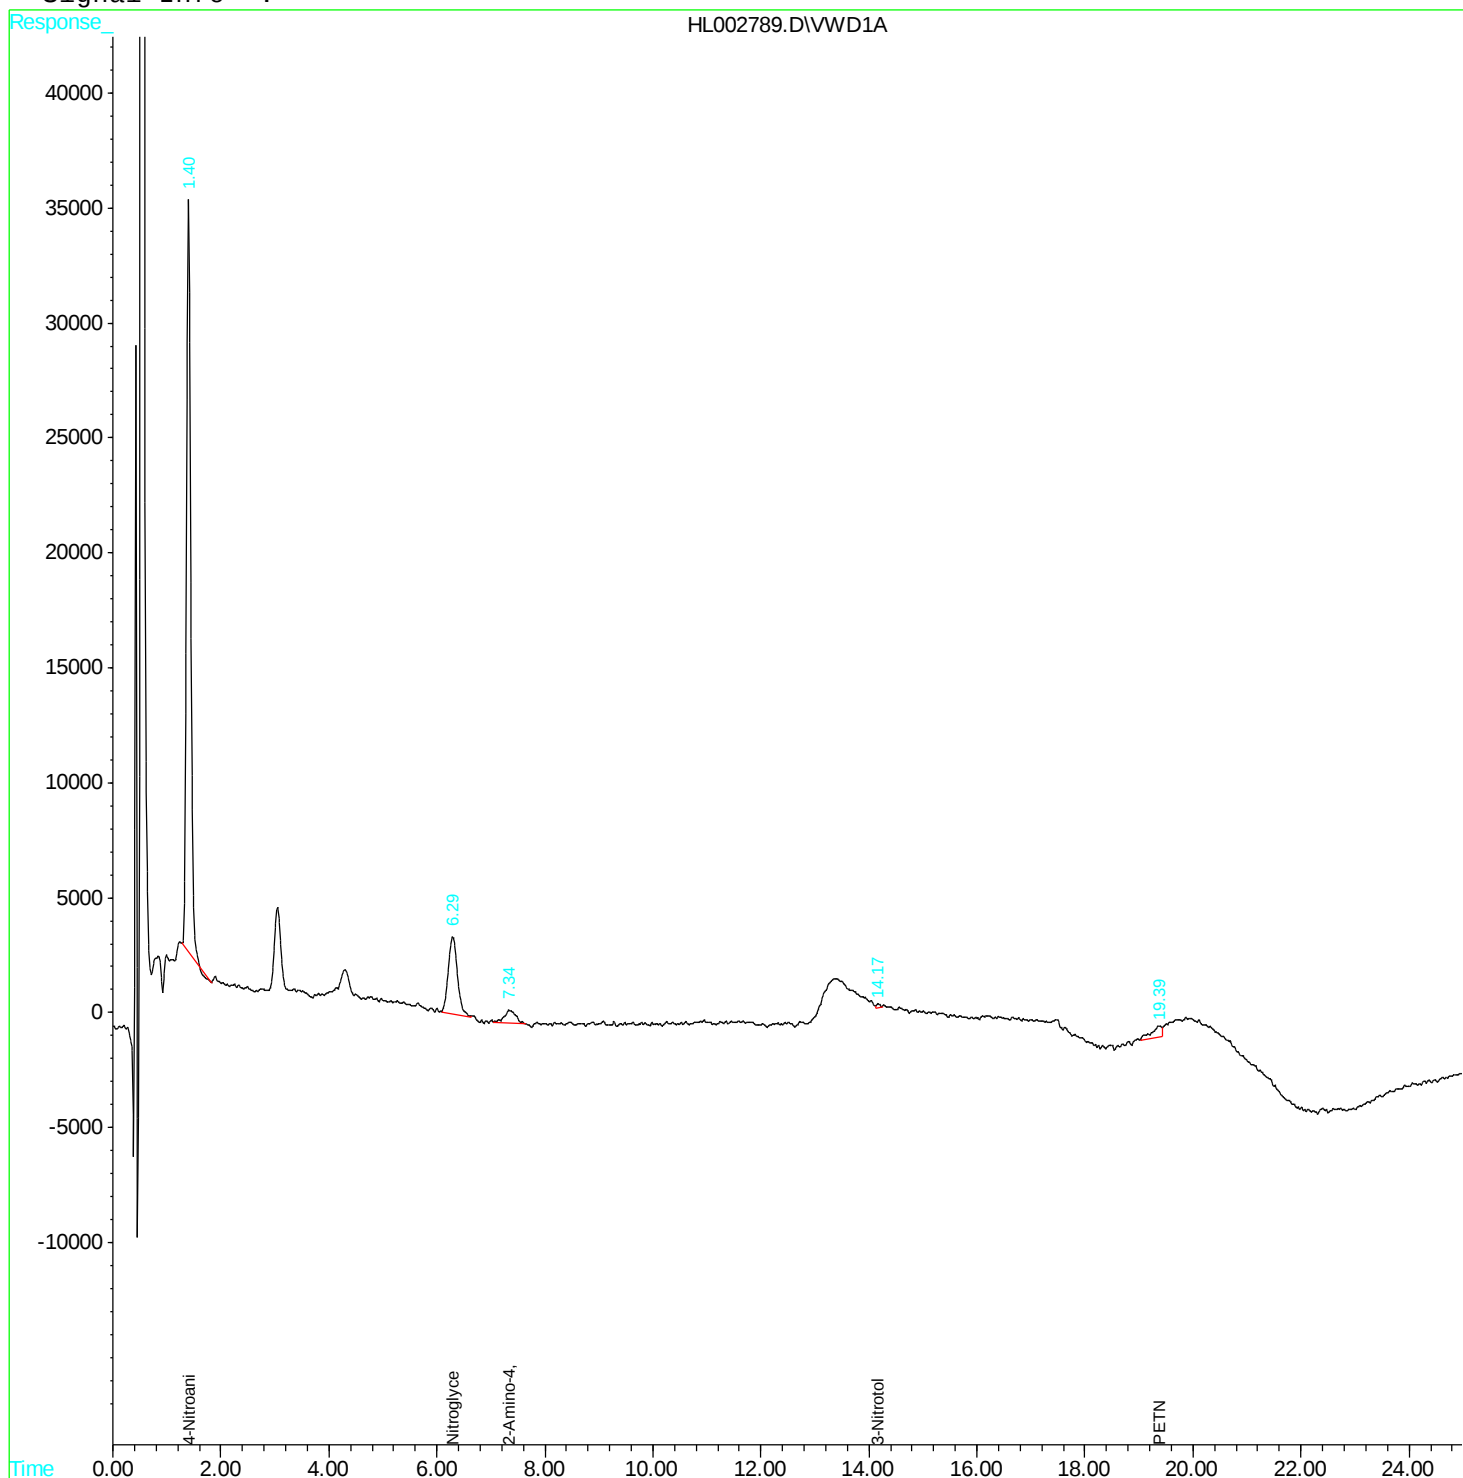

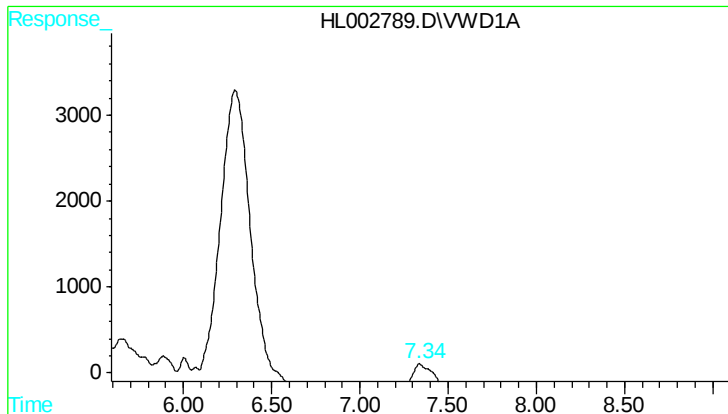


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.338 min
Delta R.T.: 0.058 min
Response: 80111
Conc: 7.14 ug/L

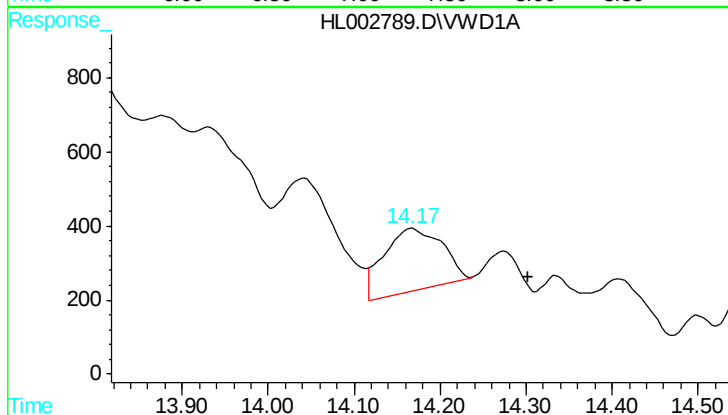


#14 3-Nitrotoluene

R.T.: 14.169 min
Delta R.T.: -0.134 min
Response: 7976
Conc: 1.12 ug/L

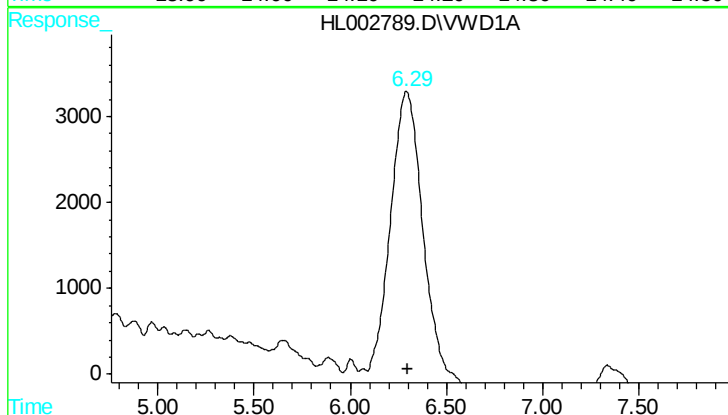

#17 Nitroglycerin

R.T.: 6.293 min
Delta R.T.: -0.007 min
Response: 395028
Conc: 6918.19 ug/L

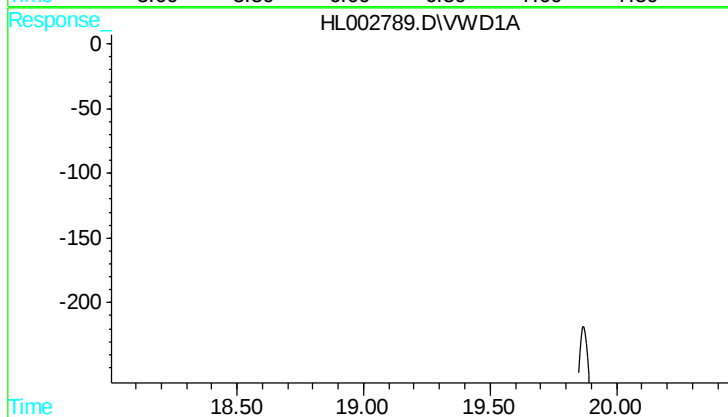

#18 PETN

R.T.: 19.389 min
Delta R.T.: 0.064 min
Response: 61127
Conc: 6.17 ug/L