

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002810.D Vial: 63
Acq On : 28-Apr-2012, 08:58 Operator: HLM
Sample : D2296-0 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 30 14:07 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Apr 30 14:06:15 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.40f	575559	151.119 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 50.37%

Target Compounds


7) T	2-Amino-4,6-dinitrotoluene	7.34f	97248	8.671 ug/L
------	----------------------------	-------	-------	------------


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002810.D Vial: 63
Acq On : 28-Apr-2012, 08:58 Operator: HLM
Sample : D2296-0 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 30 14:07 2012 Quant Results File: HL032912.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Apr 30 14:06:15 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

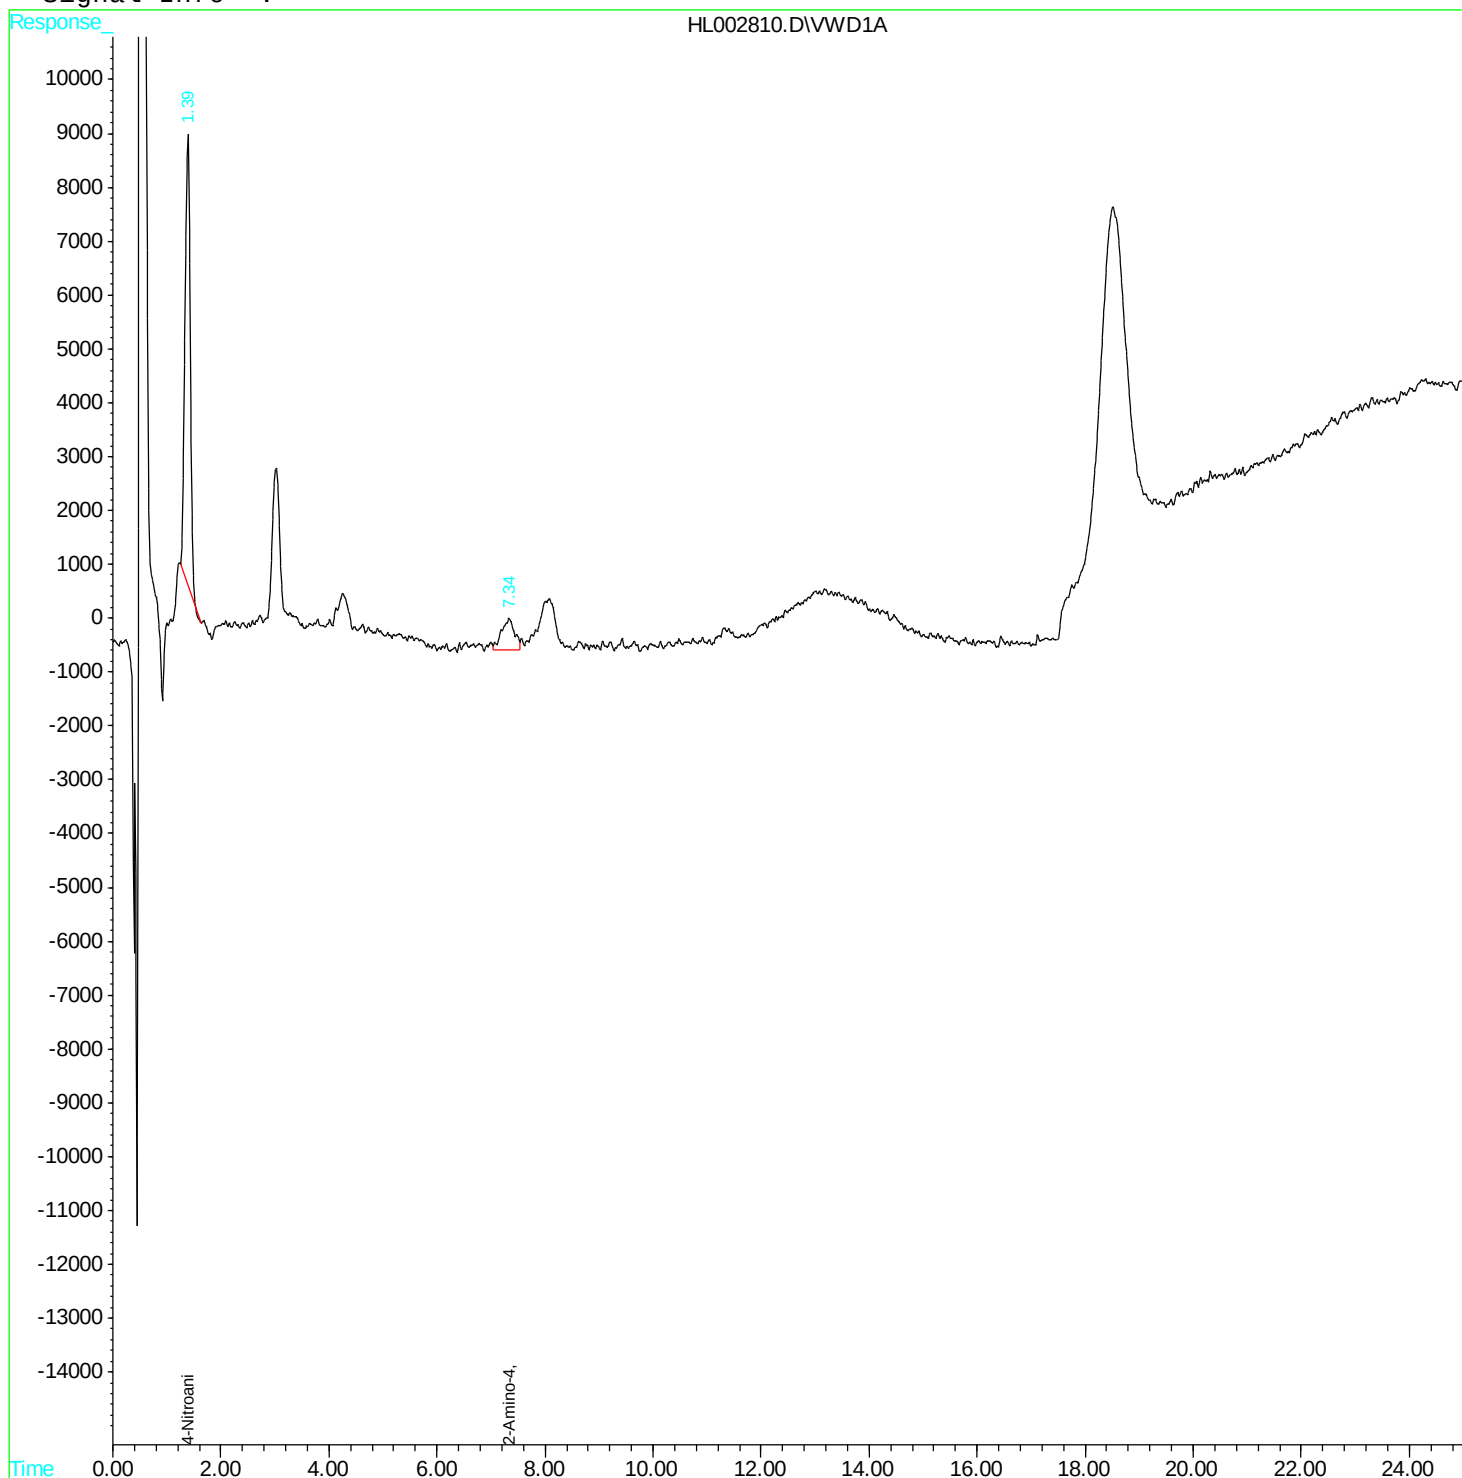

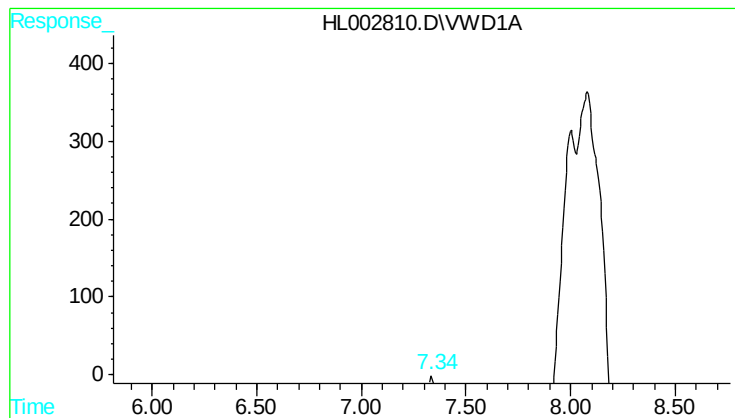

#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.338 min
Delta R.T.: 0.058 min
Response: 97248
Conc: 8.67 ug/L