

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002789.D Vial: 48
Acq On : 27-Apr-2012, 23:32 Operator: HLM
Sample : D2332-07MS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 30 17:52 2012 Quant Results File: HL032912.RES

Instrument :
HPLC_L
ClientSampleId :
TW-25MS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Apr 30 14:06:15 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.40	1789262	469.788 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 156.60%#

Target Compounds

17) T	Nitroglycerin	6.29	395028	6918.192 ug/L
-------	---------------	------	--------	---------------


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\120427\HL002789.D Vial: 48
 Acq On : 27-Apr-2012, 23:32 Operator: HLM
 Sample : D2332-07MS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Apr 30 17:52 2012 Quant Results File: HL032912.RES

Instrument :
 HPLC_L
 ClientSampleId :
 TW-25MS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Apr 30 14:06:15 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

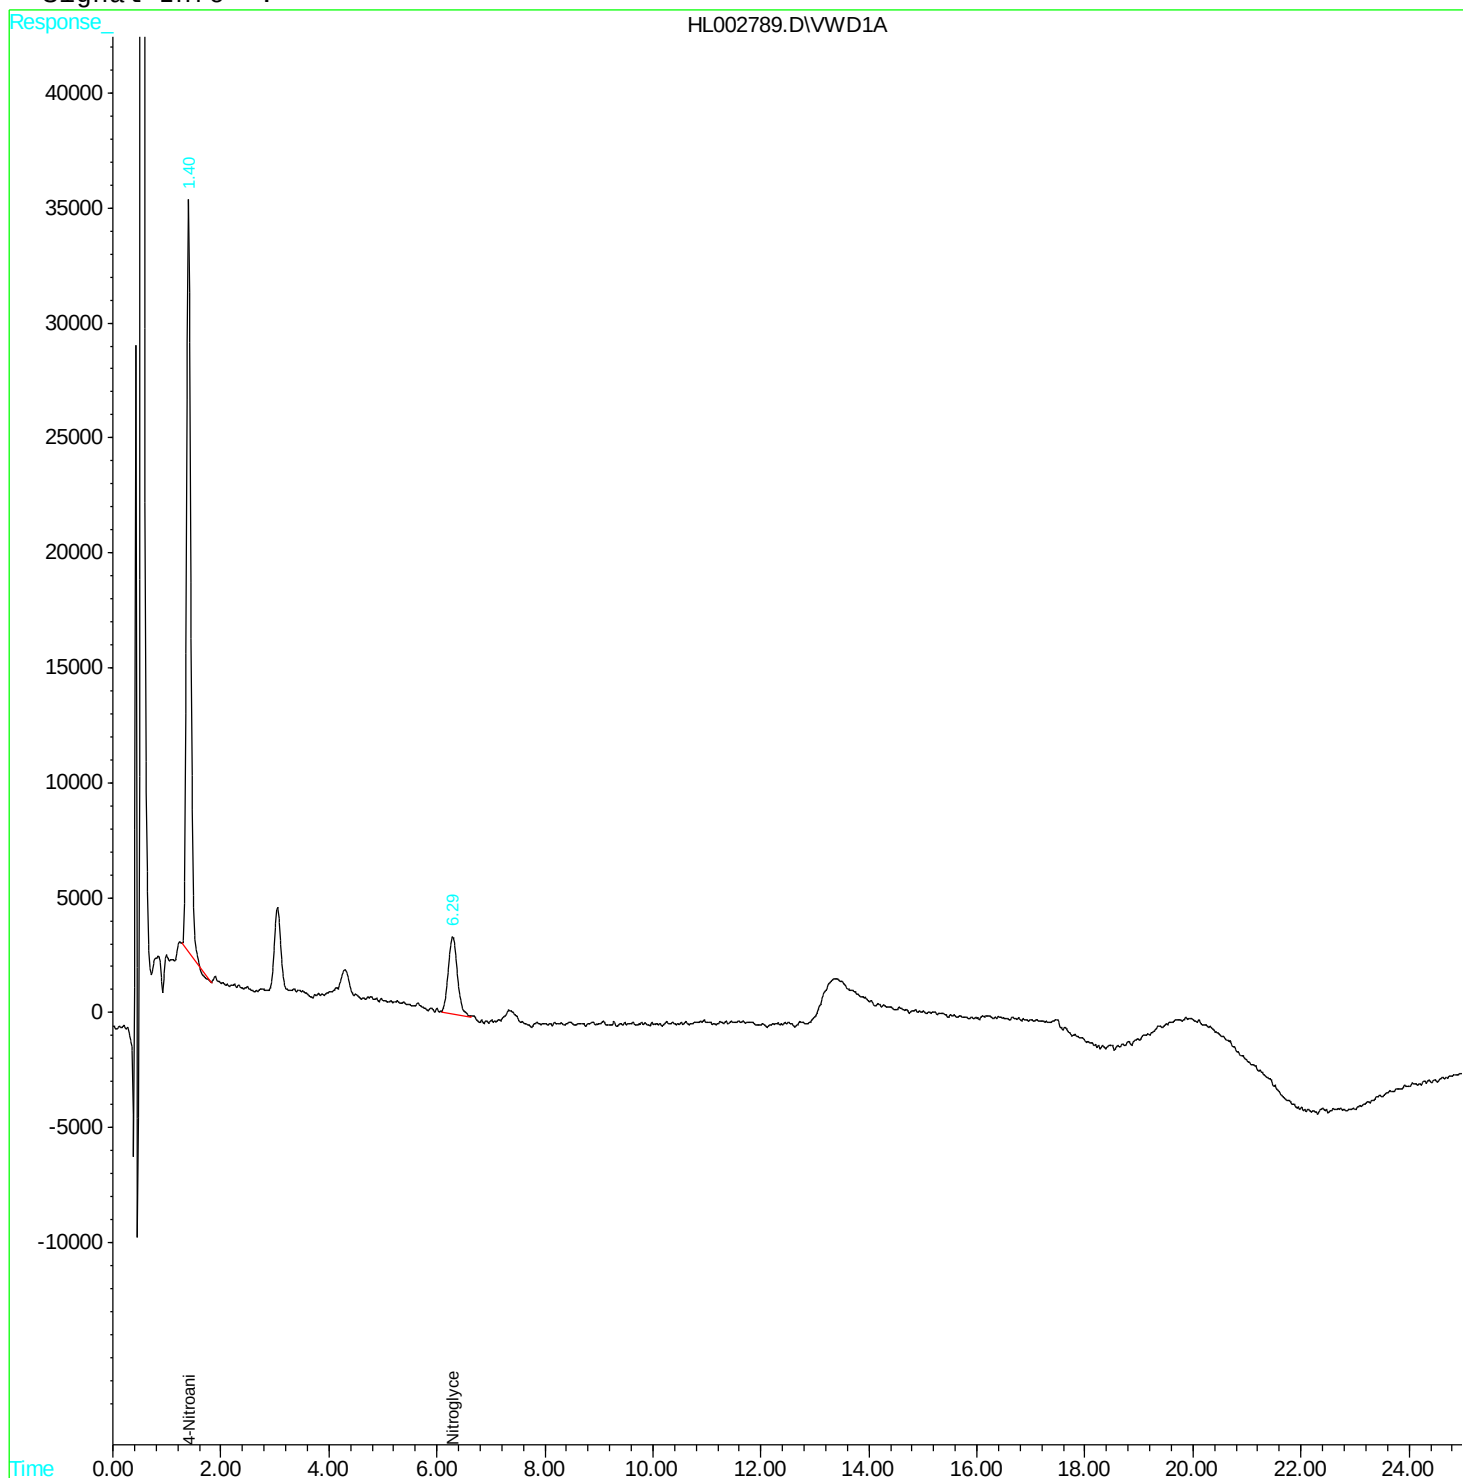

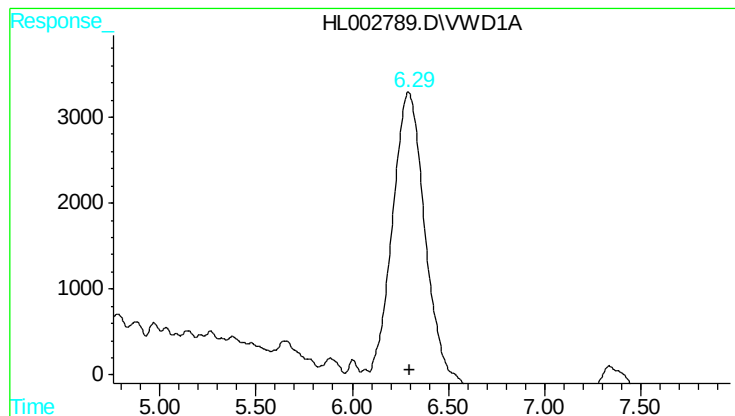

#17 Nitroglycerin

R.T.: 6.293 min
Delta R.T.: -0.007 min
Response: 395028
Conc: 6918.19 ug/L

Instrument :
HPLC_L
ClientSampleId :
TW-25MS2