

Data File : H:\VOL1\HPLC\HPLC L\120427\HL002791.D Vial: 50
Acq On : 28-Apr-2012, 00:26 Operator: HLM
Sample : D2332-08MSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 30 14:06 2012 Quant Results File: HL032912.RES

Instrument :
HPLC_L
ClientSampleId :
TW-25MSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Apr 30 14:06:15 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.41	1818159	477.376 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 159.13%#

Target Compounds


17) T	Nitroglycerin	6.31	411313	7203.401 ug/L
-------	---------------	------	--------	---------------


Data File : H:\VOL1\HPLC\HPLC L\120427\HL002791.D Vial: 50
Acq On : 28-Apr-2012, 00:26 Operator: HLM
Sample : D2332-08MSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Apr 30 14:06 2012 Quant Results File: HL032912.RES

Instrument :
HPLC_L
ClientSampleId :
TW-25MSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL032912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Apr 30 14:06:15 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

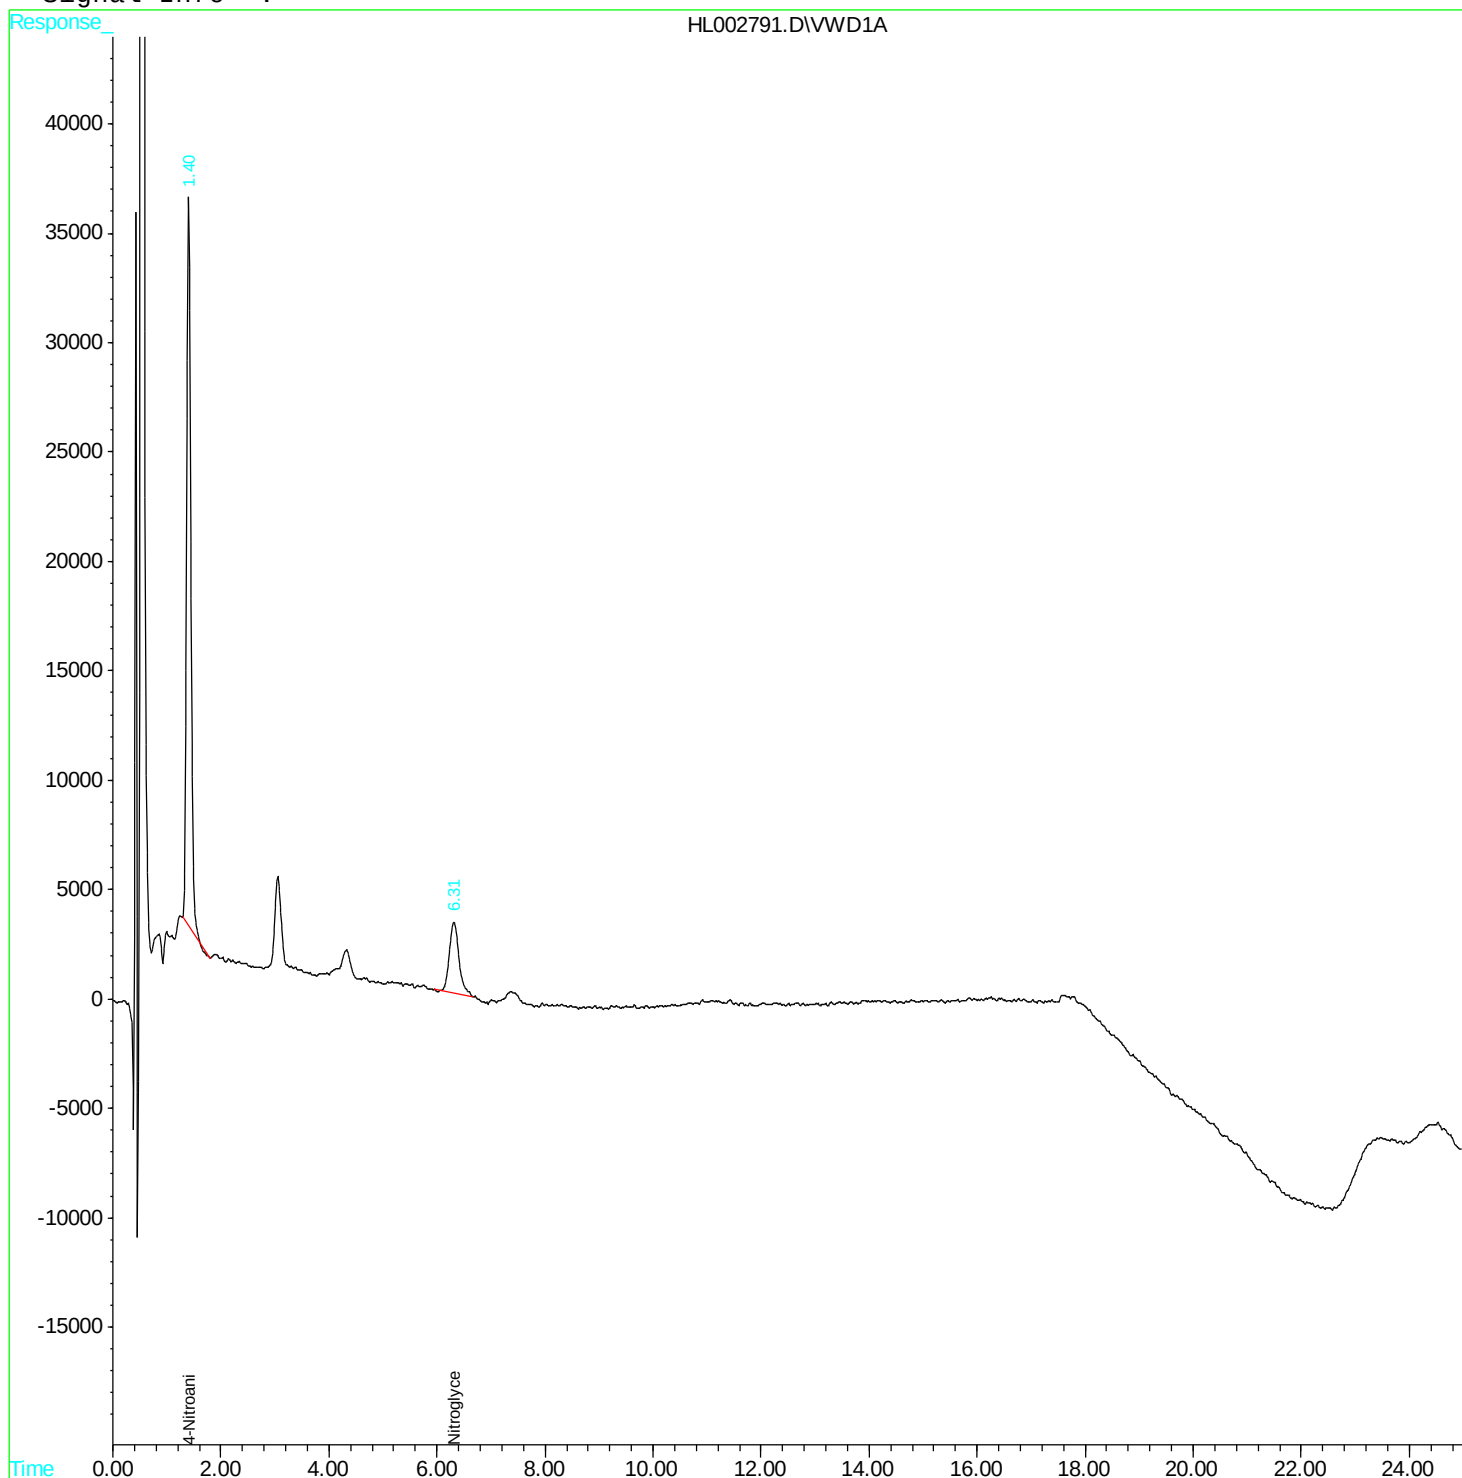

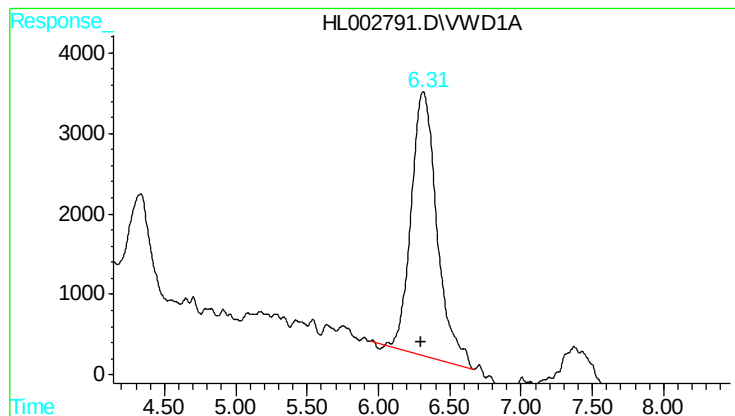

#17 Nitroglycerin

R.T.: 6.314 min
Delta R.T.: 0.014 min
Response: 411313
Conc: 7203.40 ug/L

Instrument :
HPLC_L
ClientSampleId :
TW-25MSD2