

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL050815\
 Data File : HL006198.D
 Signal(s) : vwd1A.ch
 Acq On : 08-May-2015, 17:20
 Operator : TP/IZ
 Sample : HSTDICC0100
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICC0100

Integration File: AUTOINT1.E
 Quant Time: May 22 14:05:37 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL050815.M
 Quant Title :
 QLast Update : Fri May 22 14:05:14 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) T RDX	2.431	1567752	195.851 ug/L
4) T 1,3,5-Trinitrobenzene	3.855	1829842	117.284 ug/L
5) T 1,3-Dinitrobenzene	5.068	2707196	116.873 ng/ml
6) T 3,5-Dinitroaniline	5.811	2136705	118.157 ug/L
7) T Nitrobenzene	6.521	1548388	118.826 ug/L
8) T Tetryl	8.551	1042104	88.707 ug/L
9) T 2,4,6-Trinitrotoluene	9.066	1683785	116.227 ug/L
10) T 2-Amino-4,6-dinitroto...	10.273	1716018	119.374 ug/L
11) T 4-Amino-2,6-dinitroto...	10.798	1205054	124.608 ug/L
12) T 2,4-Dinitrotoluene	11.575	2469196	118.781 ug/L
13) T 2,6-Dinitrotoluene	11.938	1327748	120.981 ug/L
14) T 2-Nitrotoluene	16.128	2781120	115.264 ug/L
15) T 4-Nitrotoluene	17.509	2081832	108.084 ug/L
16) T 3-Nitrotoluene	18.945	2999274	115.702 ug/L
17) T PETN	19.933	1479009	119.662 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL050815\
Data File : HL006198.D
Signal(s) : vwd1A.ch
Acq On : 08-May-2015, 17:20
Operator : TP/IZ
Sample : HSTDICC0100
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0100

Integration File: AUTOINT1.E
Quant Time: May 22 14:05:37 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL050815.M
Quant Title :
QLast Update : Fri May 22 14:05:14 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

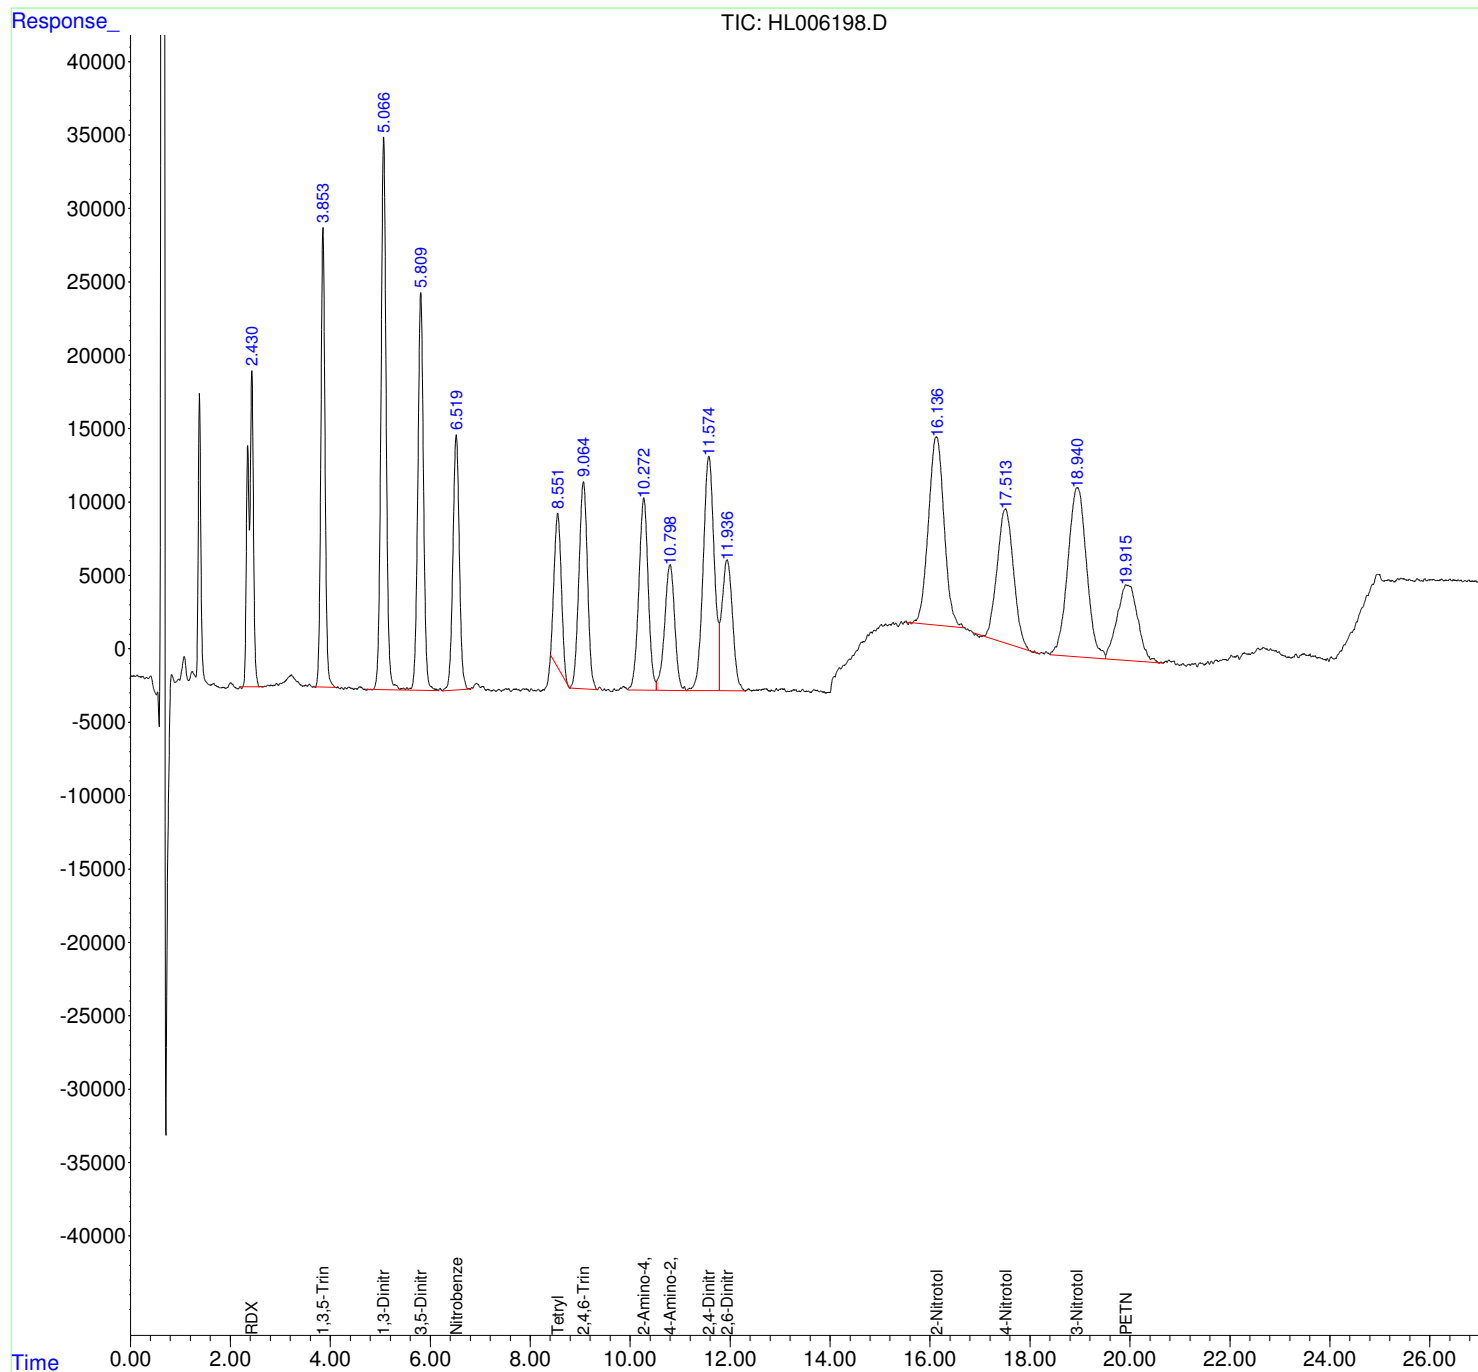


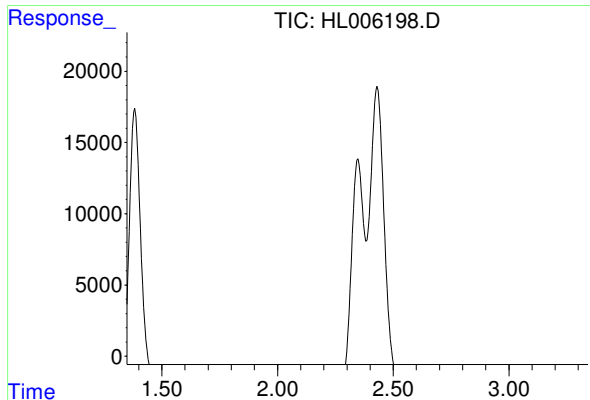

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.346 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0100

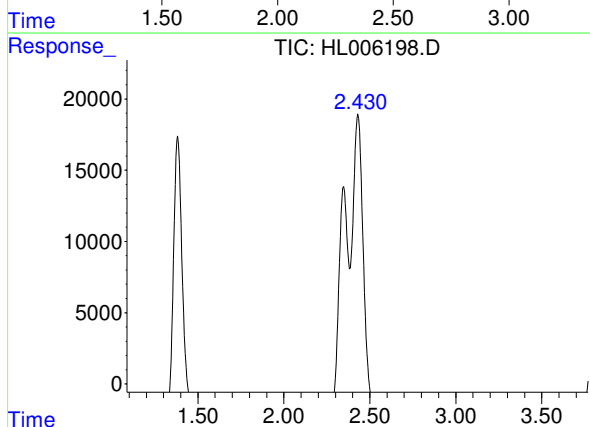


#3 RDX

R.T.: 2.431 min
Delta R.T.: 0.001 min
Response: 1567752
Conc: 195.85 ug/L

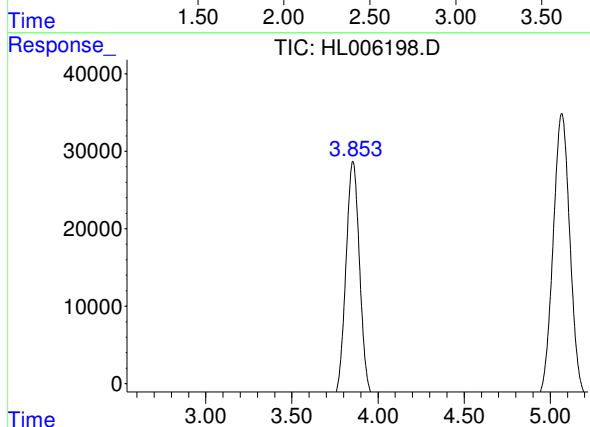


#4 1,3,5-Trinitrobenzene

R.T.: 3.855 min
Delta R.T.: 0.002 min
Response: 1829842
Conc: 117.28 ug/L

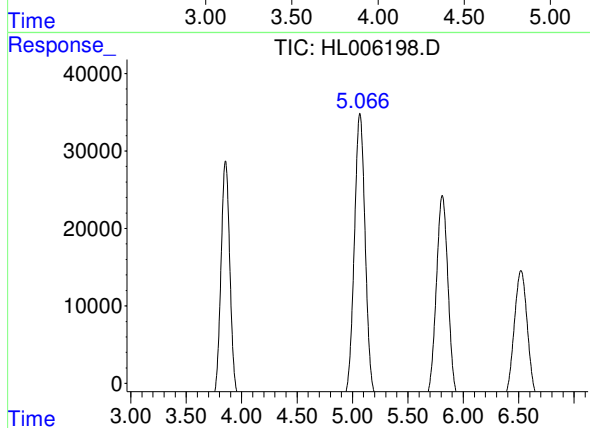

#5 1,3-Dinitrobenzene


R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 2707196
Conc: 116.87 ng/ml

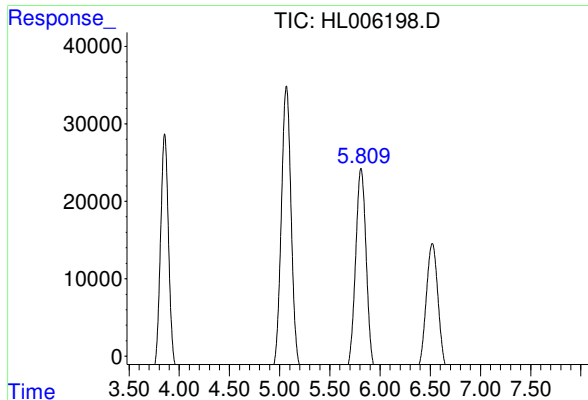

#6 3,5-Dinitroaniline


R.T.: 5.811 min
Delta R.T.: 0.000 min
Response: 2136705
Conc: 118.16 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0100

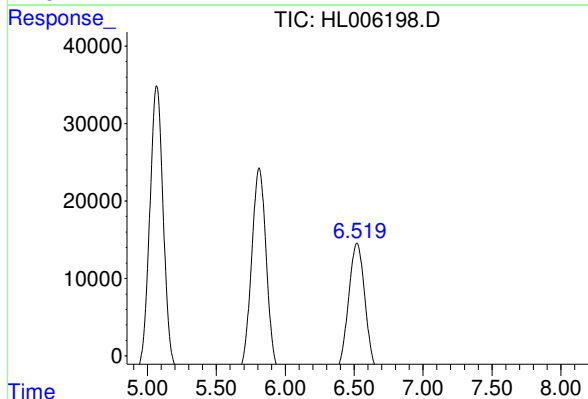


#7 Nitrobenzene

R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 1548388
Conc: 118.83 ug/L

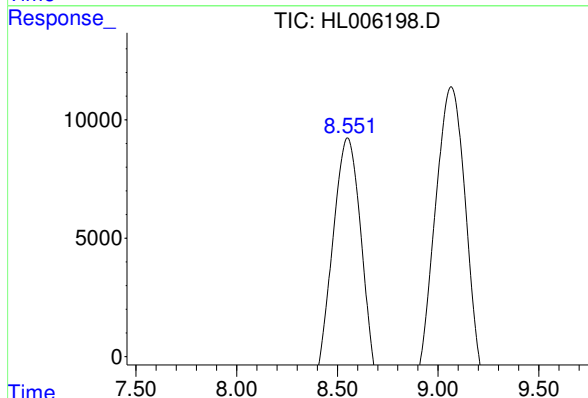


#8 Tetryl

R.T.: 8.551 min
Delta R.T.: 0.000 min
Response: 1042104
Conc: 88.71 ug/L

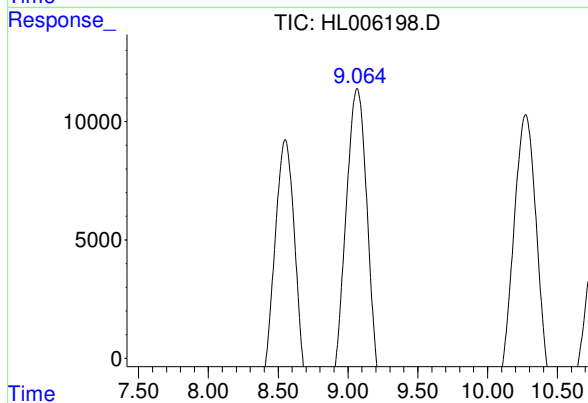

#9 2,4,6-Trinitrotoluene


R.T.: 9.066 min
Delta R.T.: 0.000 min
Response: 1683785
Conc: 116.23 ug/L

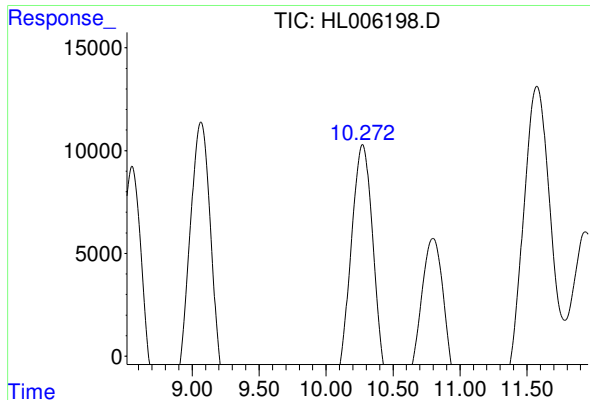

#10 2-Amino-4,6-dinitrotoluene


R.T.: 10.273 min
Delta R.T.: 0.000 min
Response: 1716018
Conc: 119.37 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0100

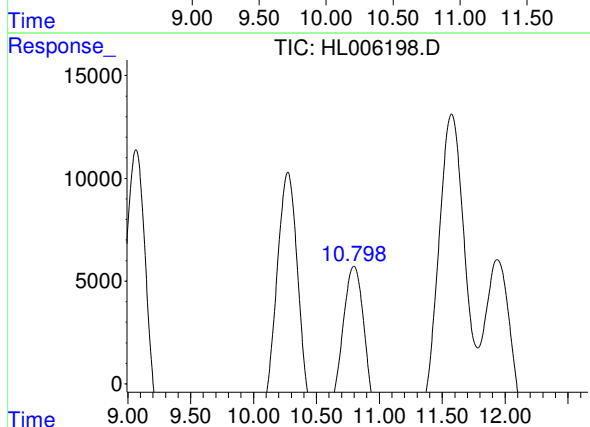


#11 4-Amino-2,6-dinitrotoluene

R.T.: 10.798 min
Delta R.T.: 0.000 min
Response: 1205054
Conc: 124.61 ug/L

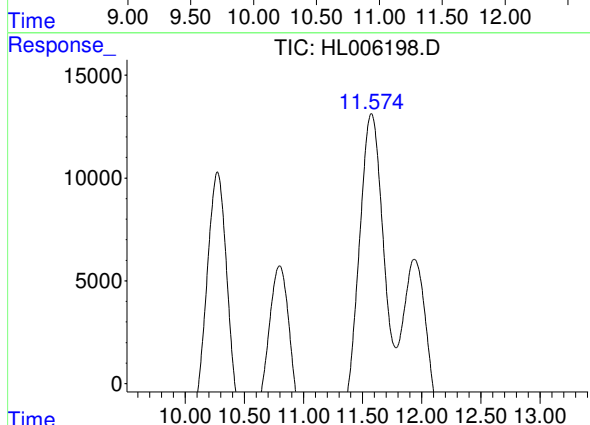


#12 2,4-Dinitrotoluene

R.T.: 11.575 min
Delta R.T.: 0.000 min
Response: 2469196
Conc: 118.78 ug/L

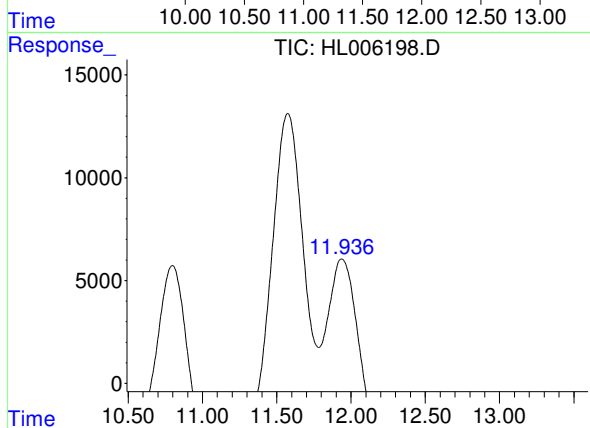

#13 2,6-Dinitrotoluene


R.T.: 11.938 min
Delta R.T.: 0.000 min
Response: 1327748
Conc: 120.98 ug/L

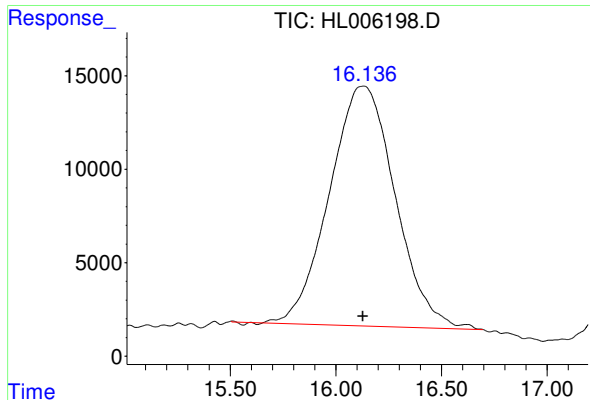

#14 2-Nitrotoluene


R.T.: 16.128 min
Delta R.T.: 0.000 min
Response: 2781120
Conc: 115.26 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0100

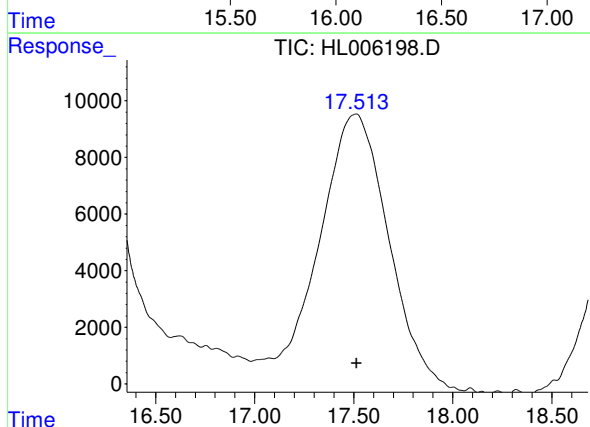


#15 4-Nitrotoluene

R.T.: 17.509 min
Delta R.T.: -0.005 min
Response: 2081832
Conc: 108.08 ug/L

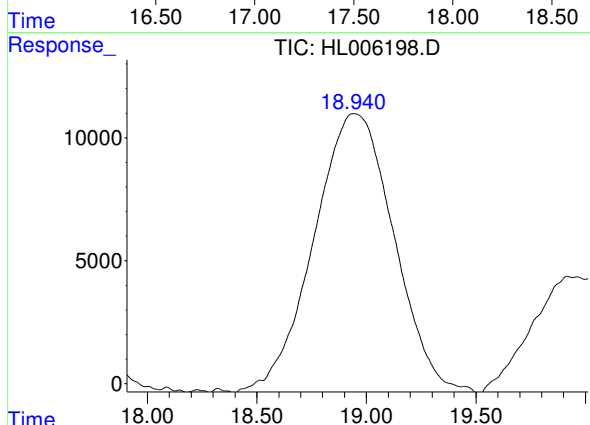

#16 3-Nitrotoluene

R.T.: 18.945 min
Delta R.T.: 0.005 min
Response: 2999274
Conc: 115.70 ug/L

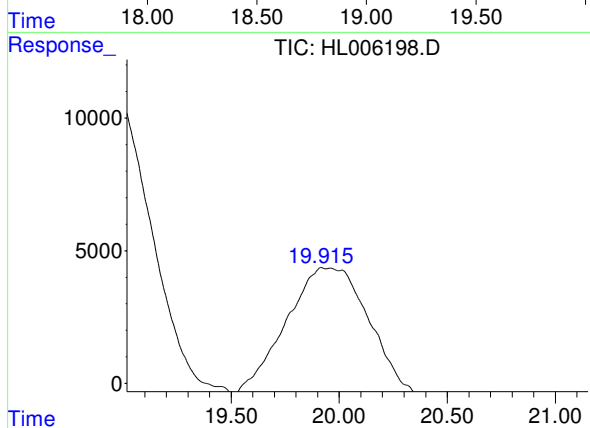

#17 PETN

R.T.: 19.933 min
Delta R.T.: 0.018 min
Response: 1479009
Conc: 119.66 ug/L