

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL050815\
Data File : HL006204.D
Signal(s) : vwd1A.ch
Acq On : 08-May-2015, 20:10
Operator : TP/IZ
Sample : SSTDICC050
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SSTDICC050

Manual Integrations
APPROVED

apatel
5/22/2015 4:34:23 PM

Integration File: AUTOINT1.E
Quant Time: May 22 15:15:11 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL0508NG.M
Quant Title :
QLast Update : Fri May 22 15:15:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.299	257998884	48.859 ng/ulm
Target Compounds			
2) T Nitroglycerin	6.884	532922268	48.263 ng/ul

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL050815\
Data File : HL006204.D
Signal(s) : vwd1A.ch
Acq On : 08-May-2015, 20:10
Operator : TP/IZ
Sample : SSTDICC050
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
SSTDICC050


Manual Integrations
APPROVED

apatel
5/22/2015 4:34:23 PM

Integration File: AUTOINT1.E
Quant Time: May 22 15:15:11 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL0508NG.M
Quant Title :
QLast Update : Fri May 22 15:15:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

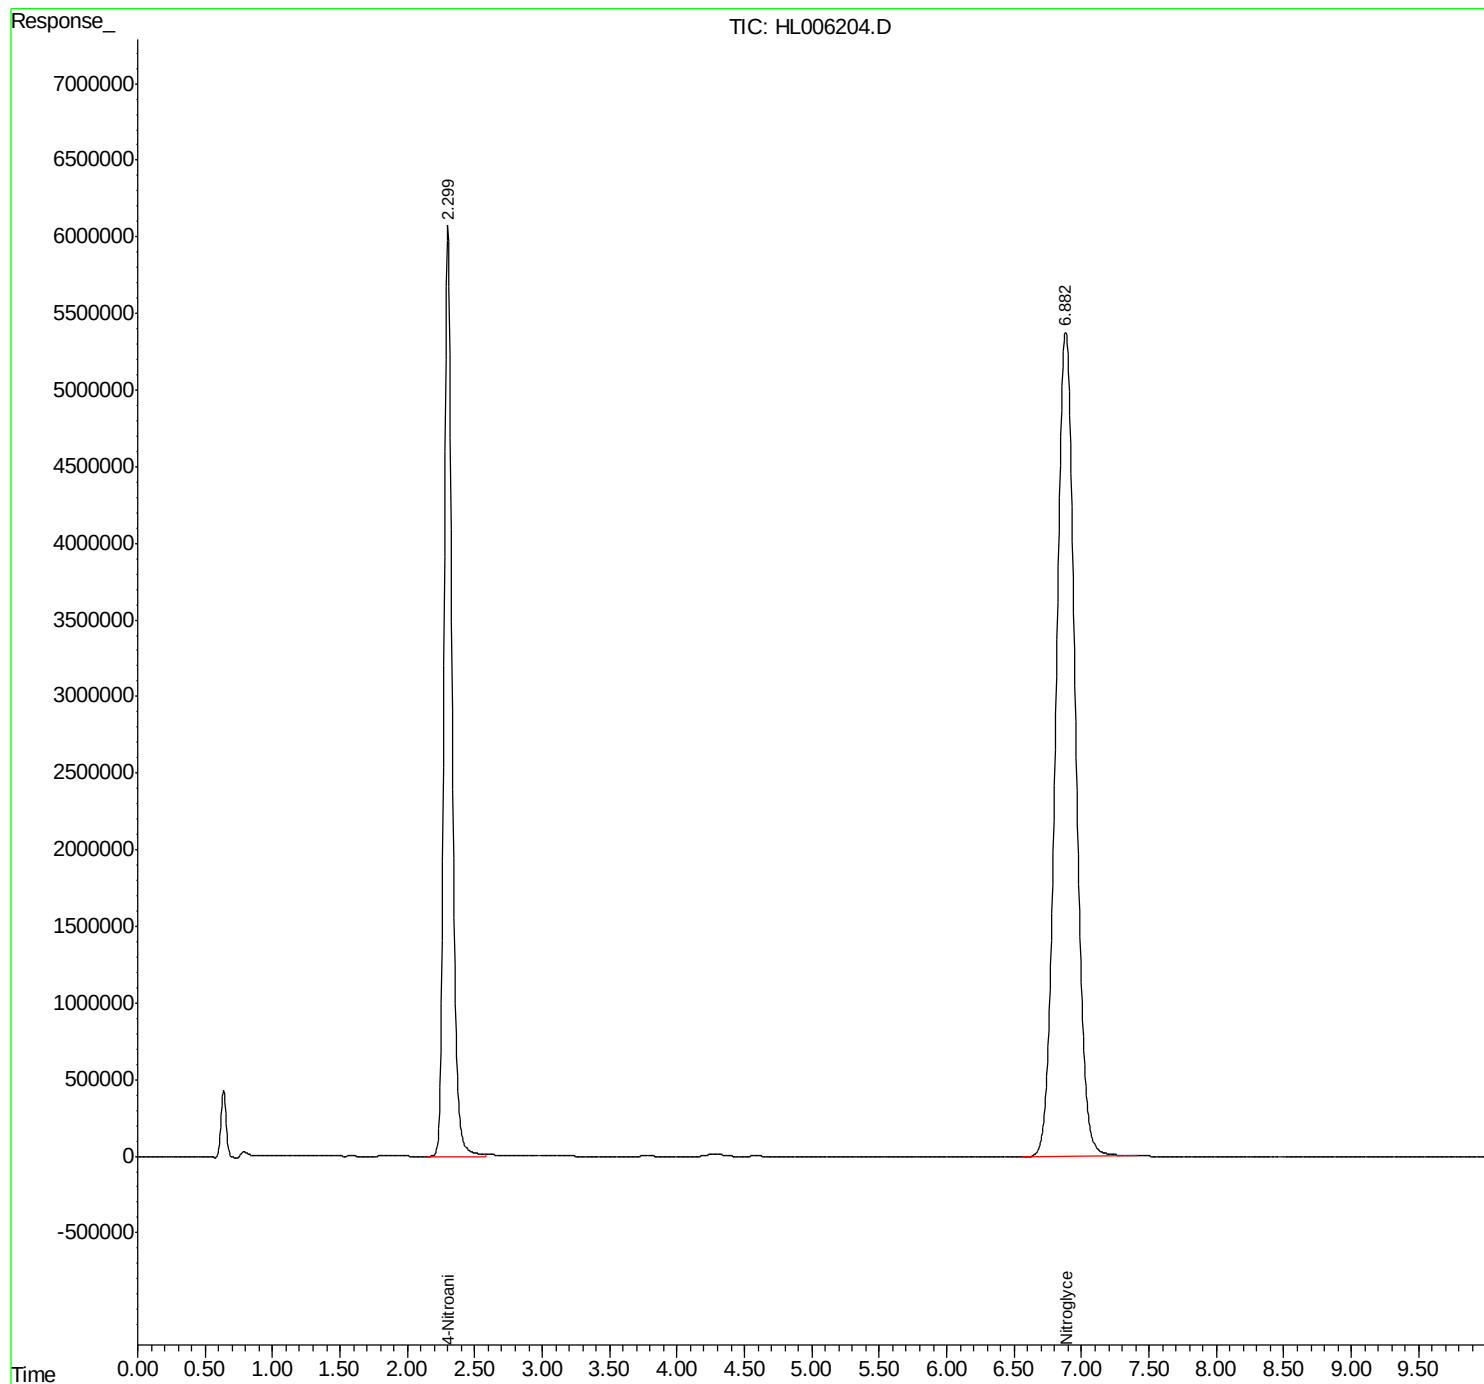

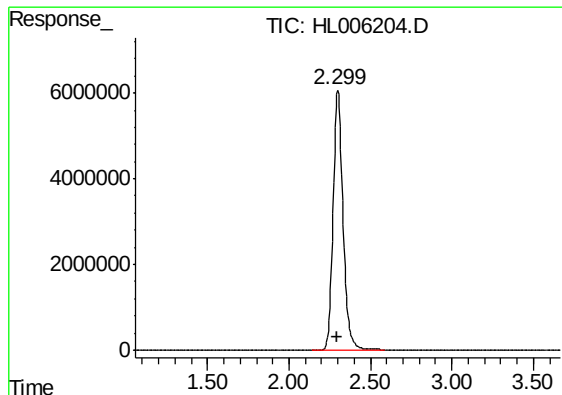


#1 4-Nitroaniline

R.T.: 2.299 min
 Delta R.T.: 0.000 min
 Response: 257998884
 Conc: 48.86 ng/ul m

Instrument :
 HPLC_L
 ClientSampleId :
 SSTDICC050

Manual Integrations
 APPROVED

apatel
 5/22/2015 4:34:23 PM

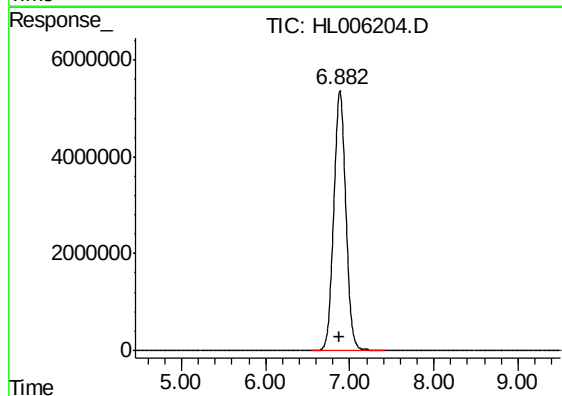

#2 Nitroglycerin

R.T.: 6.884 min
 Delta R.T.: 0.002 min
 Response: 532922268
 Conc: 48.26 ng/ul