

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL052213\HL005286.D Vial: 11
Acq On : 22-May-2013, 22:40 Operator: QM
Sample : E2171-09 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 23 11:20 2013 Quant Results File: HL052213.RES

Instrument :
HPLC_L
ClientSampleId :
B1222SW-01

Manual Integrations
APPROVED

mohammad
5/31/2013 5:15:47 PM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL052213.M
Title :
Last Update : Thu May 23 10:04:01 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	1234814	311.023 ug/L

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005286.D HL052213.M

Thu May 23 12:26:19 2013

RPT1

Quantitation Report

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL052213\HL005286.D Vial: 11
Acq On : 22-May-2013, 22:40 Operator: QM
Sample : E2171-09 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 23 11:20 2013 Quant Results File: HL052213.RES


Instrument :
HPLC_L
ClientSampleId :
B1222SW-01


Manual Integrations
APPROVED

mohammad
5/31/2013 5:15:47 PM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL052213.M
Title :
Last Update : Thu May 23 10:04:01 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

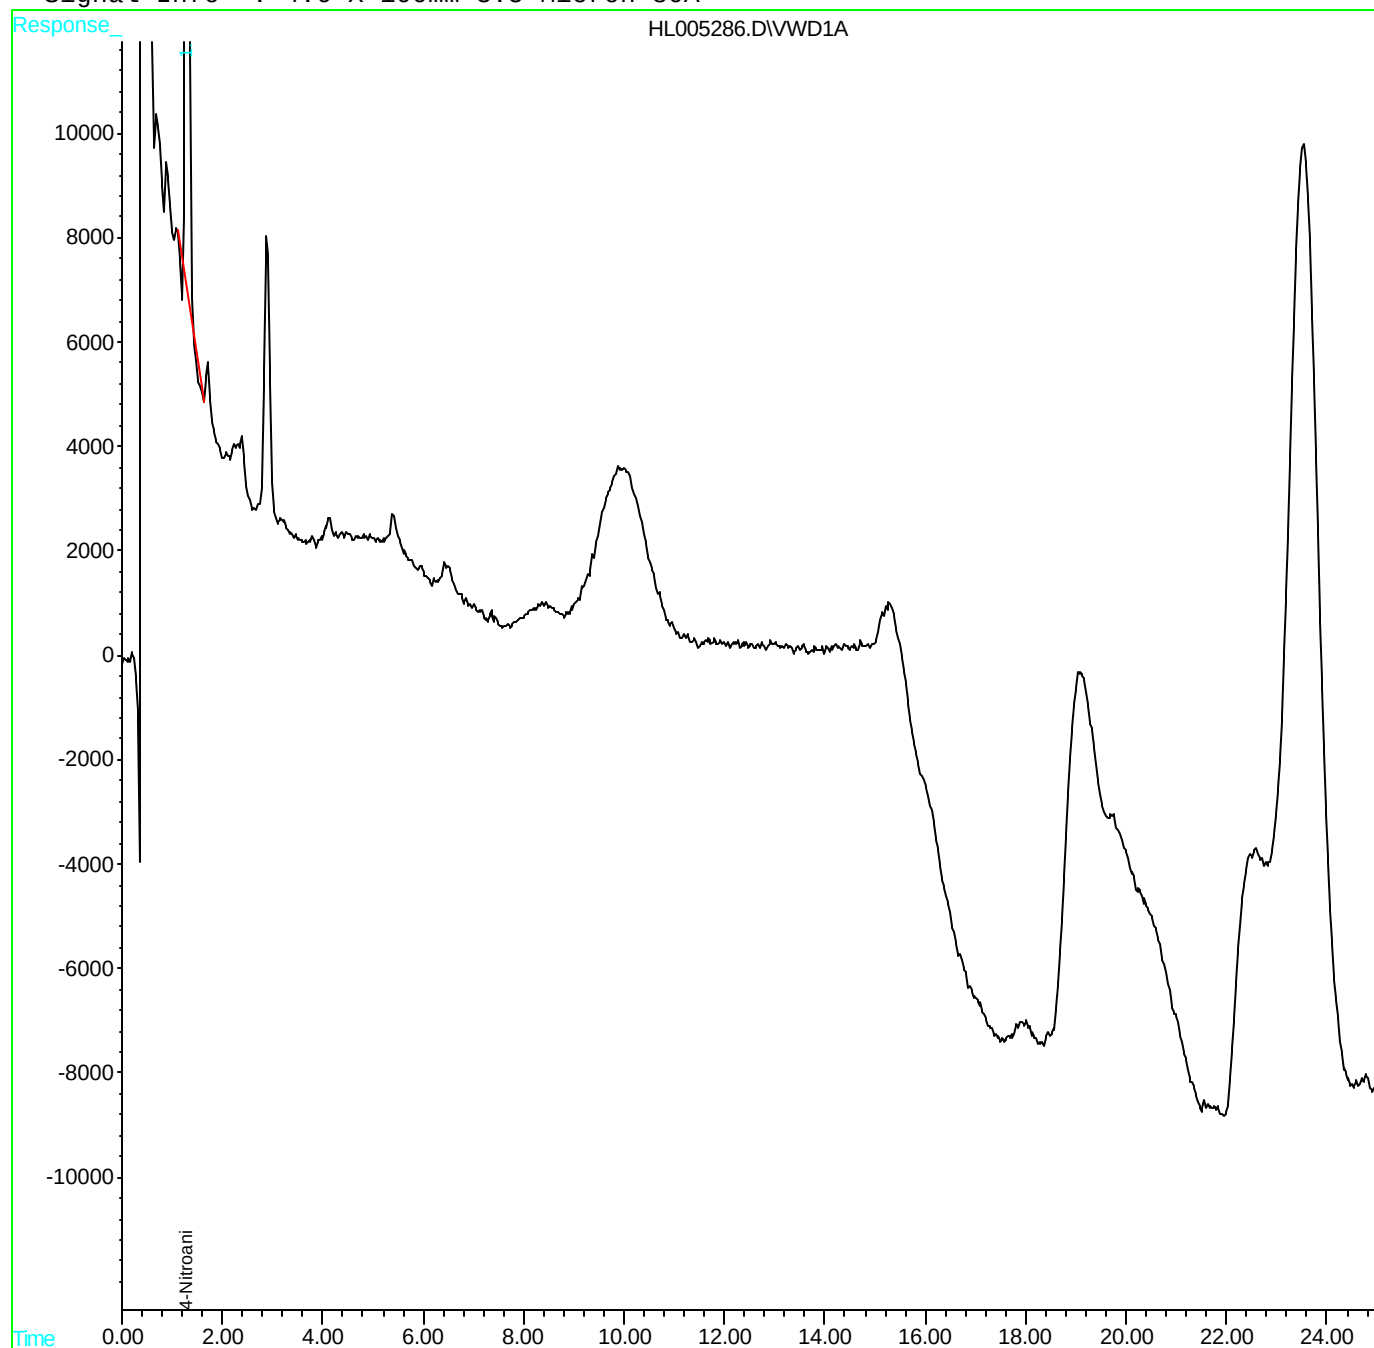

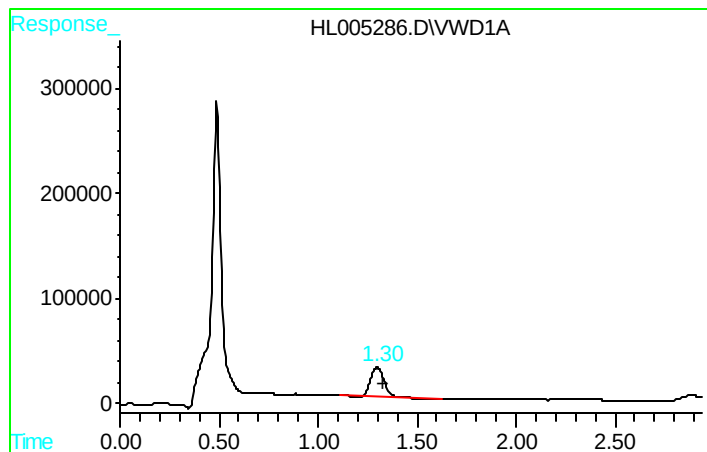

#1 4-Nitroaniline

R.T.: 1.299 min
Delta R.T.: -0.030 min
Response: 1234814
Conc: 311.02 ug/L

Instrument :

HPLC_L

ClientSampleId :

B1222SW-01

Manual Integrations
APPROVED

mohammad
5/31/2013 5:15:47 PM