

Data Path : X:\HPCHEM1\HPLC_L\Data\HL052512\
 Data File : HL003059.D
 Signal(s) : VWD1A.CH
 Acq On : 25-May-2012, 15:20
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: events.e
 Quant Time: Jun 05 04:16:41 2012
 Quant Method : X:\HPCHEM1\HPLC_L\methods\HL050312.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Fri May 04 10:29:09 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.389f	4147575	1133.570 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 377.86%#
Target Compounds			
4) T 1,3,5-Trinitrobenzene	2.812f	6165848	491.663 ug/L
5) T Tetryl	6.425	8990343	1000.912 ug/L
6) T 2,4,6-Trinitrotoluene	6.824	6011724	499.986 ug/L
7) T 2-Amino-4,6-dinitroto...	7.261f	5801331	526.323 ug/L
8) T 4-Amino-2,6-dinitroto...	7.624	3960991	523.209 ug/L
9) T 2,4-Dinitrotoluene	8.513	8052179	496.090 ug/L
10) T 2,6-Dinitrotoluene	8.922	4488633	499.701 ug/L
11) T 1,3-Dinitrobenzene	3.729f	8680789	494.245 ug/L
12) T Nitrobenzene	5.020	5634713	510.069 ug/L
13) T 2-Nitrotoluene	12.309	7072851	1017.357 ug/L
14) T 3-Nitrotoluene	14.423	7650341	1016.120 ug/L
15) T 4-Nitrotoluene	13.107	6054550	1027.473 ug/L


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : X:\HPCHEM1\HPLC_L\Data\HL052512\
Data File : HL003059.D
Signal(s) : VWD1A.CH
Acq On : 25-May-2012, 15:20
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: events.e
Quant Time: Jun 05 04:16:41 2012
Quant Method : X:\HPCHEM1\HPLC_L\methods\HL050312.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri May 04 10:29:09 2012
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. :
Signal Phase :
Signal Info :

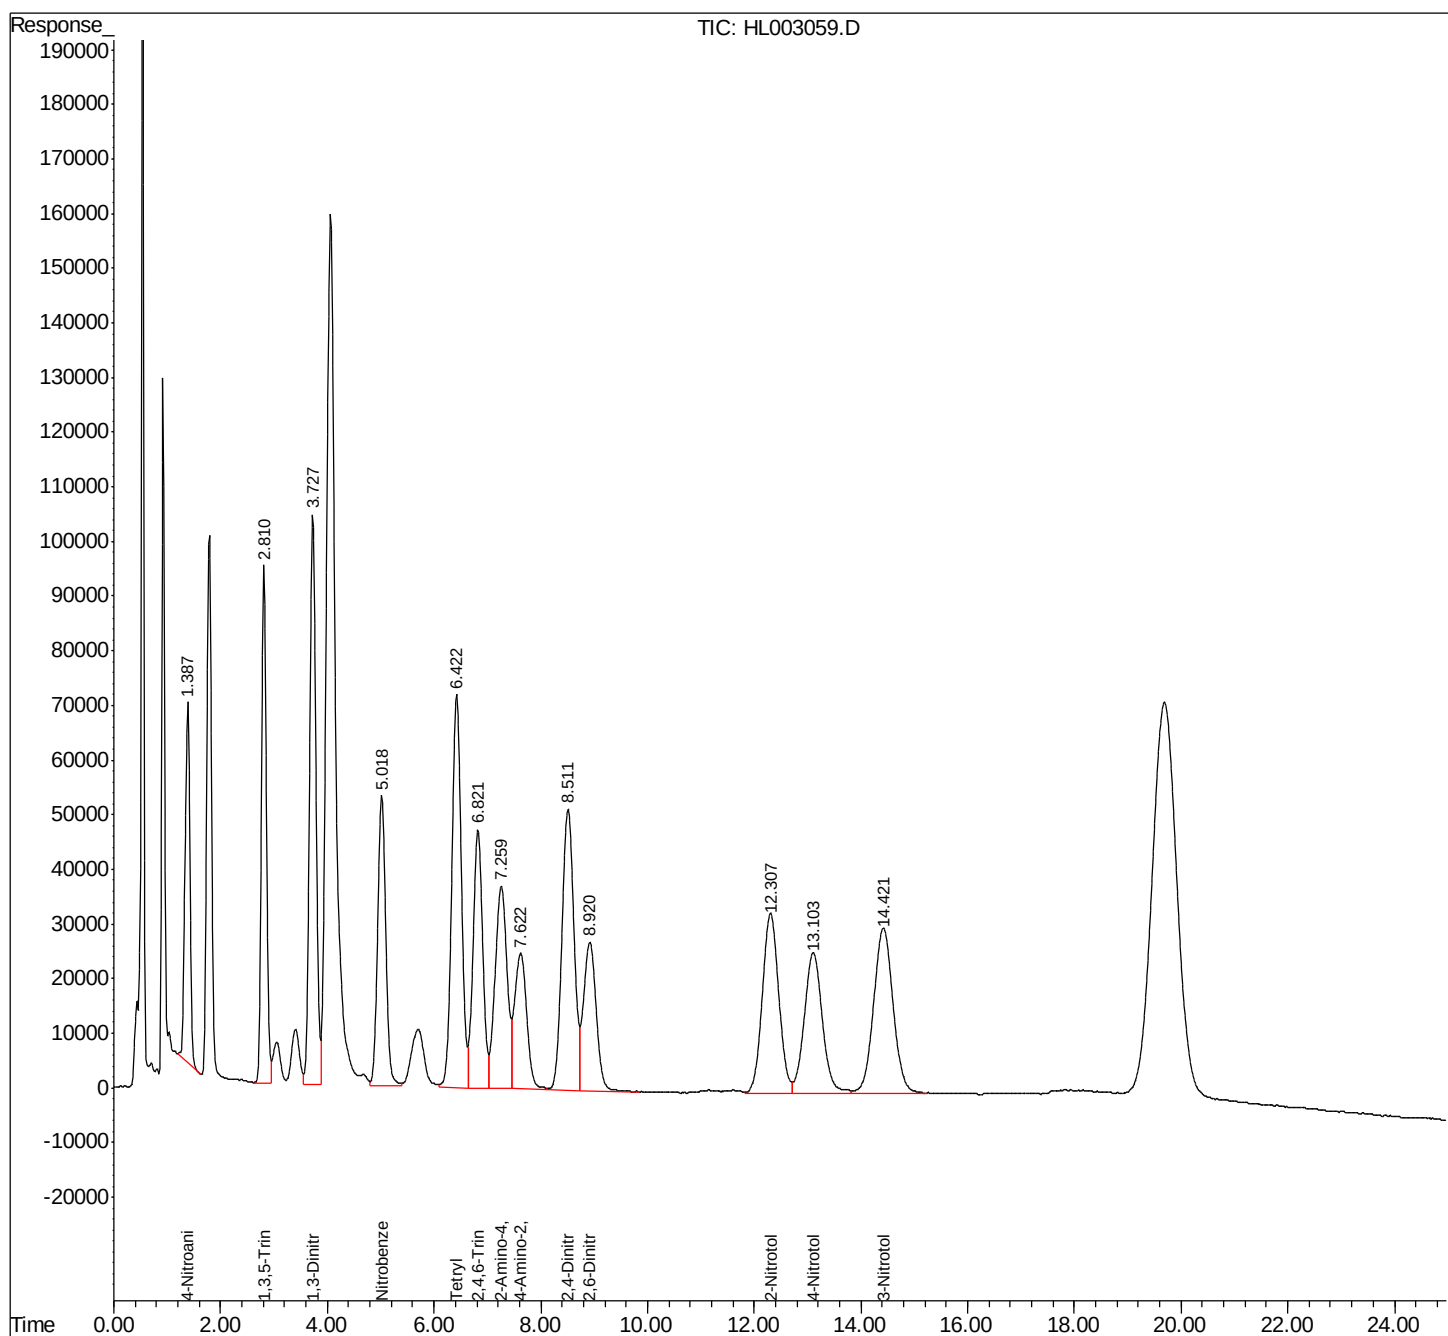

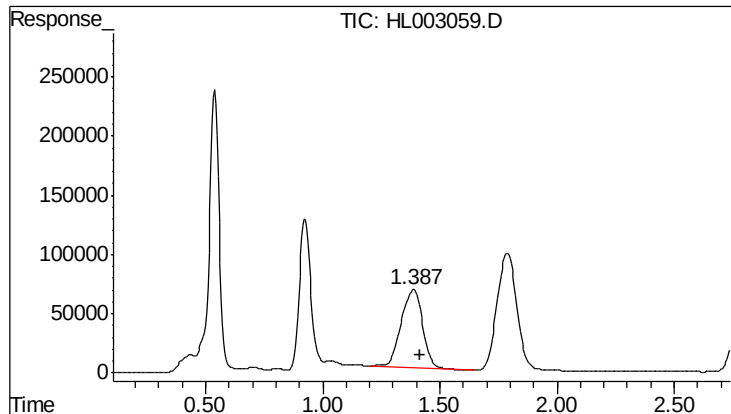


#1 4-Nitroaniline

R.T.: 1.389 min
 Delta R.T.: -0.024 min
 Response: 4147575
 Conc: 1133.57 ug/L

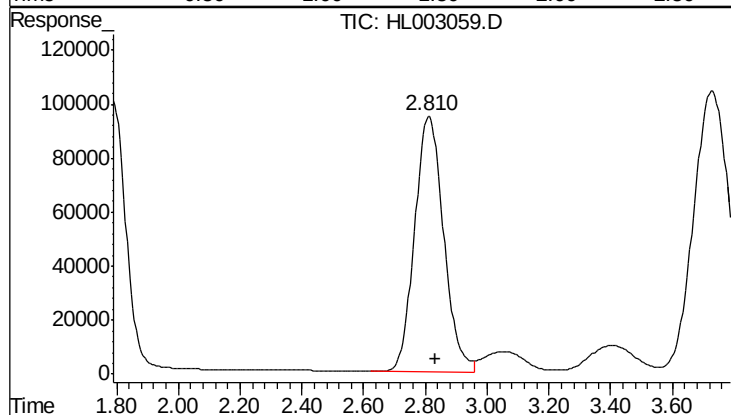


#4 1,3,5-Trinitrobenzene

R.T.: 2.812 min
 Delta R.T.: -0.020 min
 Response: 6165848
 Conc: 491.66 ug/L

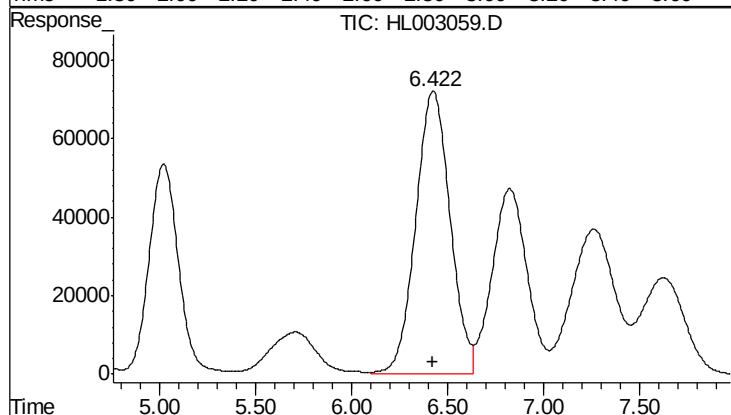


#5 Tetryl

R.T.: 6.425 min
 Delta R.T.: 0.000 min
 Response: 8990343
 Conc: 1000.91 ug/L

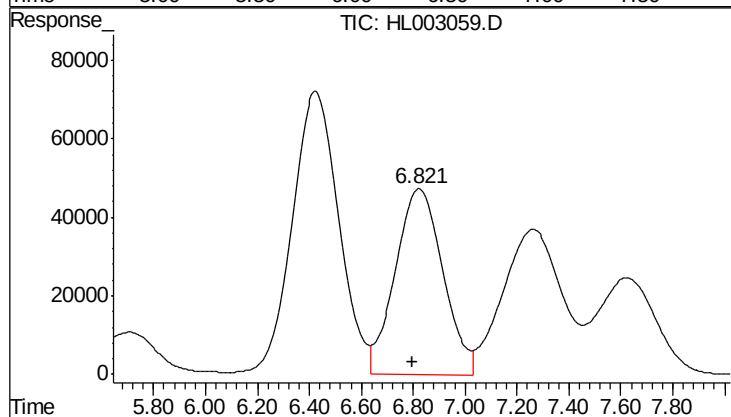


#6 2,4,6-Trinitrotoluene

R.T.: 6.824 min
 Delta R.T.: 0.028 min
 Response: 6011724
 Conc: 499.99 ug/L

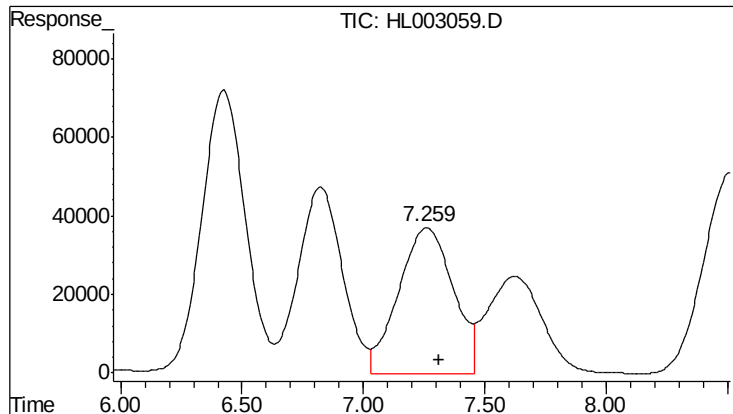


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.261 min
Delta R.T.: -0.052 min
Response: 5801331
Conc: 526.32 ug/L

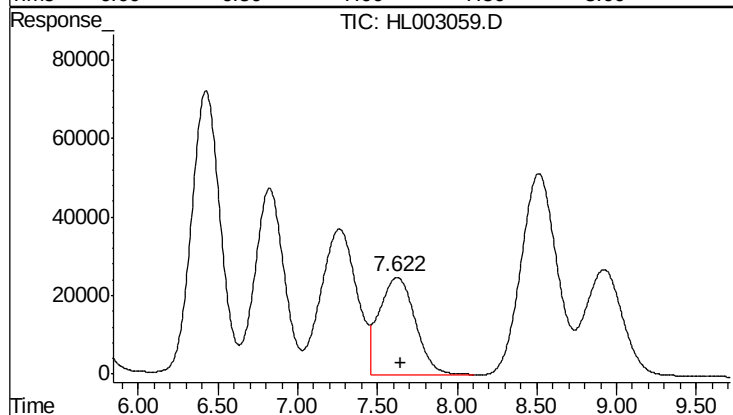


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.624 min
Delta R.T.: -0.025 min
Response: 3960991
Conc: 523.21 ug/L

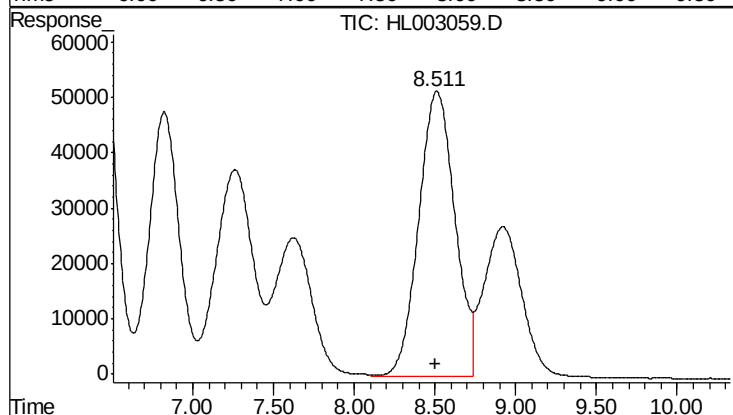


#9 2,4-Dinitrotoluene

R.T.: 8.513 min
Delta R.T.: 0.007 min
Response: 8052179
Conc: 496.09 ug/L

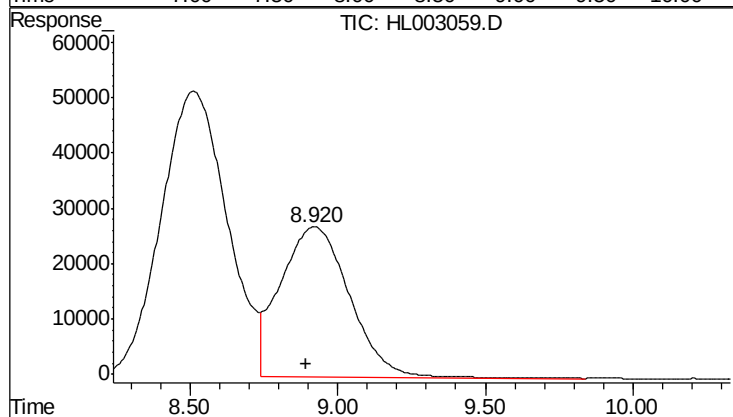


#10 2,6-Dinitrotoluene


R.T.: 8.922 min
Delta R.T.: 0.029 min
Response: 4488633
Conc: 499.70 ug/L

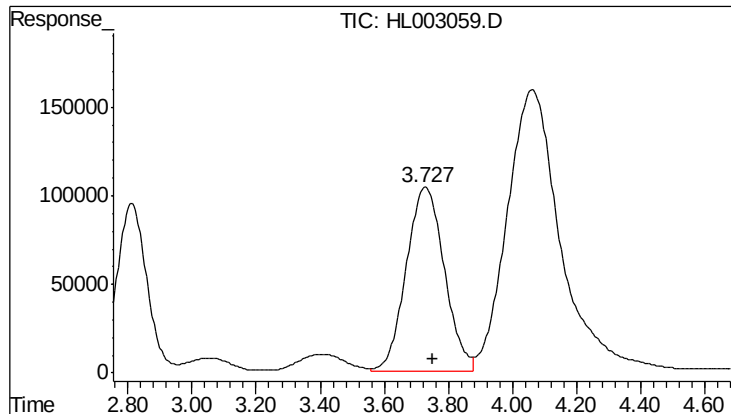


#11 1,3-Dinitrobenzene
 R.T.: 3.729 min
 Delta R.T.: -0.022 min
 Response: 8680789
 Conc: 494.25 ug/L

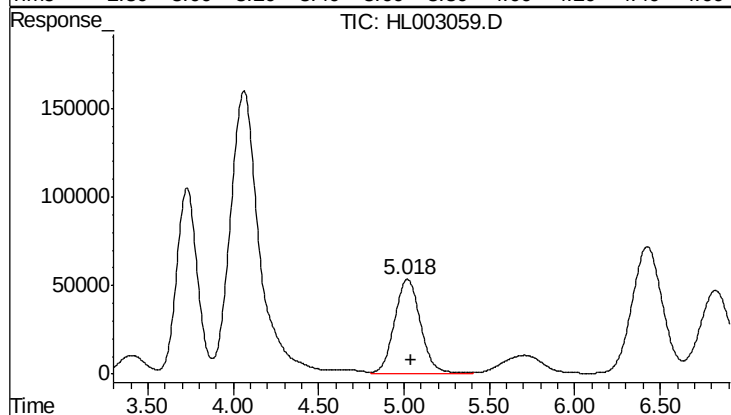


#12 Nitrobenzene
 R.T.: 5.020 min
 Delta R.T.: -0.017 min
 Response: 5634713
 Conc: 510.07 ug/L

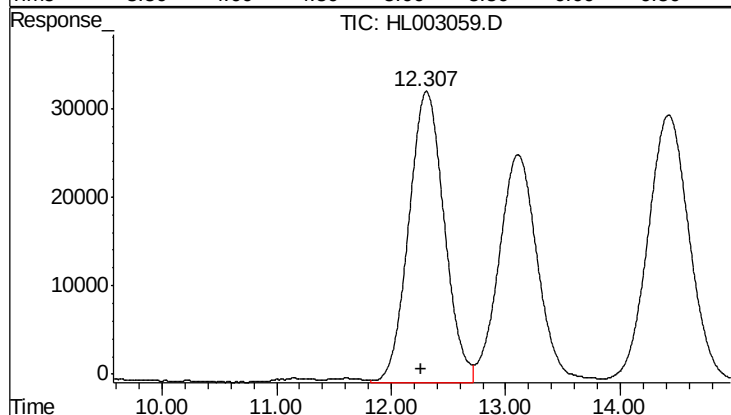

#13 2-Nitrotoluene
 R.T.: 12.309 min
 Delta R.T.: 0.044 min
 Response: 7072851
 Conc: 1017.36 ug/L

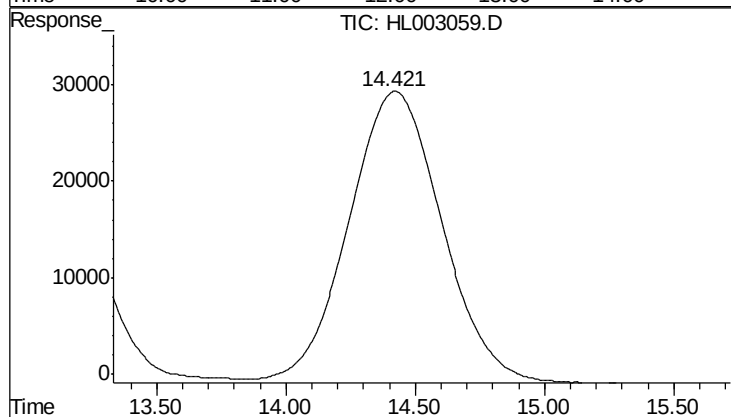

#14 3-Nitrotoluene
 R.T.: 14.423 min
 Delta R.T.: 0.057 min
 Response: 7650341
 Conc: 1016.12 ug/L

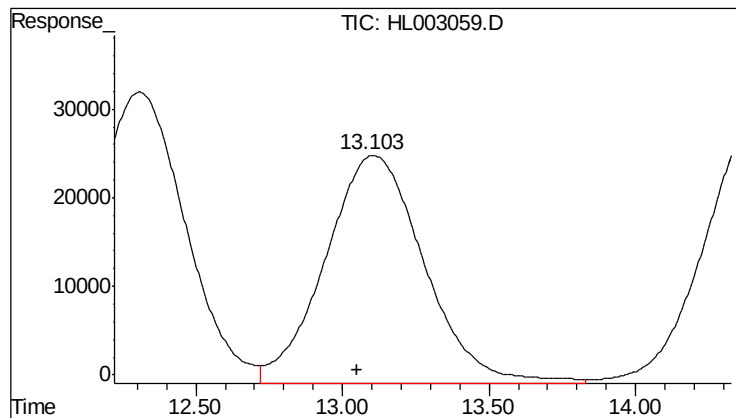

#15 4-Nitrotoluene

R.T.: 13.107 min
Delta R.T.: 0.057 min
Response: 6054550
Conc: 1027.47 ug/L