

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL052813\HL005311.D Vial: 32
Acq On : 29-May-2013, 00:58 Operator: QM
Sample : HSTDICC020 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 29 18:53 2013 Quant Results File: HL052813.RES

Instrument :
HPLC_L
LabSampleId :
HSTDICC020

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL052813.M
Title :
Last Update : Wed May 29 18:53:01 2013
Response via : Initial Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.38	82276549	19.847 ng/L
Target Compounds			
2) T Nitroglycerin	6.41	163846787	19.887 ng/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005311.D HL052813.M

Wed May 29 18:53:42 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL052813\HL005311.D Vial: 32
Acq On : 29-May-2013, 00:58 Operator: QM
Sample : HSTDICC020 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 29 18:53 2013 Quant Results File: HL052813.RES

Instrument :
HPLC_L
LabSampleId :
HSTDICC020

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL052813.M
Title :
Last Update : Wed May 29 18:53:01 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

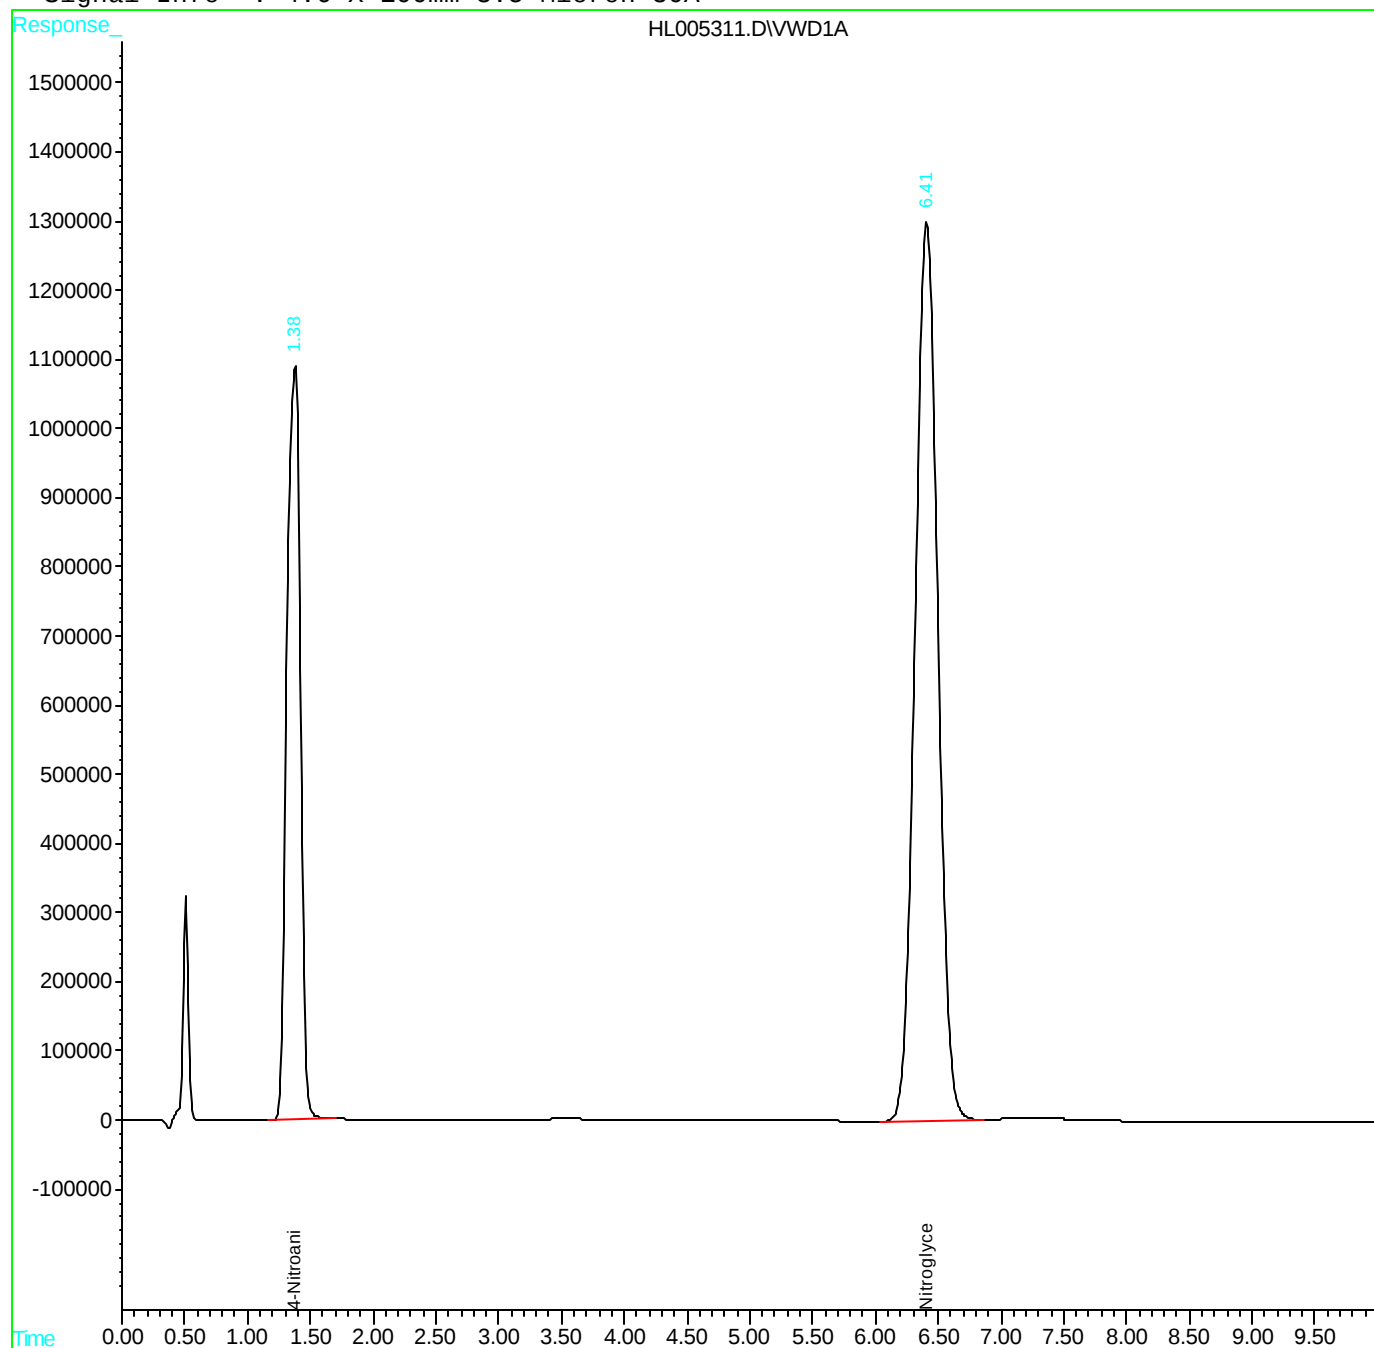


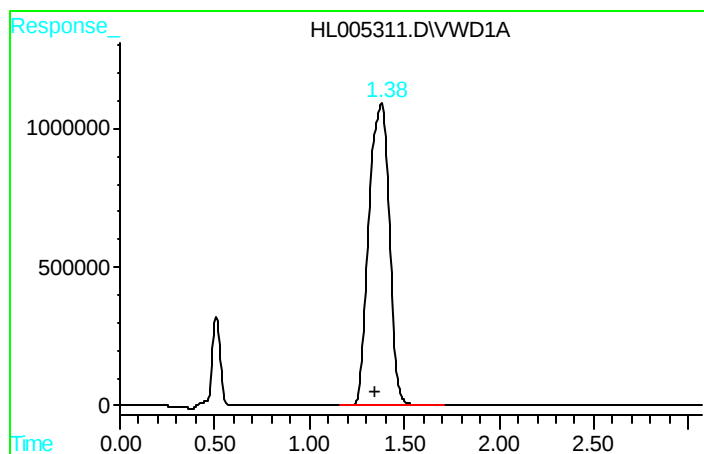

#1 4-Nitroaniline

R.T.: 1.382 min
Delta R.T.: 0.032 min
Response: 82276549
Conc: 19.85 ng/L

Instrument :
HPLC_L
LabSampleId :
HSTDIC020

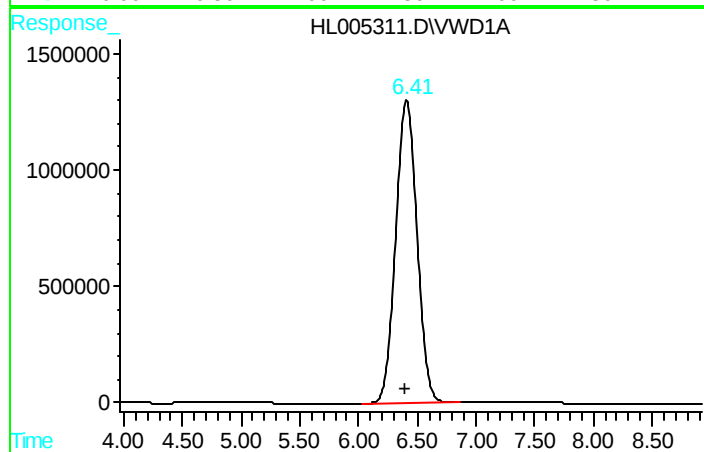

#2 Nitroglycerin

R.T.: 6.408 min
Delta R.T.: 0.018 min
Response: 163846787
Conc: 19.89 ng/L