

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL052813\HL005314.D Vial: 35
Acq On : 29-May-2013, 01:34 Operator: QM
Sample : HSTDICC001 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 29 18:55 2013 Quant Results File: HL052813.RES

Instrument :
HPLC_L
LabSampleId :
HSTDICC001

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL052813.M
Title :
Last Update : Wed May 29 18:55:17 2013
Response via : Initial Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.36	4112531	0.992 ng/L
Target Compounds			
2) T Nitroglycerin	6.42	8131986	0.987 ng/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005314.D HL052813.M

Wed May 29 18:55:47 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL052813\HL005314.D Vial: 35
Acq On : 29-May-2013, 01:34 Operator: QM
Sample : HSTDICC001 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 29 18:55 2013 Quant Results File: HL052813.RES

Instrument :
HPLC_L
LabSampleId :
HSTDICC001

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL052813.M
Title :
Last Update : Wed May 29 18:55:17 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

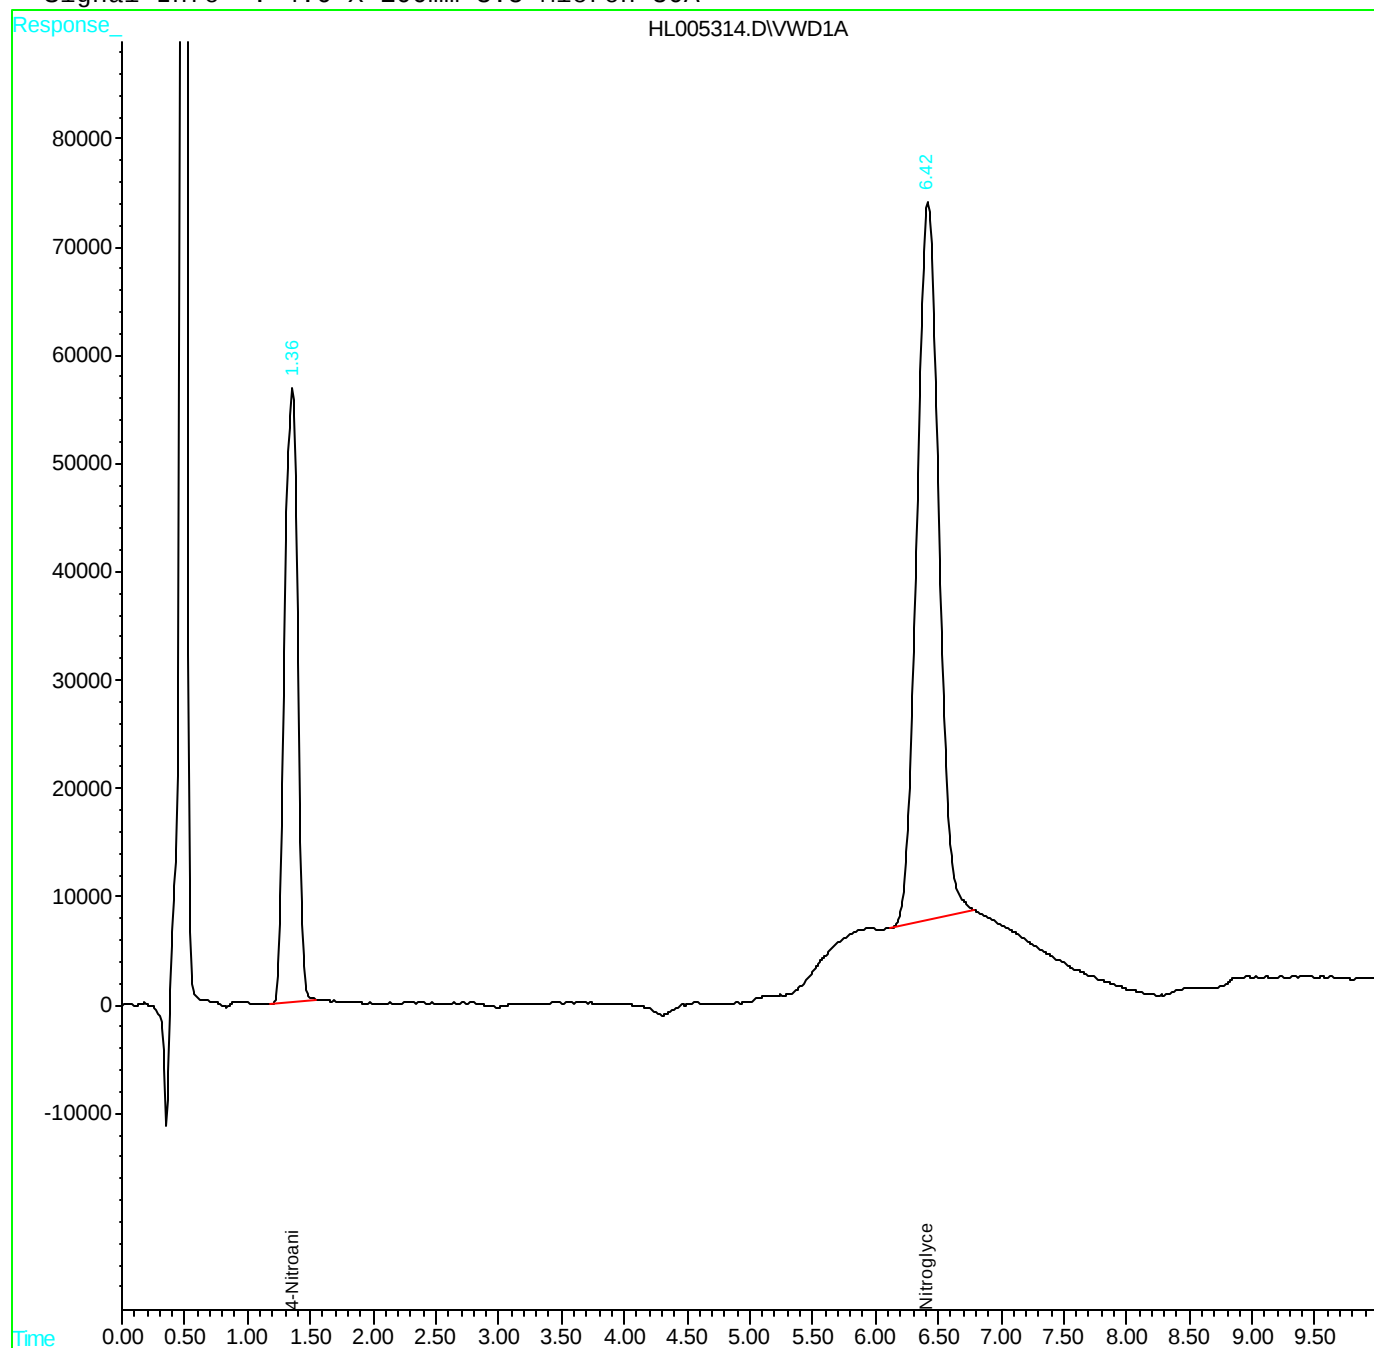


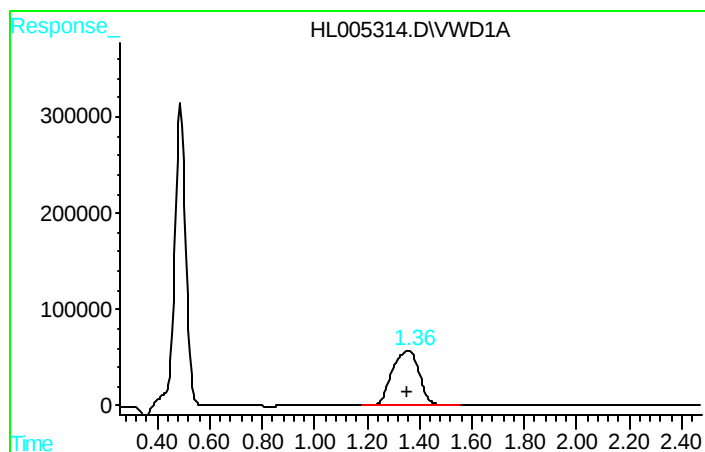

#1 4-Nitroaniline

R.T.: 1.360 min
Delta R.T.: 0.010 min
Response: 4112531
Conc: 0.99 ng/L

Instrument :
HPLC_L
LabSampleId :
HSTDIC001

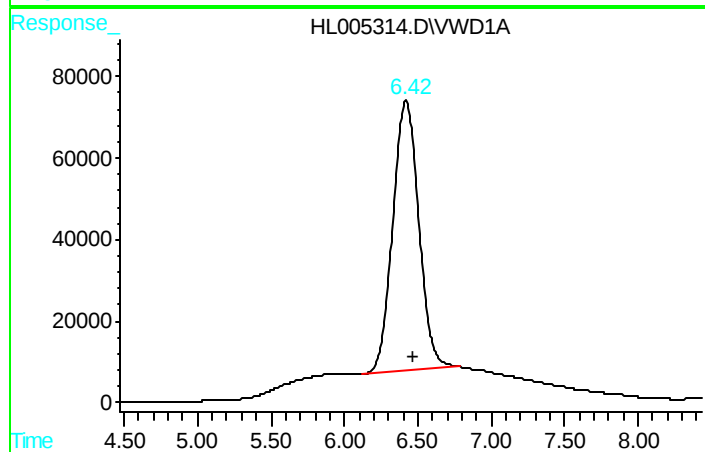

#2 Nitroglycerin

R.T.: 6.420 min
Delta R.T.: -0.050 min
Response: 8131986
Conc: 0.99 ng/L