

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL052815\
 Data File : HL006222.D
 Signal(s) : vwd1A.ch
 Acq On : 28-May-2015, 22:01
 Operator : TP/IZ
 Sample : SSTDICC2000
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 SSTDICC2000

Integration File: AUTOINT1.E
 Quant Time: May 29 08:10:08 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL052815.M
 Quant Title :
 QLast Update : Fri May 29 08:09:21 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.408	25079536	1891.604 ug/L
Target Compounds			
2) T HMX	1.375	11221185	1928.794 ug/L
3) T RDX	2.408	25079536	1898.004 ug/L
4) T 1,3,5-Trinitrobenzene	3.879	29284596	1904.221 ug/L
5) T 1,3-Dinitrobenzene	5.162	43658562	1918.890 ng/ml
6) T 3,5-Dinitroaniline	6.065	33787700	1915.607 ug/L
7) T Nitrobenzene	6.664	26019974	1913.668 ug/L
8) T Tetryl	8.979	20889204	1878.713 ug/L
9) T 2,4,6-Trinitrotoluene	9.402	27681695	1774.847 ug/L
10) T 2-Amino-4,6-dinitroto...	10.918	26953610	1885.579 ug/L
11) T 4-Amino-2,6-dinitroto...	11.507	18246589	1880.394 ug/L
12) T 2,4-Dinitrotoluene	12.118	40066464	1973.195 ug/L
13) T 2,6-Dinitrotoluene	12.528	20879404	1818.296 ug/L
14) T 2-Nitrotoluene	16.943	48293994	1797.864 ug/L
15) T 4-Nitrotoluene	18.407	39021272	1996.301 ug/L
16) T 3-Nitrotoluene	19.922	55923172	2113.362 ug/L
17) T PETN	20.458	21684685	1787.254 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL052815\
Data File : HL006222.D
Signal(s) : vwd1A.ch
Acq On : 28-May-2015, 22:01
Operator : TP/IZ
Sample : SSTDICC2000
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

Integration File: AUTOINT1.E
Quant Time: May 29 08:10:08 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL052815.M
Quant Title :
QLast Update : Fri May 29 08:09:21 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

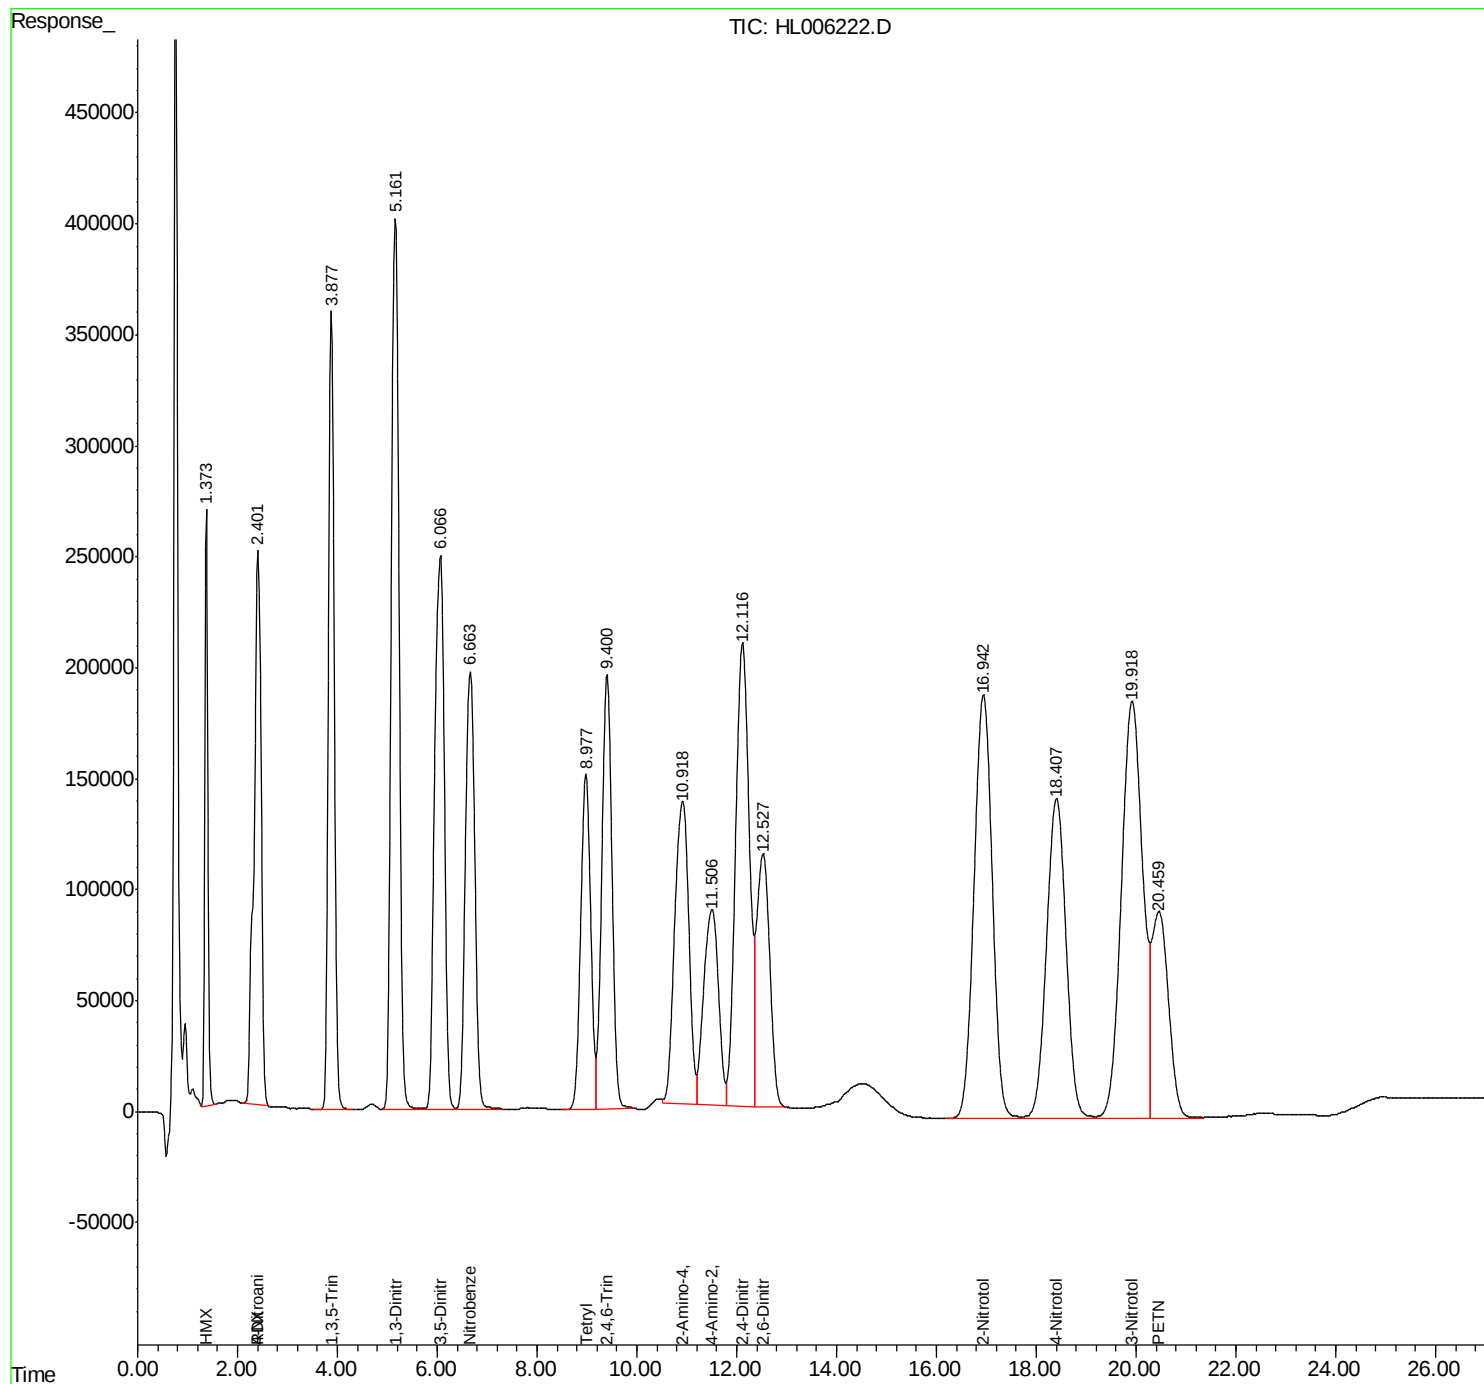


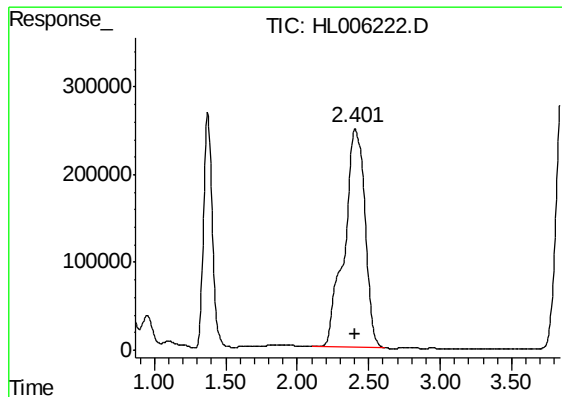

#1 4-Nitroaniline


R.T.: 2.408 min
Delta R.T.: 0.007 min
Response: 25079536
Conc: 1891.60 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

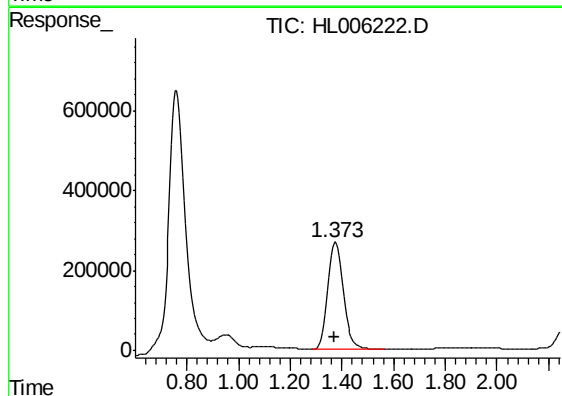


#2 HMX

R.T.: 1.375 min
Delta R.T.: 0.002 min
Response: 11221185
Conc: 1928.79 ug/L

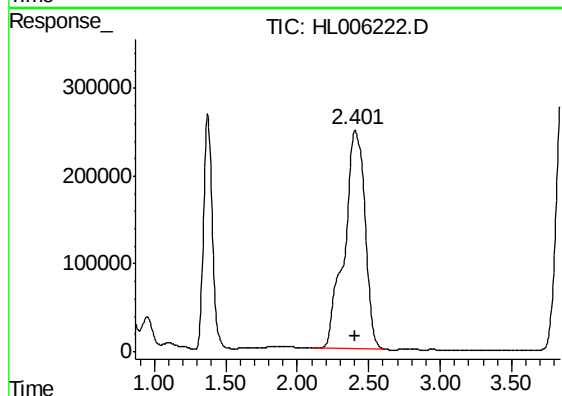


#3 RDX

R.T.: 2.408 min
Delta R.T.: 0.007 min
Response: 25079536
Conc: 1898.00 ug/L

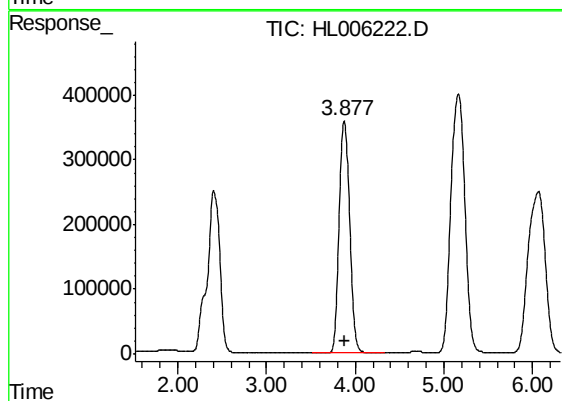

#4 1,3,5-Trinitrobenzene


R.T.: 3.879 min
Delta R.T.: 0.002 min
Response: 29284596
Conc: 1904.22 ug/L

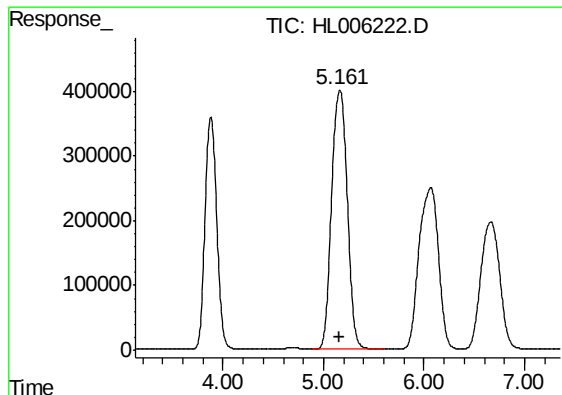

#5 1,3-Dinitrobenzene


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 43658562
Conc: 1918.89 ng/ml

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

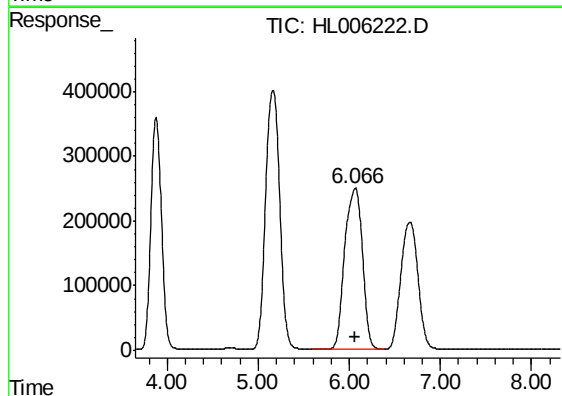


#6 3,5-Dinitroaniline

R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 33787700
Conc: 1915.61 ug/L

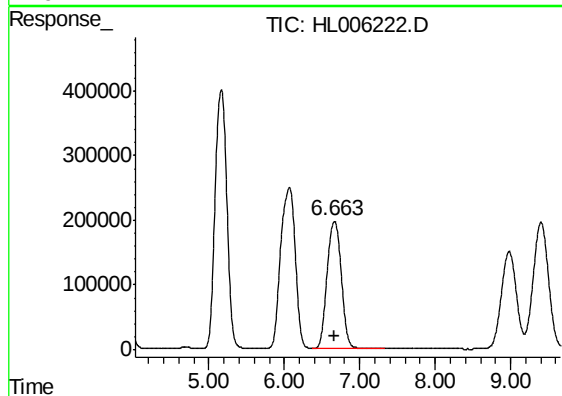


#7 Nitrobenzene

R.T.: 6.664 min
Delta R.T.: 0.001 min
Response: 26019974
Conc: 1913.67 ug/L

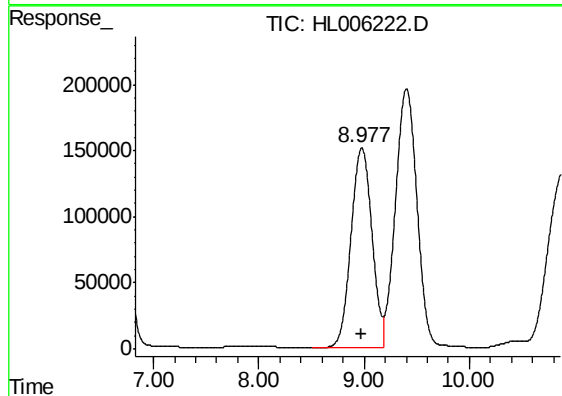

#8 Tetryl


R.T.: 8.979 min
Delta R.T.: 0.002 min
Response: 20889204
Conc: 1878.71 ug/L

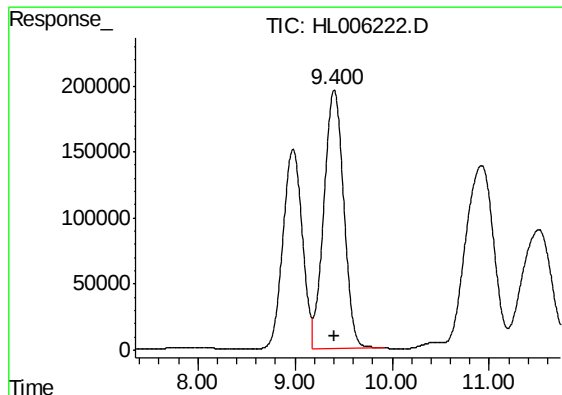

#9 2,4,6-Trinitrotoluene


R.T.: 9.402 min
Delta R.T.: 0.002 min
Response: 27681695
Conc: 1774.85 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

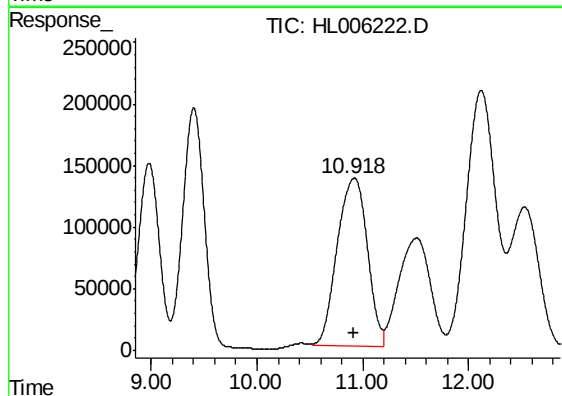


#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.918 min
Delta R.T.: 0.001 min
Response: 26953610
Conc: 1885.58 ug/L

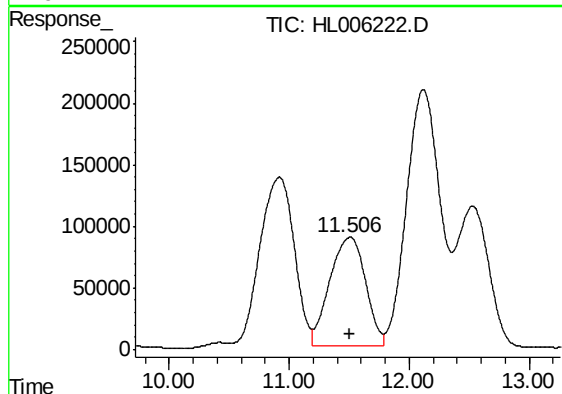


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.507 min
Delta R.T.: 0.000 min
Response: 18246589
Conc: 1880.39 ug/L

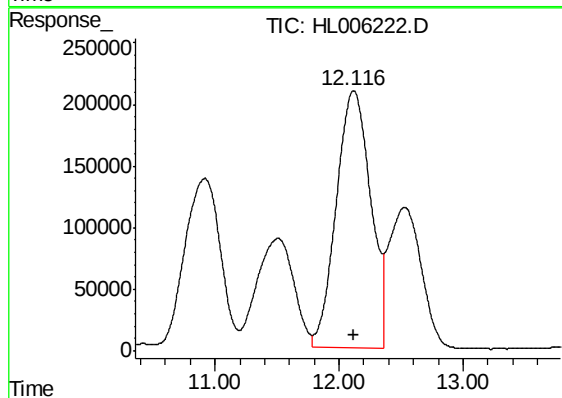

#12 2,4-Dinitrotoluene


R.T.: 12.118 min
Delta R.T.: 0.002 min
Response: 40066464
Conc: 1973.20 ug/L

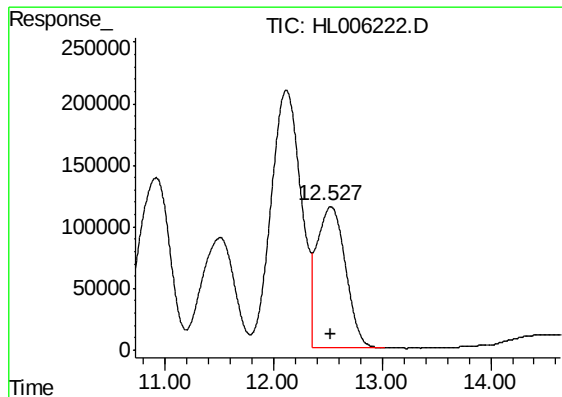

#13 2,6-Dinitrotoluene


R.T.: 12.528 min
Delta R.T.: 0.000 min
Response: 20879404
Conc: 1818.30 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

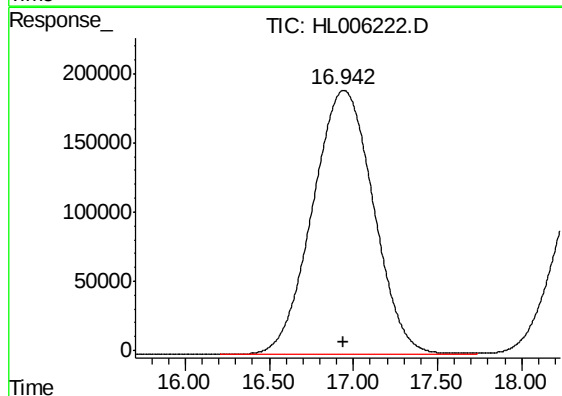


#14 2-Nitrotoluene

R.T.: 16.943 min
Delta R.T.: 0.002 min
Response: 48293994
Conc: 1797.86 ug/L

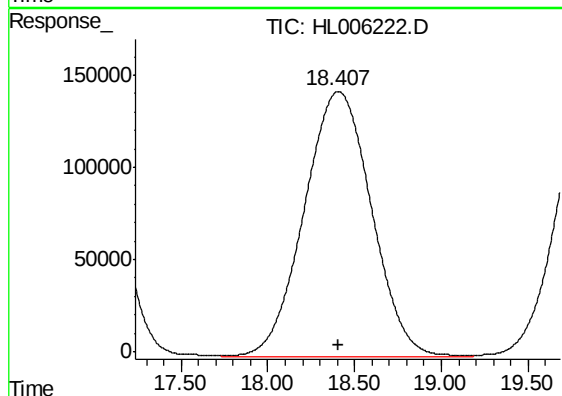


#15 4-Nitrotoluene

R.T.: 18.407 min
Delta R.T.: 0.000 min
Response: 39021272
Conc: 1996.30 ug/L

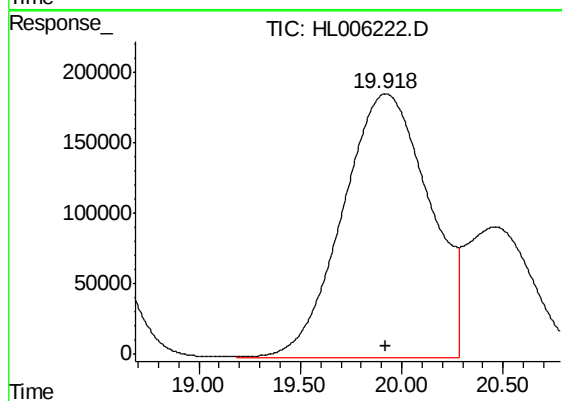

#16 3-Nitrotoluene

R.T.: 19.922 min
Delta R.T.: 0.003 min
Response: 55923172
Conc: 2113.36 ug/L

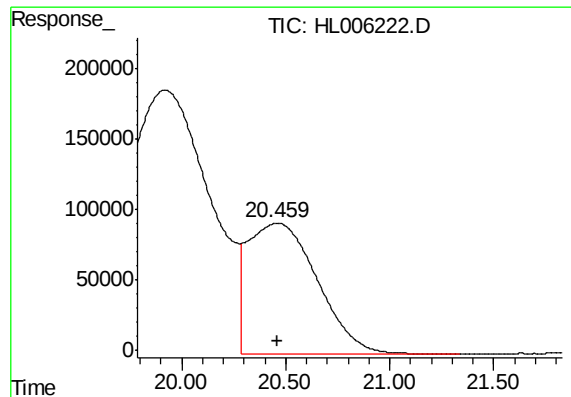

#17 PETN

R.T.: 20.458 min
Delta R.T.: 0.000 min
Response: 21684685
Conc: 1787.25 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000