

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL052815\
 Data File : HL006219.D
 Signal(s) : vwd1A.ch
 Acq On : 28-May-2015, 20:36
 Operator : TP/IZ
 Sample : SSTDICCC0500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 SSTDICCC0500

Integration File: AUTOINT1.E
 Quant Time: May 29 04:15:57 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL052815.M
 Quant Title :
 QLast Update : Fri May 29 04:15:50 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.393	6352871	936.007 ug/L
Target Compounds			
2) T HMX	1.365	2707350	449.958 ug/L
3) T RDX	2.393	6352871	689.262 ug/L
4) T 1,3,5-Trinitrobenzene	3.859	7293392	457.622 ug/L
5) T 1,3-Dinitrobenzene	5.123	10819314	461.255 ng/ml
6) T 3,5-Dinitroaniline	5.974	8378433	460.073 ug/L
7) T Nitrobenzene	6.611	6340060	476.137 ug/L
8) T Tetryl	8.863	5304806	456.709 ug/L
9) T 2,4,6-Trinitrotoluene	9.318	7799526	519.582 ug/L
10) T 2-Amino-4,6-dinitroto...	10.738	7018451	474.496 ug/L
11) T 4-Amino-2,6-dinitroto...	11.309	4493516	451.157 ug/L
12) T 2,4-Dinitrotoluene	11.983	9727453	467.480 ug/L
13) T 2,6-Dinitrotoluene	12.402	5514840	486.599 ug/L
14) T 2-Nitrotoluene	17.313	12546080	513.707 ug/L
15) T 4-Nitrotoluene	18.883	10368186	510.620 ug/L
16) T 3-Nitrotoluene	20.493	13636331	496.895 ug/L
17) T PETN	21.203	5796424	446.462 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL052815\
Data File : HL006219.D
Signal(s) : vwd1A.ch
Acq On : 28-May-2015, 20:36
Operator : TP/IZ
Sample : SSTDICCC0500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SSTDICCC0500

Integration File: AUTOINT1.E
Quant Time: May 29 04:15:57 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL052815.M
Quant Title :
QLast Update : Fri May 29 04:15:50 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

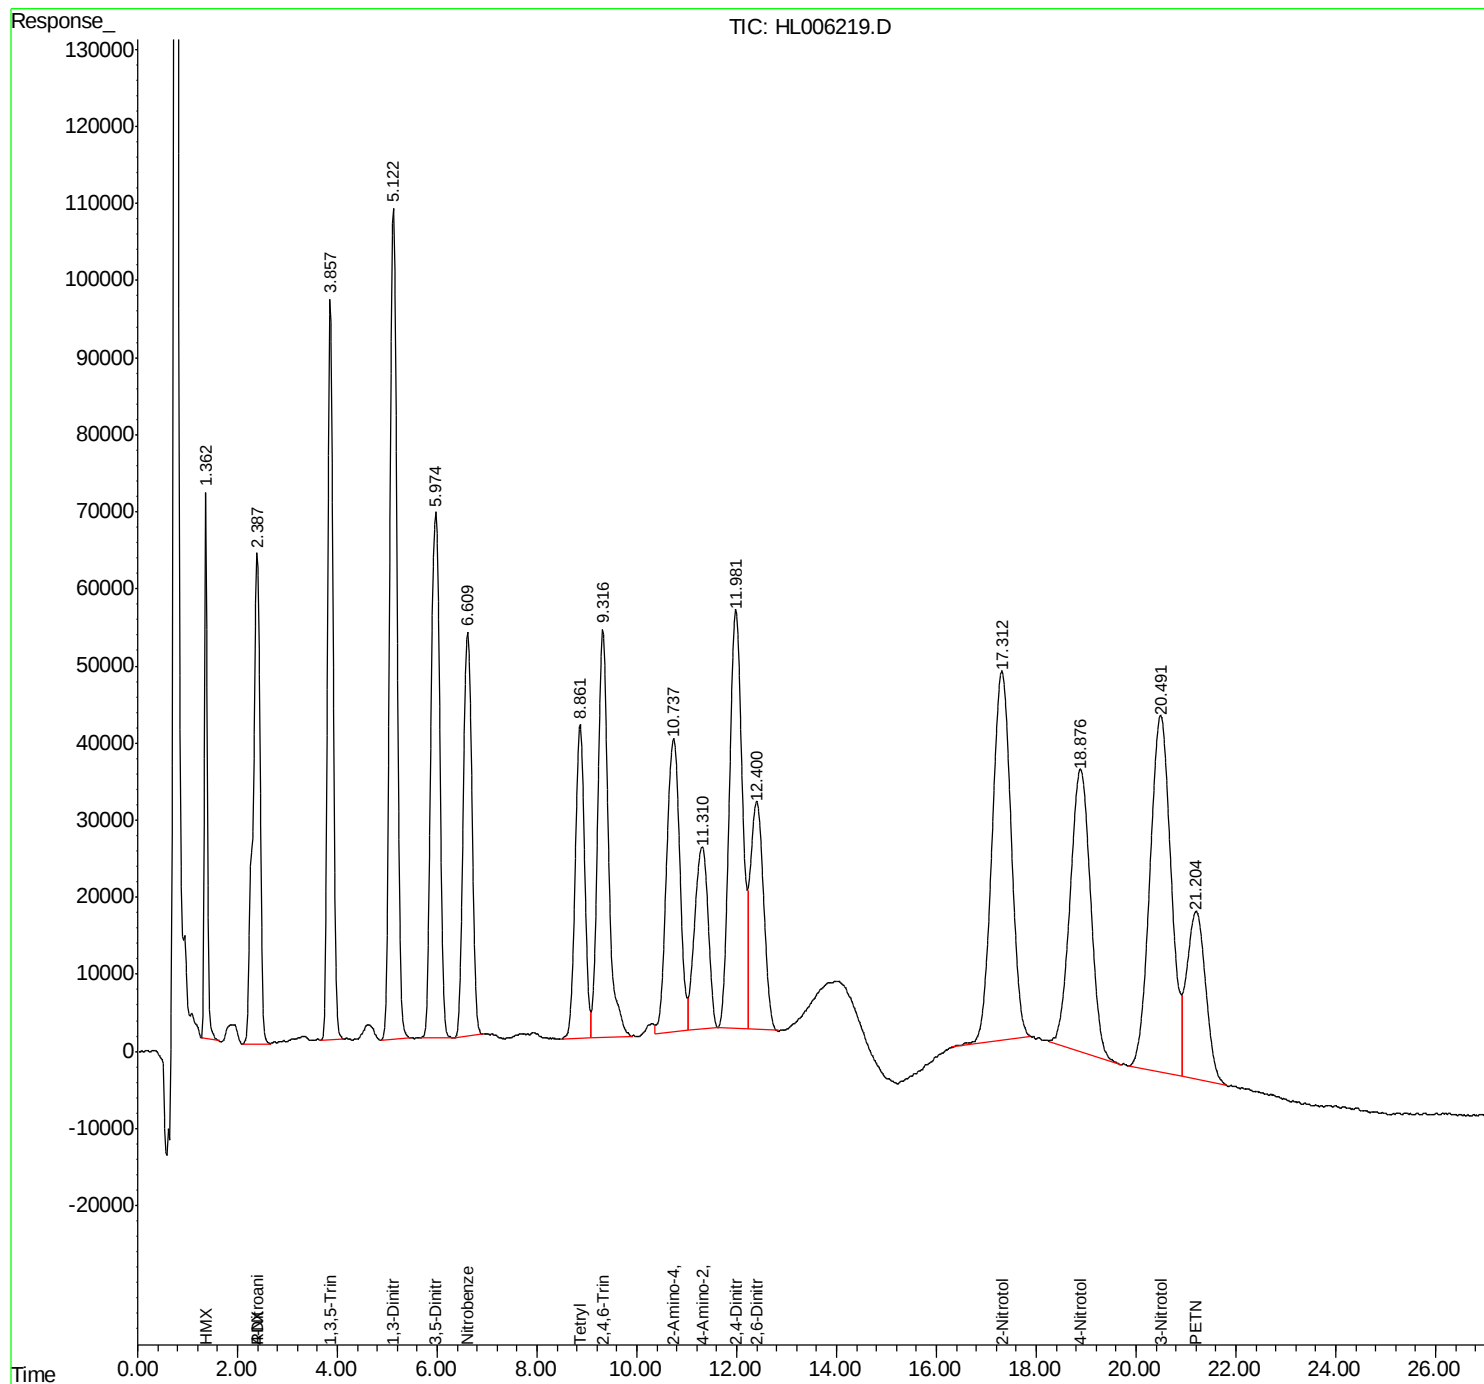


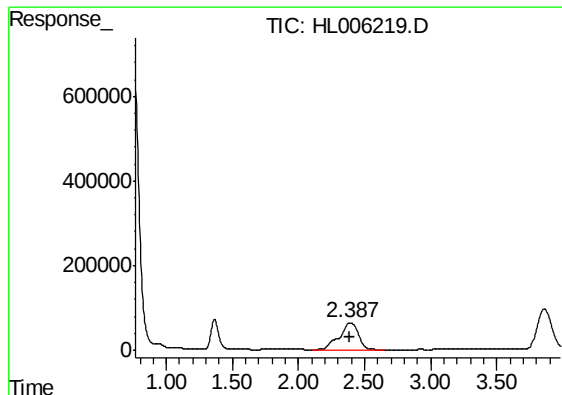

#1 4-Nitroaniline


R.T.: 2.393 min
Delta R.T.: 0.000 min
Response: 6352871
Conc: 936.01 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICCC0500

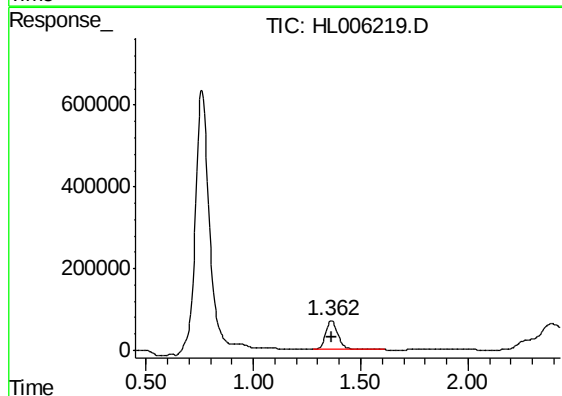


#2 HMX

R.T.: 1.365 min
Delta R.T.: 0.000 min
Response: 2707350
Conc: 449.96 ug/L

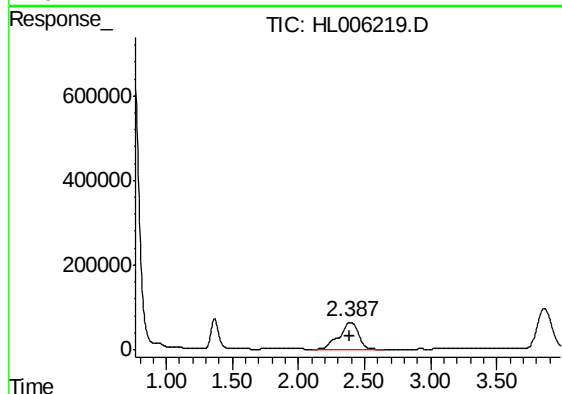


#3 RDX

R.T.: 2.393 min
Delta R.T.: 0.000 min
Response: 6352871
Conc: 689.26 ug/L

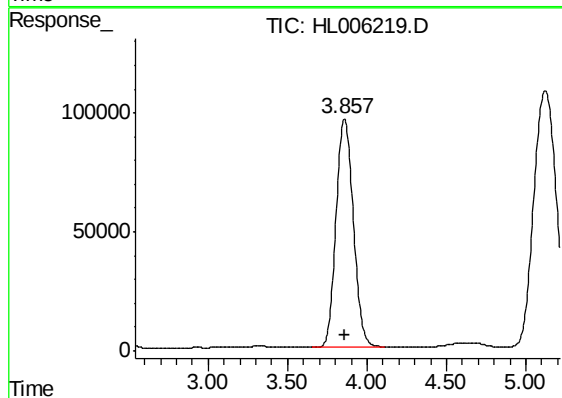

#4 1,3,5-Trinitrobenzene


R.T.: 3.859 min
Delta R.T.: 0.000 min
Response: 7293392
Conc: 457.62 ug/L

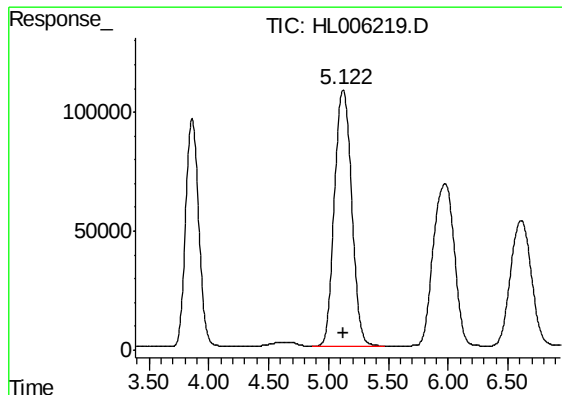

#5 1,3-Dinitrobenzene


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 10819314
Conc: 461.26 ng/ml

Instrument :
HPLC_L
ClientSampleId :
SSTDICCC0500

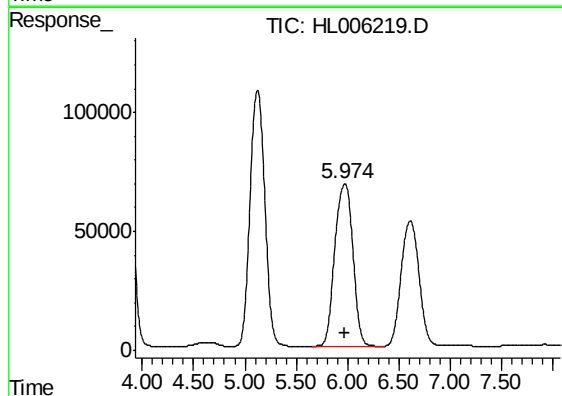


#6 3,5-Dinitroaniline

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 8378433
Conc: 460.07 ug/L

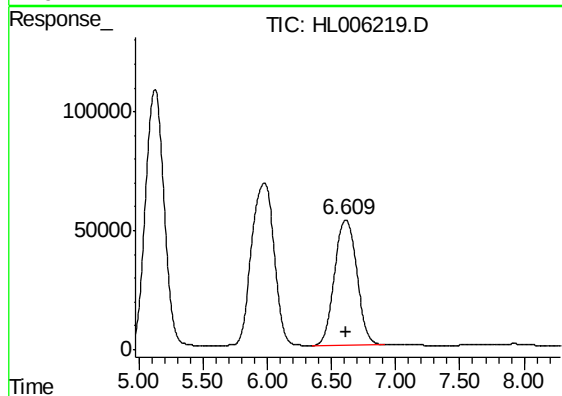


#7 Nitrobenzene

R.T.: 6.611 min
Delta R.T.: 0.000 min
Response: 6340060
Conc: 476.14 ug/L

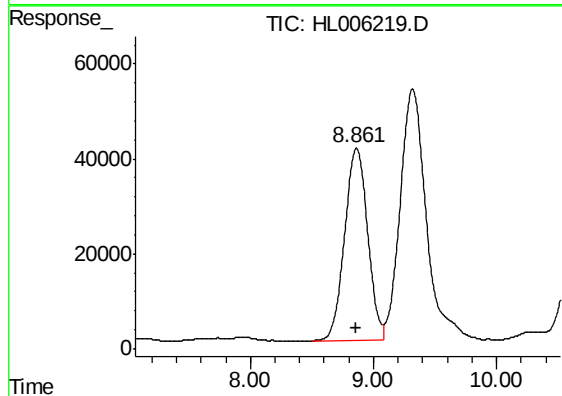

#8 Tetryl


R.T.: 8.863 min
Delta R.T.: 0.000 min
Response: 5304806
Conc: 456.71 ug/L

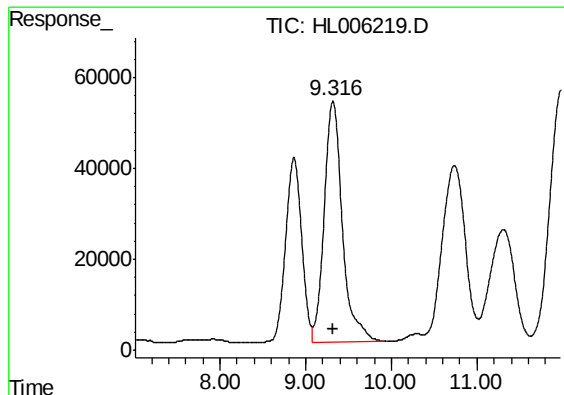

#9 2,4,6-Trinitrotoluene


R.T.: 9.318 min
Delta R.T.: 0.000 min
Response: 7799526
Conc: 519.58 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICCC0500

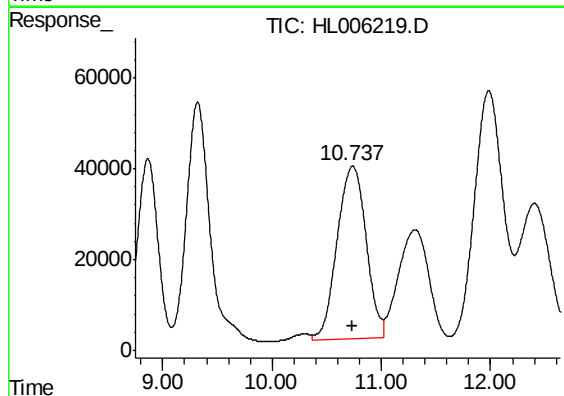


#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.738 min
Delta R.T.: 0.000 min
Response: 7018451
Conc: 474.50 ug/L

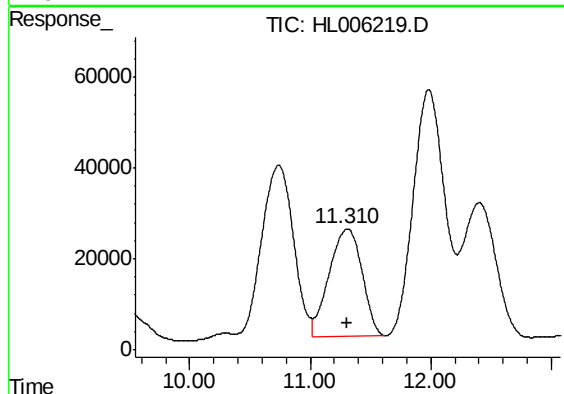


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.309 min
Delta R.T.: 0.000 min
Response: 4493516
Conc: 451.16 ug/L

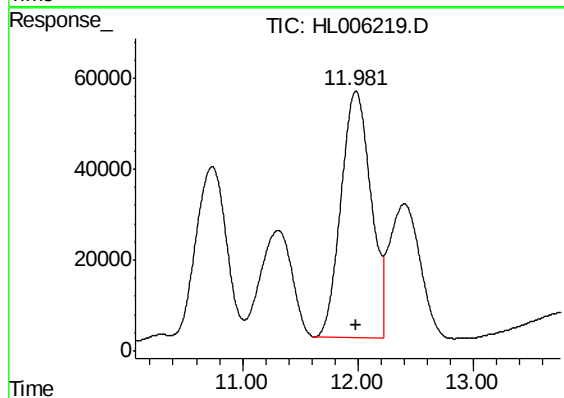

#12 2,4-Dinitrotoluene


R.T.: 11.983 min
Delta R.T.: 0.000 min
Response: 9727453
Conc: 467.48 ug/L

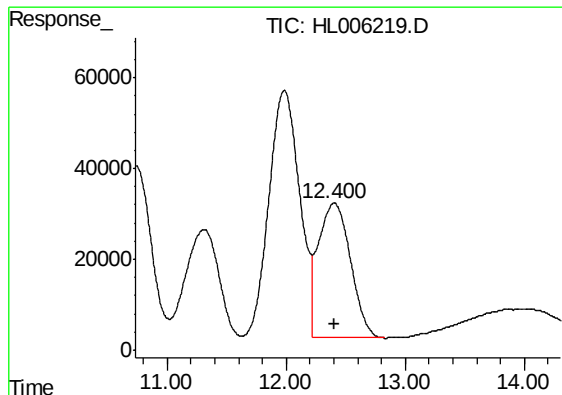

#13 2,6-Dinitrotoluene


R.T.: 12.402 min
Delta R.T.: 0.000 min
Response: 5514840
Conc: 486.60 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICCC0500

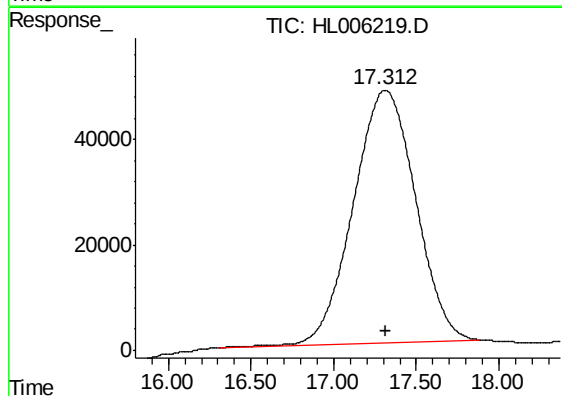


#14 2-Nitrotoluene

R.T.: 17.313 min
Delta R.T.: 0.000 min
Response: 12546080
Conc: 513.71 ug/L

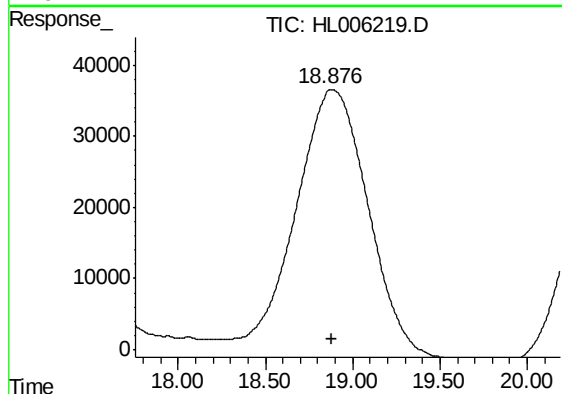


#15 4-Nitrotoluene

R.T.: 18.883 min
Delta R.T.: 0.000 min
Response: 10368186
Conc: 510.62 ug/L

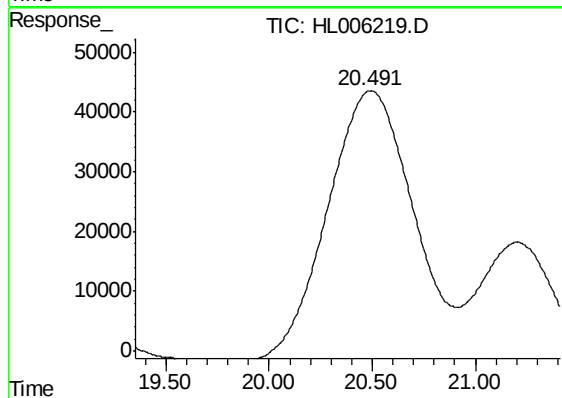

#16 3-Nitrotoluene

R.T.: 20.493 min
Delta R.T.: 0.000 min
Response: 13636331
Conc: 496.89 ug/L

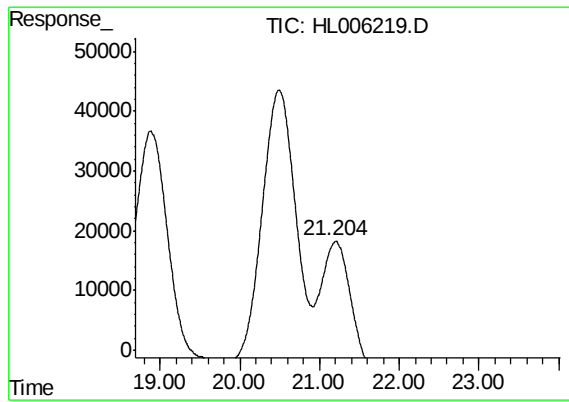

#17 PETN

R.T.: 21.203 min
Delta R.T.: 0.000 min
Response: 5796424
Conc: 446.46 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICCC0500