

Data File : Z:\HPCHEM1\HPLC\_L\DATA\HL052913\HL005322.D Vial: 6  
Acq On : 29-May-2013, 12:49 Operator: QM  
Sample : LOQ-S-NG-1PPM Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: May 29 19:23 2013 Quant Results File: HL052813.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
LOQ-S-NG-1PPM

Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL052813.M  
Title :  
Last Update : Wed May 29 18:55:17 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units |
|-----------------------------|------|----------|------------|
| -----                       |      |          |            |
| System Monitoring Compounds |      |          |            |
| 1) S 4-Nitroaniline         | 1.38 | 632692   | 0.153 ng/L |
| Target Compounds            |      |          |            |
| 2) T Nitroglycerin          | 6.48 | 9426469  | 1.144 ng/L |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005322.D HL052813.M

Wed May 29 19:23:06 2013

RPT1


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_L\DATA\HL052913\HL005322.D Vial: 6  
Acq On : 29-May-2013, 12:49 Operator: QM  
Sample : LOQ-S-NG-1PPM Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: May 29 19:23 2013 Quant Results File: HL052813.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
LOQ-S-NG-1PPM

Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL052813.M  
Title :  
Last Update : Wed May 29 18:55:17 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

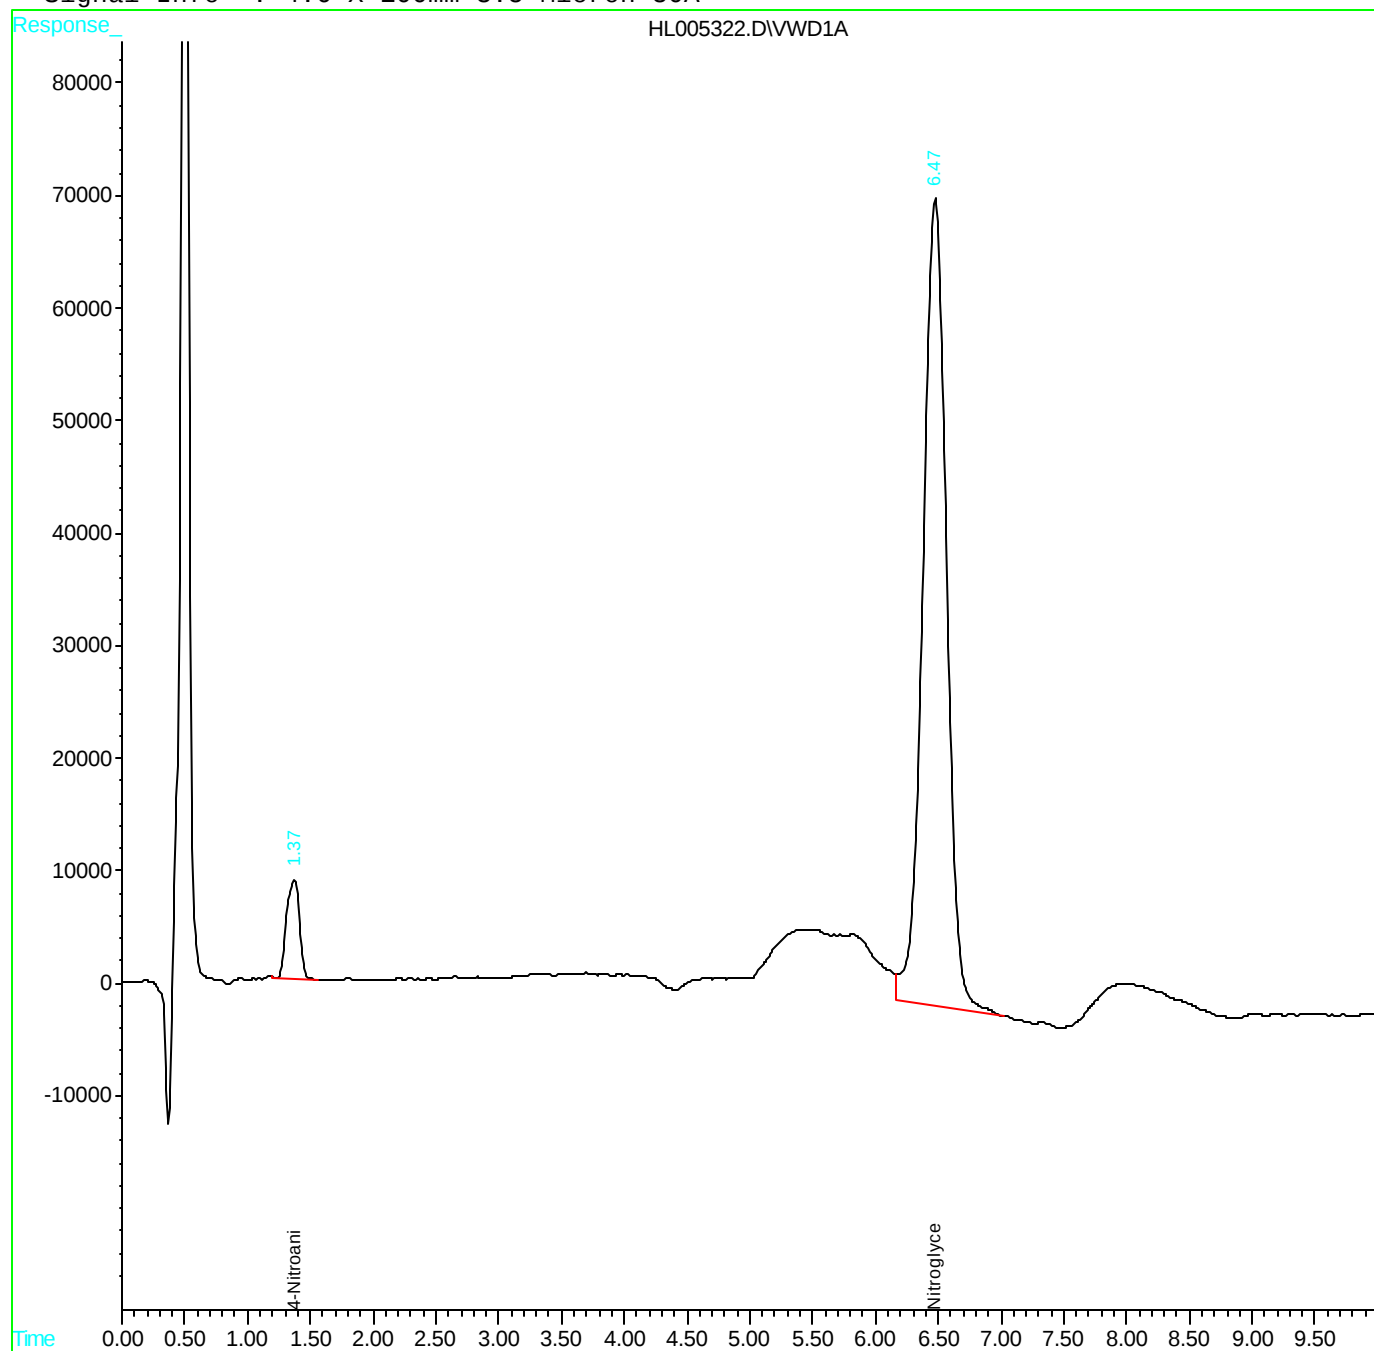


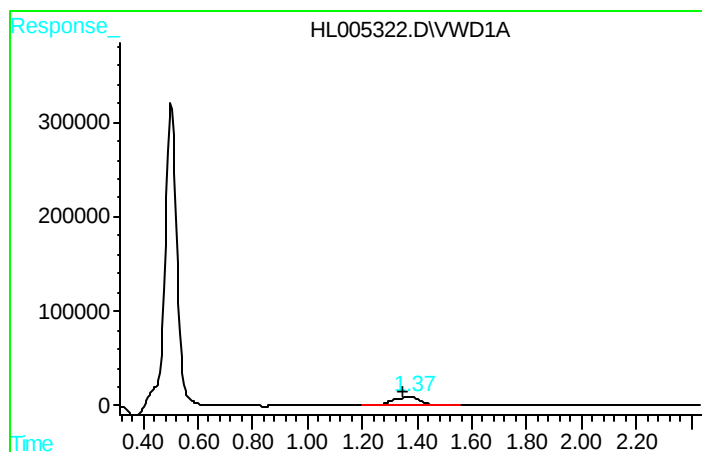

#1 4-Nitroaniline

R.T.: 1.375 min  
Delta R.T.: 0.025 min  
Response: 632692  
Conc: 0.15 ng/L

Instrument :  
HPLC\_L  
ClientSampleId :  
LOQ-S-NG-1PPM

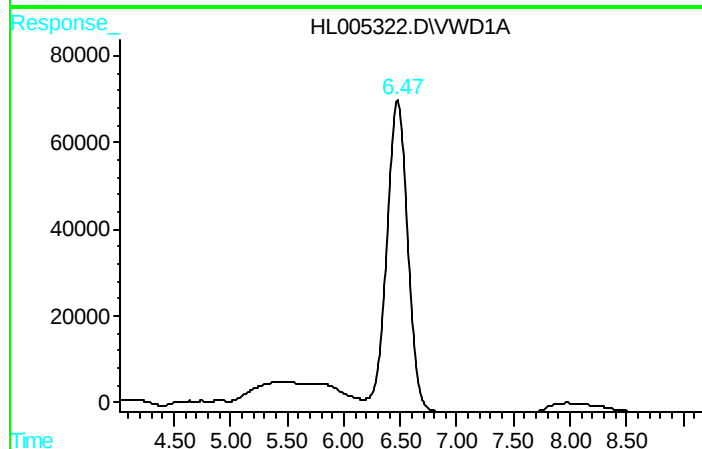

#2 Nitroglycerin

R.T.: 6.476 min  
Delta R.T.: 0.006 min  
Response: 9426469  
Conc: 1.14 ng/L