



Data Path : Z:\HPCHEM1\HPLC_L\Data\HL053012\
Data File : HL003101.D
Signal(s) : VWD1A.CH
Acq On : 30-May-2012, 13:27
Operator : HLM
Sample : 8330-4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
8330-4

Integration File: events.e
Quant Time: Jun 14 02:26:25 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL053012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu May 31 11:09:51 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

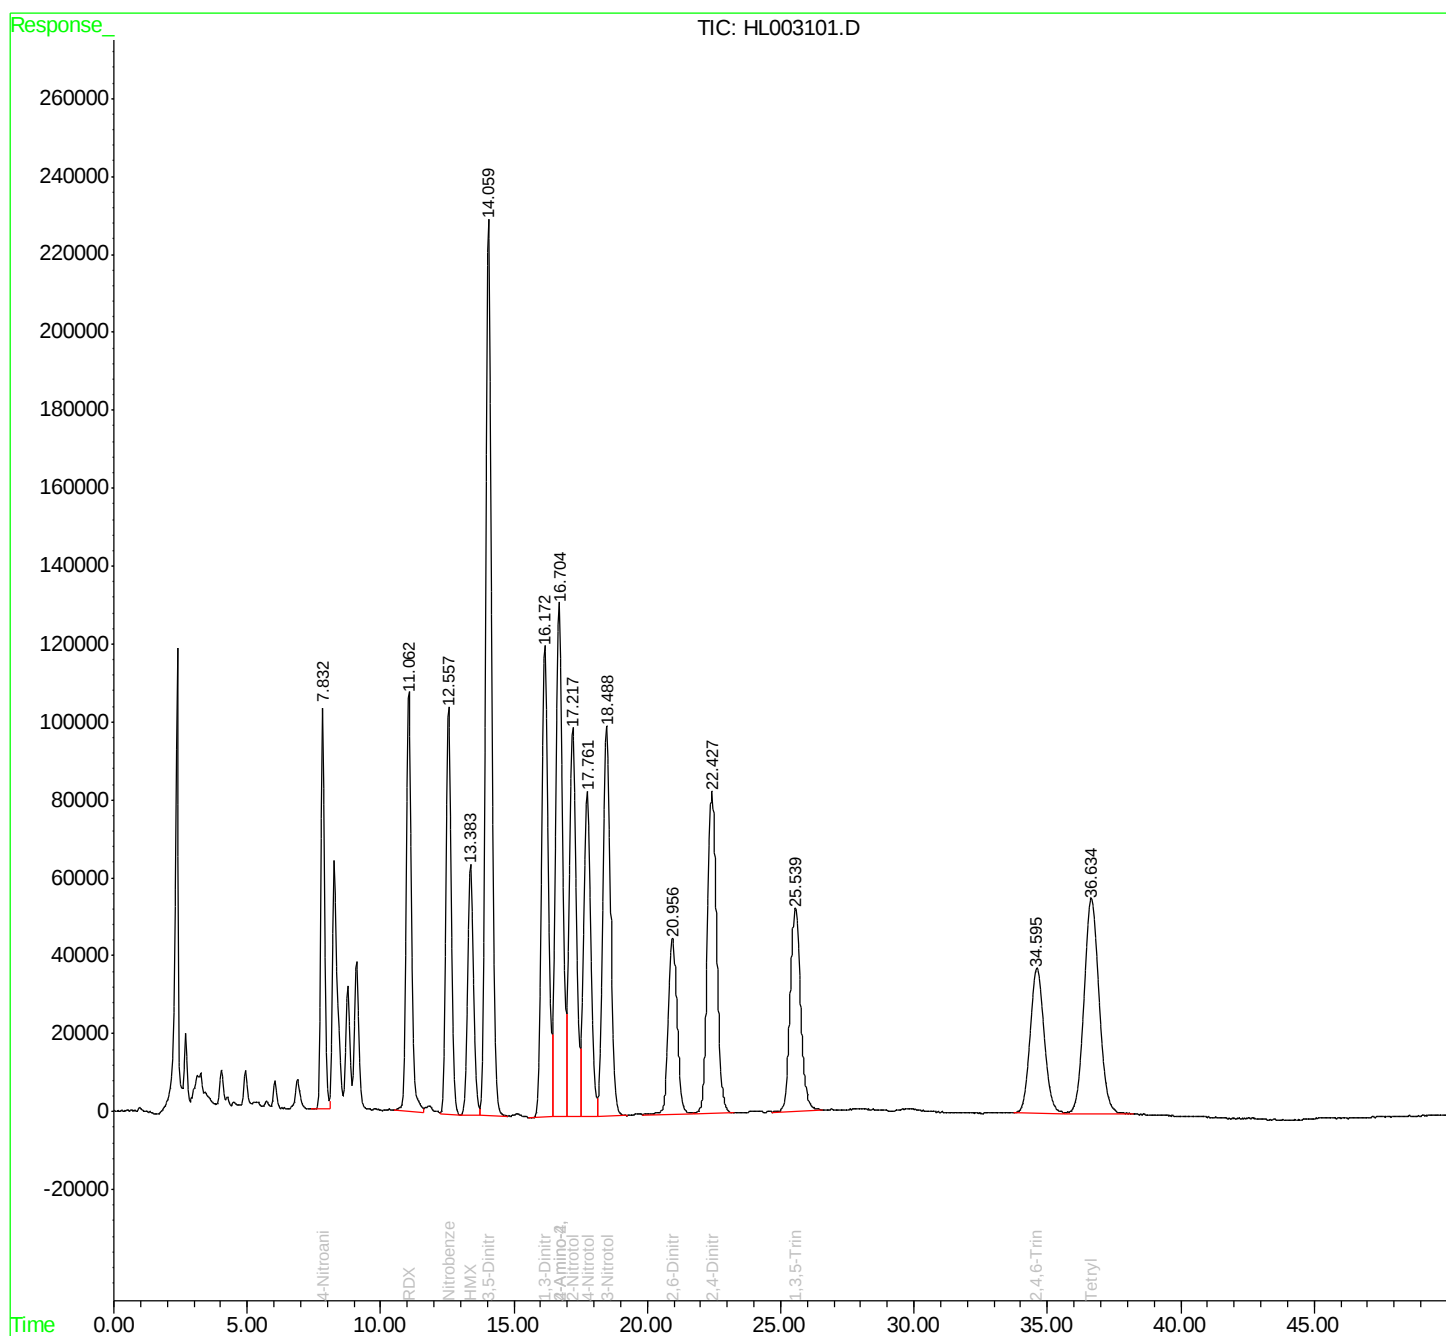


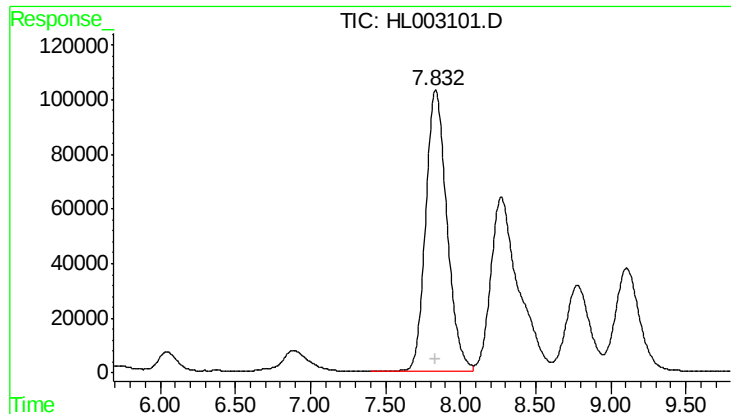

#1 4-Nitroaniline


R.T.: 7.835 min
Delta R.T.: 0.000 min
Response: 10105872
Conc: 1000.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-4

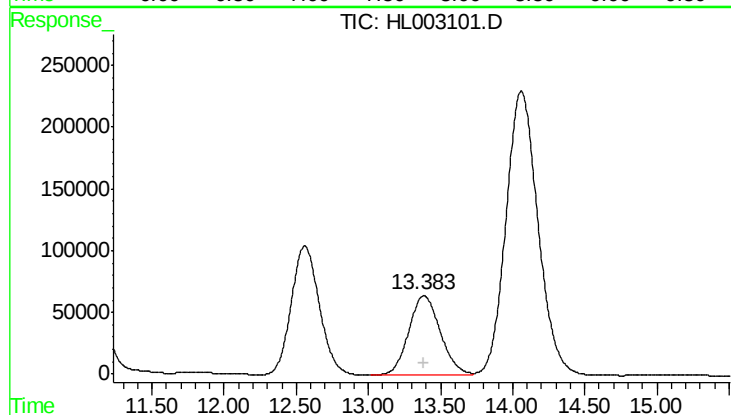


#2 HMX

R.T.: 13.386 min
Delta R.T.: 0.000 min
Response: 9856416
Conc: 1000.00 ug/L

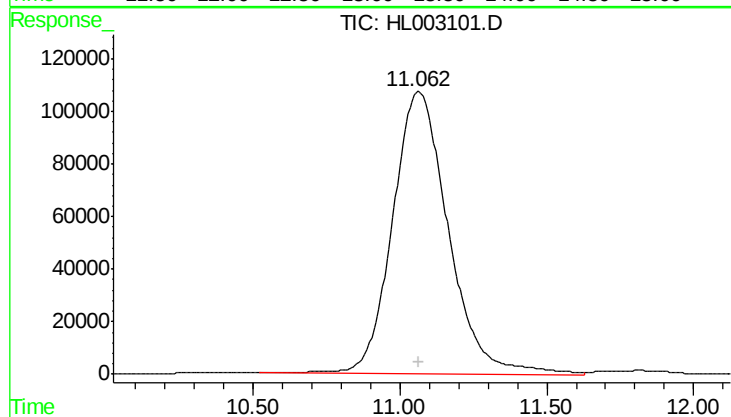


#3 RDX

R.T.: 11.064 min
Delta R.T.: 0.000 min
Response: 14264504
Conc: 1000.00 ug/L

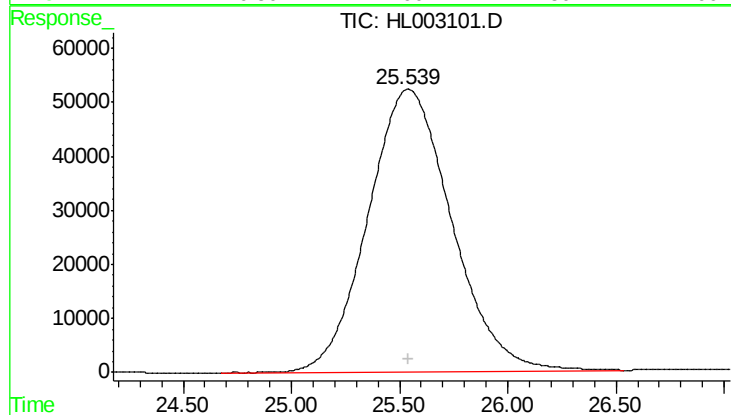

#4 1,3,5-Trinitrobenzene


R.T.: 25.541 min
Delta R.T.: 0.000 min
Response: 14137762
Conc: 500.00 ug/L

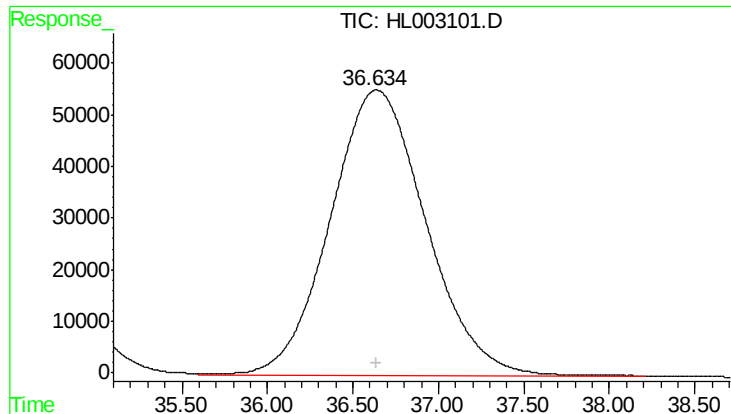

#5 Tetryl


R.T.: 36.637 min
Delta R.T.: 0.000 min
Response: 21617760
Conc: 1000.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-4

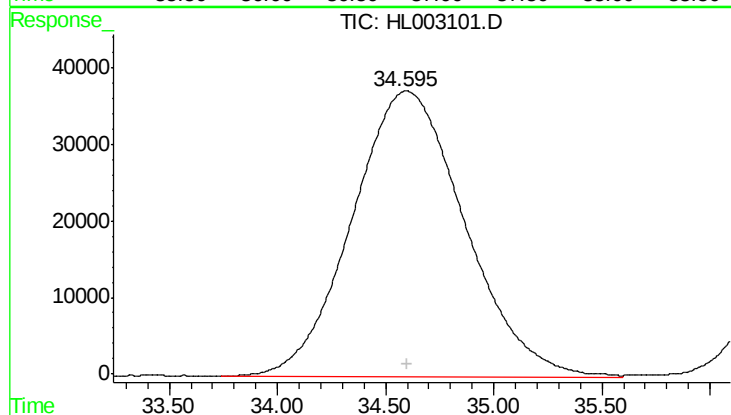


#6 2,4,6-Trinitrotoluene

R.T.: 34.597 min
Delta R.T.: 0.000 min
Response: 13570606
Conc: 500.00 ug/L

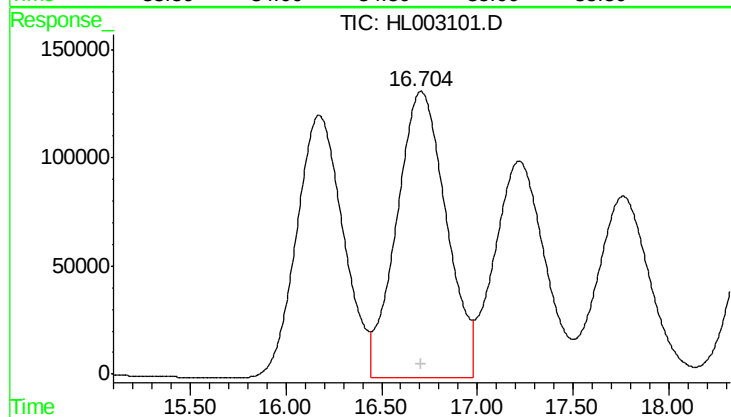


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.707 min
Delta R.T.: 0.000 min
Response: 23867035
Conc: 500.00 ug/L

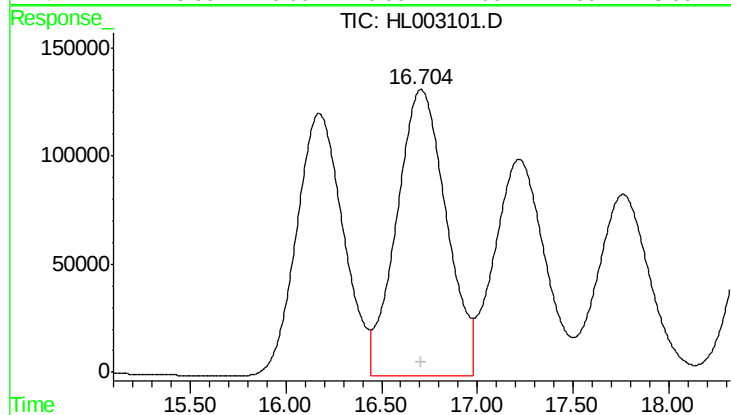

#8 4-Amino-2,6-dinitrotoluene


R.T.: 16.707 min
Delta R.T.: 0.000 min
Response: 23867035
Conc: 500.00 ug/L

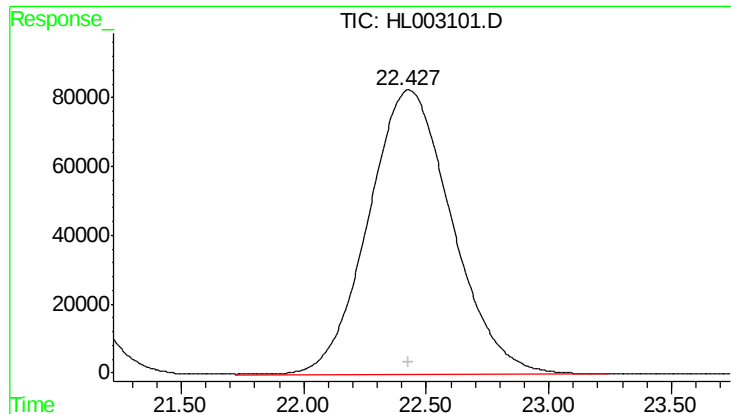

#9 2,4-Dinitrotoluene


R.T.: 22.429 min
Delta R.T.: 0.000 min
Response: 19718688
Conc: 500.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-4

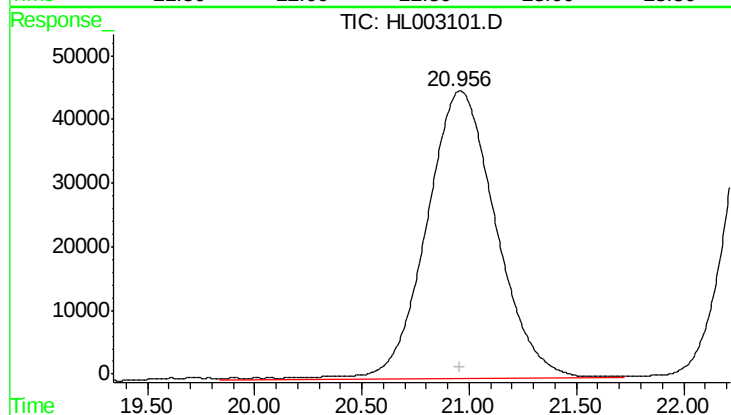


#10 2,6-Dinitrotoluene

R.T.: 20.959 min
Delta R.T.: 0.000 min
Response: 10299907
Conc: 500.00 ug/L

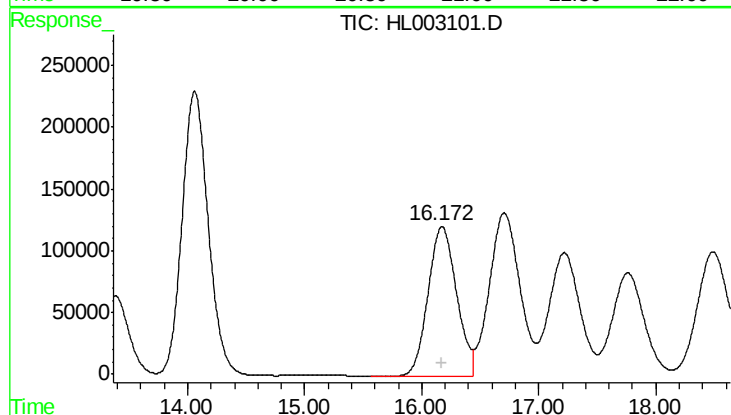


#11 1,3-Dinitrobenzene

R.T.: 16.174 min
Delta R.T.: 0.000 min
Response: 20502312
Conc: 500.00 ug/L

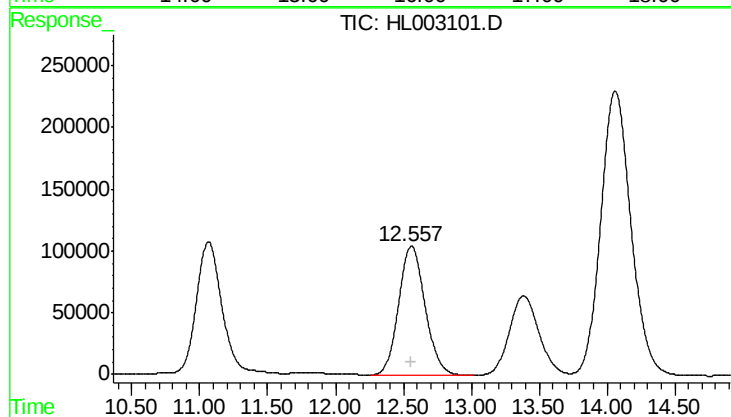

#12 Nitrobenzene


R.T.: 12.559 min
Delta R.T.: 0.000 min
Response: 14164154
Conc: 500.00 ug/L

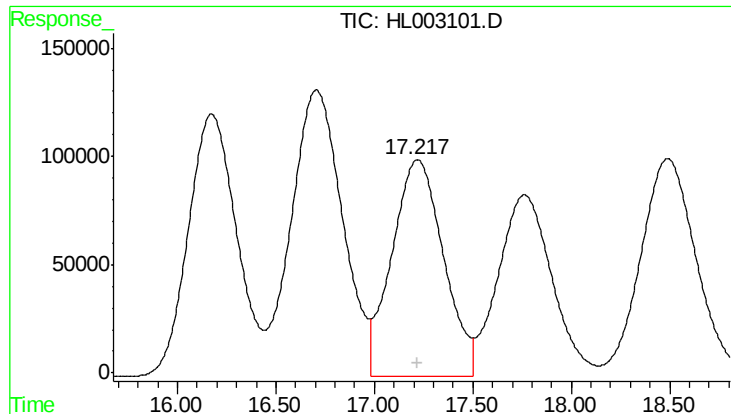

#13 2-Nitrotoluene


R.T.: 17.219 min
Delta R.T.: 0.000 min
Response: 18255253
Conc: 1000.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-4

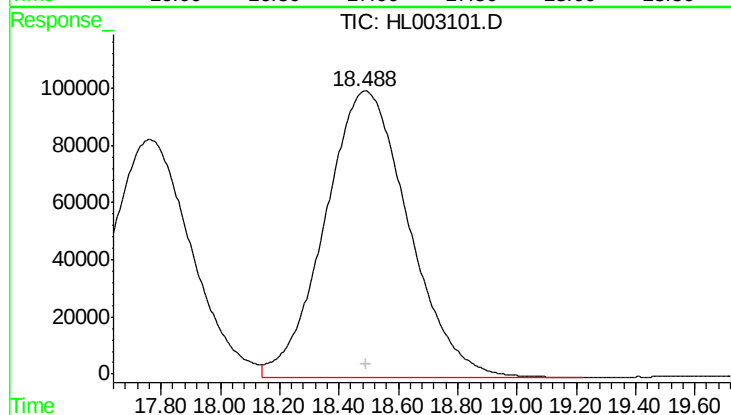


#14 3-Nitrotoluene

R.T.: 18.490 min
Delta R.T.: 0.000 min
Response: 19714175
Conc: 1000.00 ug/L

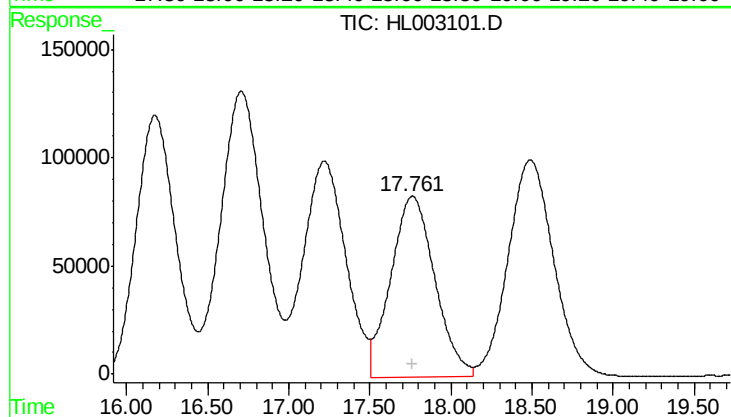

#15 4-Nitrotoluene

R.T.: 17.763 min
Delta R.T.: 0.000 min
Response: 15828931
Conc: 1000.00 ug/L

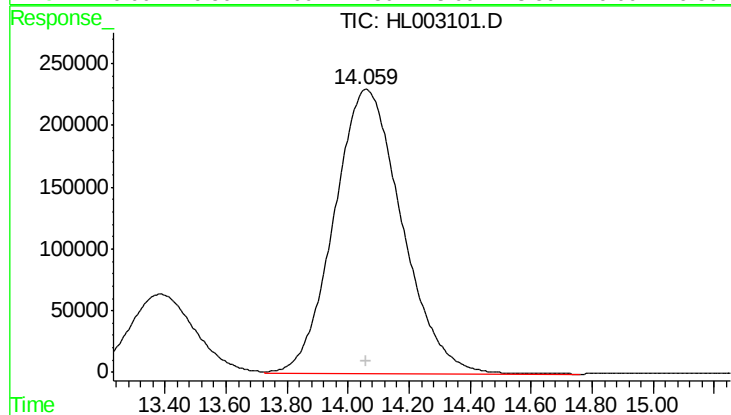

#16 3,5-Dinitroaniline

R.T.: 14.061 min
Delta R.T.: 0.000 min
Response: 35705268
Conc: 1000.00 ug/L

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL053012\
 Data File : HL003101.D
 Signal(s) : VWD1A.CH
 Acq On : 30-May-2012, 13:27
 Operator : HLM
 Sample : 8330-4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 8330-4

Integration File: events.e
 Quant Time: Jun 14 02:26:25 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL053012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Thu May 31 11:09:51 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc	Units

System Monitoring Compounds					
1) S	4-Nitroaniline	7.835	10105872	1000.000	ug/L
Target Compounds					
2) T	HMX	13.386	9856416	1000.000	ug/L
3) T	RDX	11.064	14264504	1000.000	ug/L
4) T	1,3,5-Trinitrobenzene	25.541	14137762	500.000	ug/L
5) T	Tetryl	36.637	21617760	1000.000	ug/L
6) T	2,4,6-Trinitrotoluene	34.597	13570606	500.000	ug/L
7) T	2-Amino-4,6-dinitroto...	16.707	23867035	500.000	ug/L
8) T	4-Amino-2,6-dinitroto...	16.707	23867035	500.000	ug/L
9) T	2,4-Dinitrotoluene	22.429	19718688	500.000	ug/L
10) T	2,6-Dinitrotoluene	20.959	10299907	500.000	ug/L
11) T	1,3-Dinitrobenzene	16.174	20502312	500.000	ug/L
12) T	Nitrobenzene	12.559	14164154	500.000	ug/L
13) T	2-Nitrotoluene	17.219	18255253	1000.000	ug/L
14) T	3-Nitrotoluene	18.490	19714175	1000.000	ug/L
15) T	4-Nitrotoluene	17.763	15828931	1000.000	ug/L
16) T	3,5-Dinitroaniline	14.061	35705268	1000.000	ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.