

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL053113\HL005344.D Vial: 6
Acq On : 31-May-2013, 15:47 Operator: QM
Sample : E2366-03 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 31 17:03 2013 Quant Results File: HL053013.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL053013.M
Title :
Last Update : Fri May 31 17:03:11 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

5) T	1,3-Dinitrobenzene	3.45	6989	0.436 ng/ml
9) T	2,4,6-Trinitrotoluene	6.35	125832	10.668 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HL005344.D HL053013.M Fri May 31 17:03:18 2013 RPT1


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL053113\HL005344.D Vial: 6
Acq On : 31-May-2013, 15:47 Operator: QM
Sample : E2366-03 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 31 17:03 2013 Quant Results File: HL053013.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL053013.M
Title :
Last Update : Fri May 31 17:03:11 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M


Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

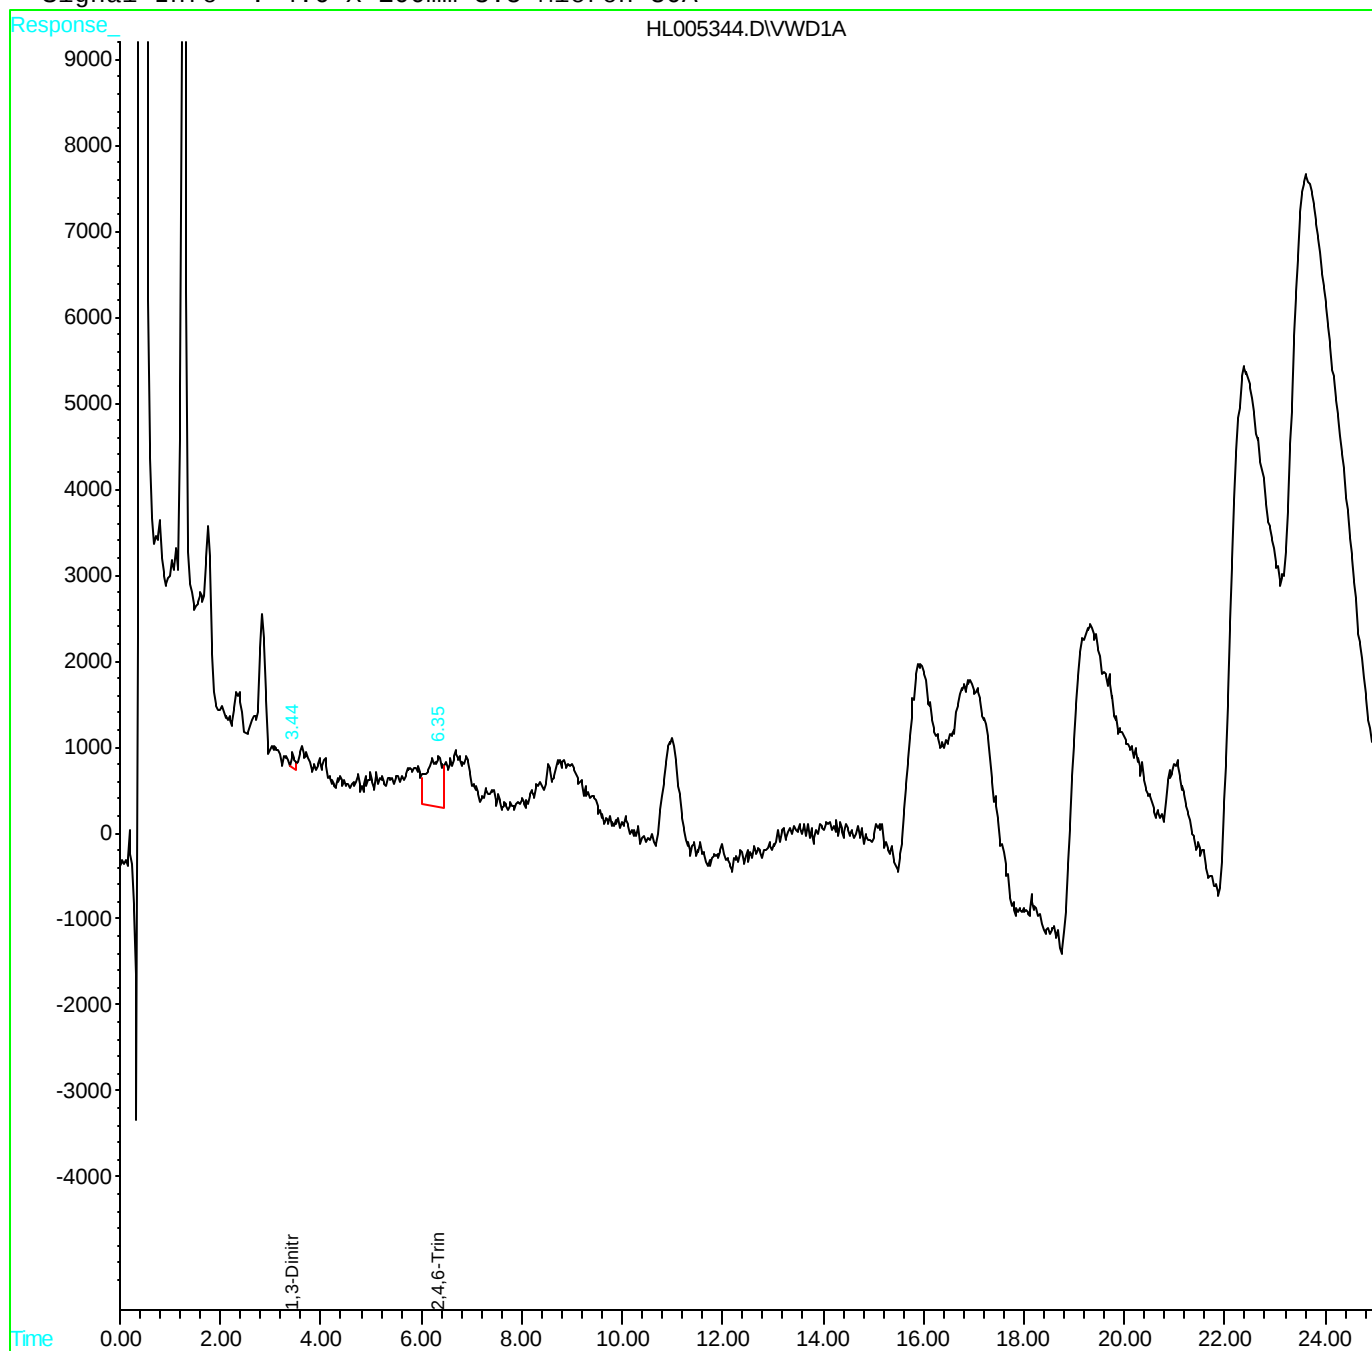

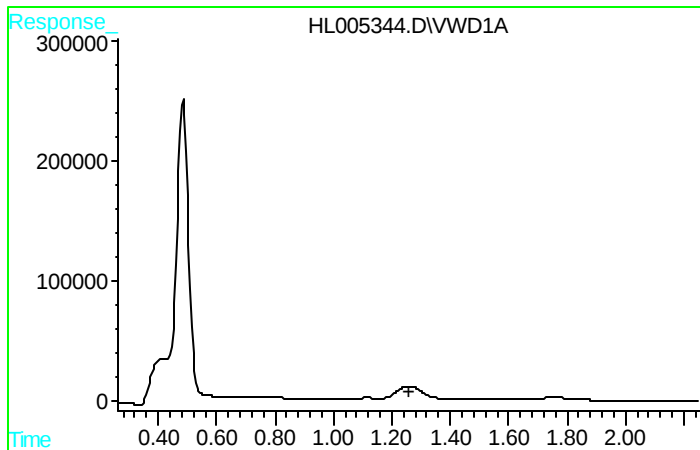


#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.260 min
Response: 0
Conc: N.D.

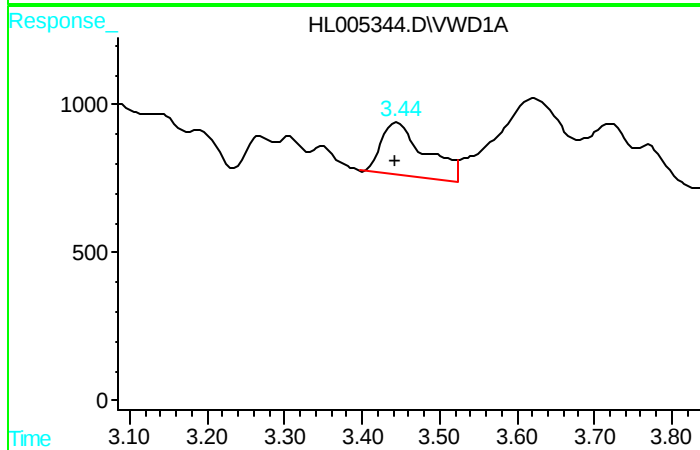

#5 1,3-Dinitrobenzene

R.T.: 3.447 min
Delta R.T.: 0.004 min
Response: 6989
Conc: 0.44 ng/ml

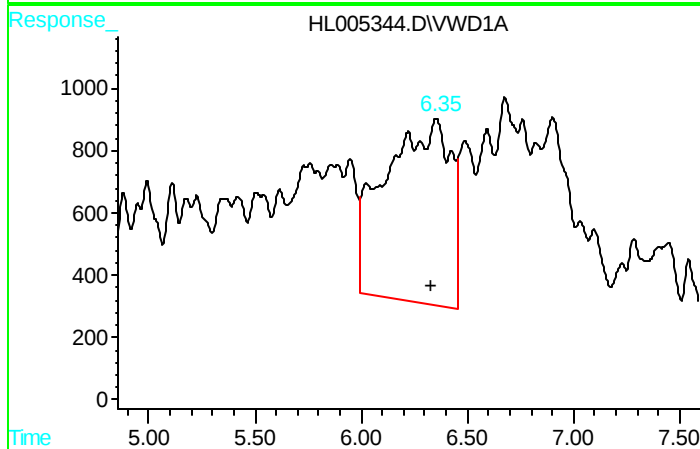

#9 2,4,6-Trinitrotoluene

R.T.: 6.354 min
Delta R.T.: 0.026 min
Response: 125832
Conc: 10.67 ug/L