

Data File : H:\VOL1\HPLC\HPLC L\120601\HL003146.D Vial: 49
Acq On : 01-Jun-2012, 21:54 Operator: HLM
Sample : D2872-02 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jun 4 10:37 2012 Quant Results File: HL050312.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL050312.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Jun 04 10:17:03 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.37	1654125	452.087 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 150.70%#

Target Compounds


16) T	3,5-Dinitroaniline	4.02f	178409	10.002 ug/L
-------	--------------------	-------	--------	-------------


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120601\HL003146.D Vial: 49
 Acq On : 01-Jun-2012, 21:54 Operator: HLM
 Sample : D2872-02 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jun 4 10:37 2012 Quant Results File: HL050312.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL050312.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Jun 04 10:17:03 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

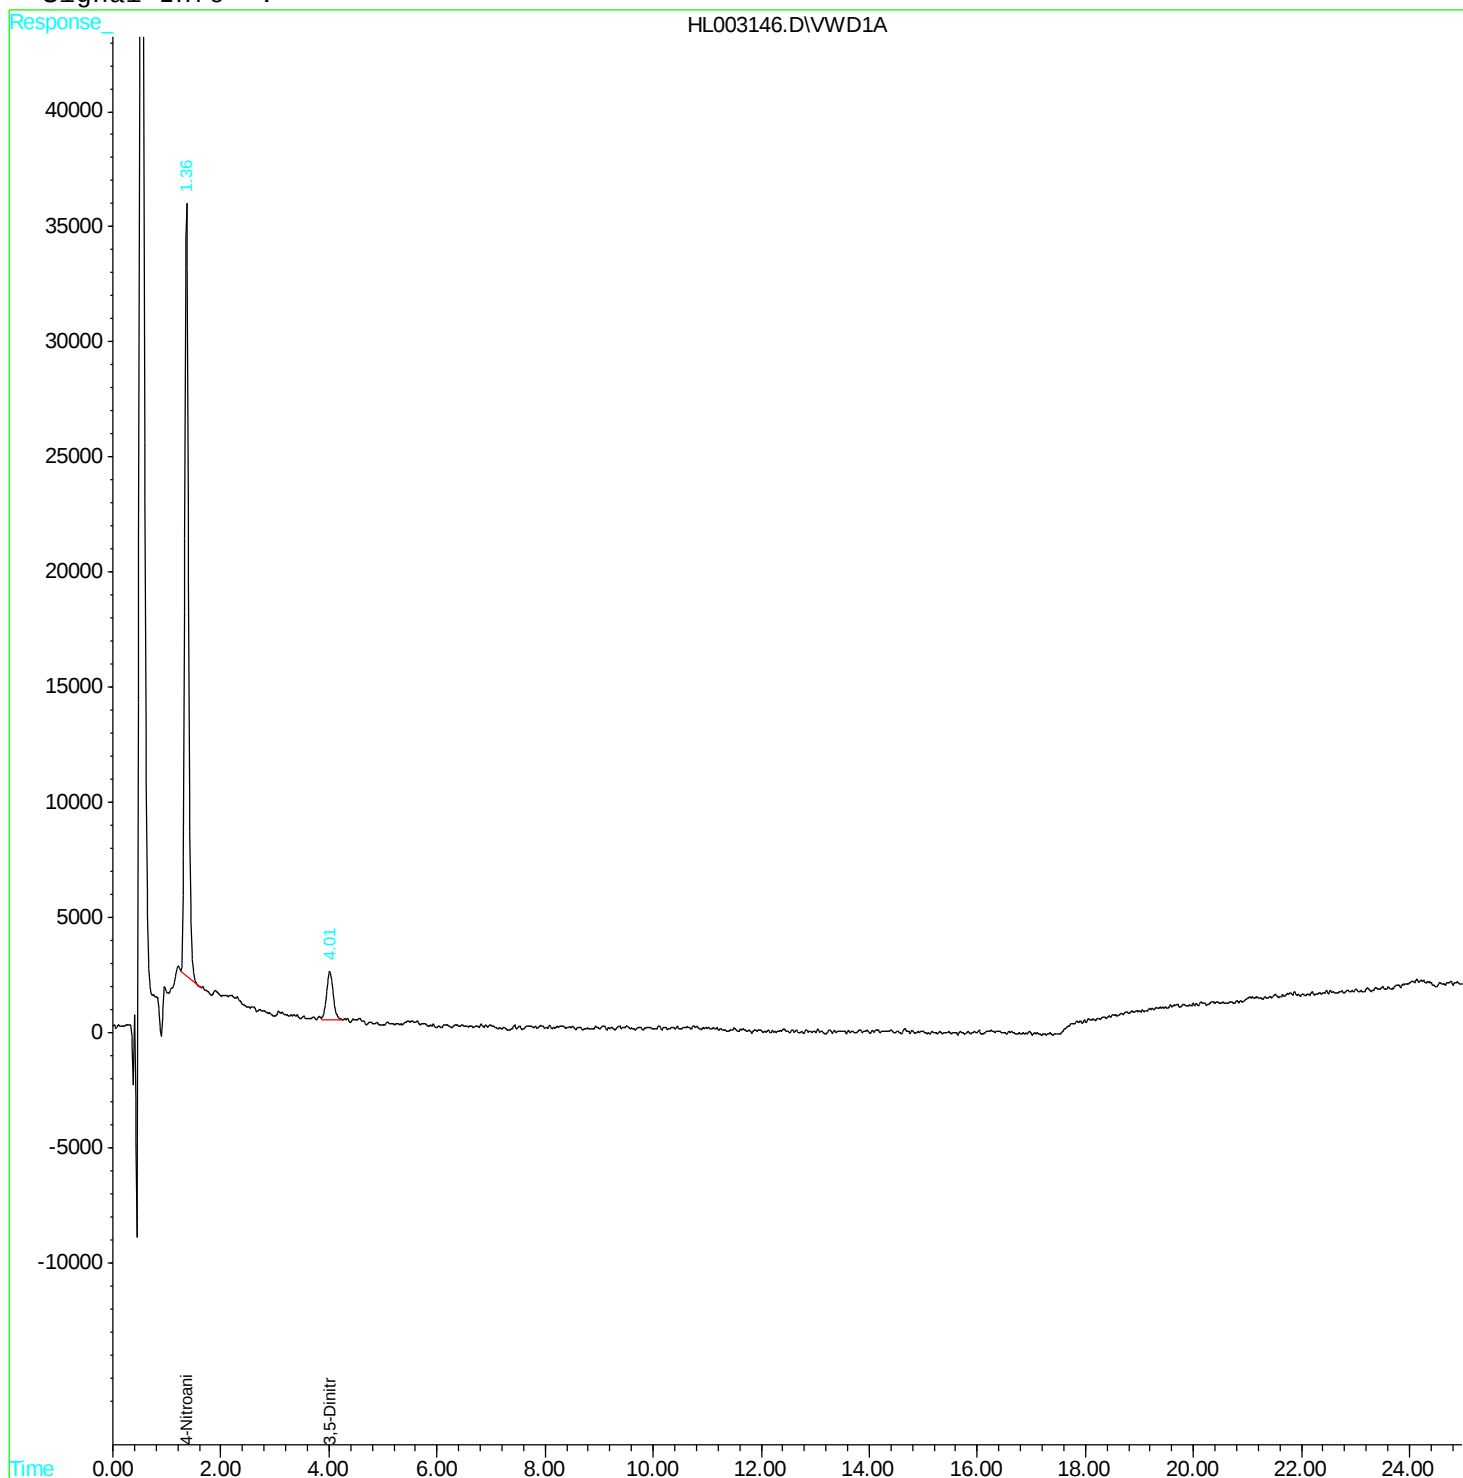

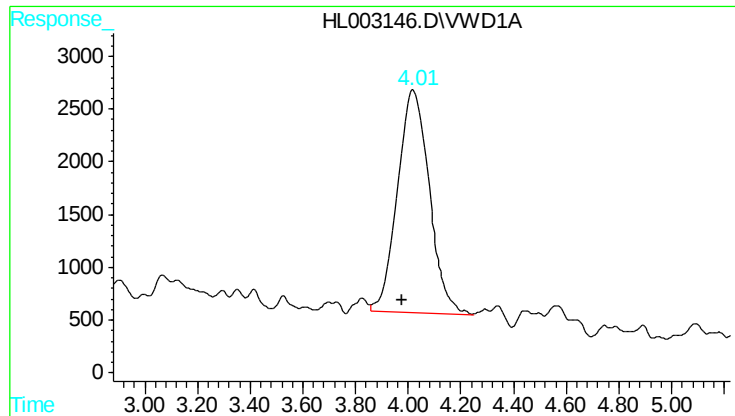

#16 3,5-Dinitroaniline

R.T.: 4.016 min
Delta R.T.: 0.038 min
Response: 178409
Conc: 10.00 ug/L