

Data File : H:\VOL1\HPLC\HPLC L\120601\HL003157.D Vial: 58
Acq On : 02-Jun-2012, 02:51 Operator: HLM
Sample : D2816-04MSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jun 4 10:18 2012 Quant Results File: HL050312.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL050312.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Mon Jun 04 10:17:03 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.36	929258	253.975 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 84.66%

Target Compounds


5) T	Tetryl	6.22f	218615	24.339 ug/L
13) T	2-Nitrotoluene	12.00	16596	2.387 ug/L
17) T	Nitroglycerin	6.22	218615	3723.605 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120601\HL003157.D Vial: 58
 Acq On : 02-Jun-2012, 02:51 Operator: HLM
 Sample : D2816-04MSD2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jun 4 10:18 2012 Quant Results File: HL050312.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL050312.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Jun 04 10:17:03 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M


Volume Inj. :
 Signal Phase :
 Signal Info :

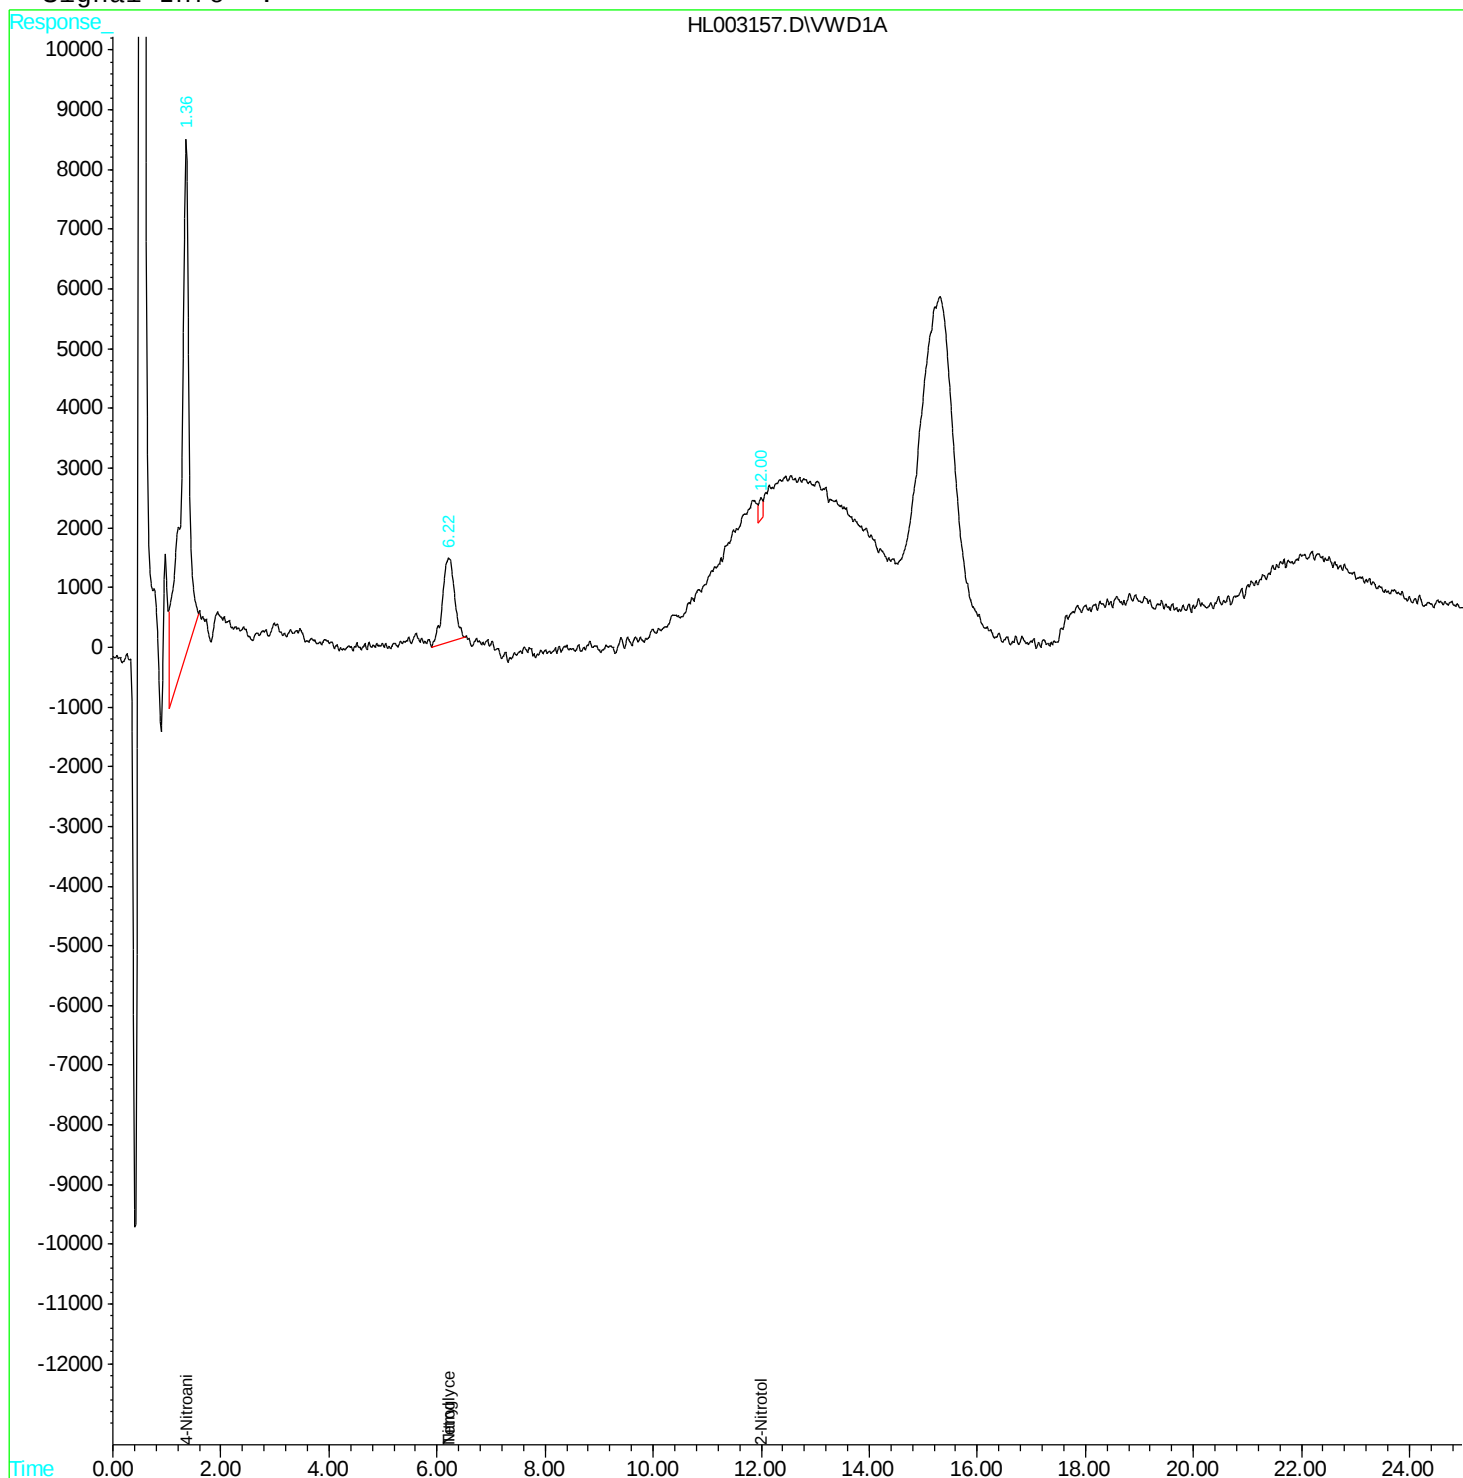

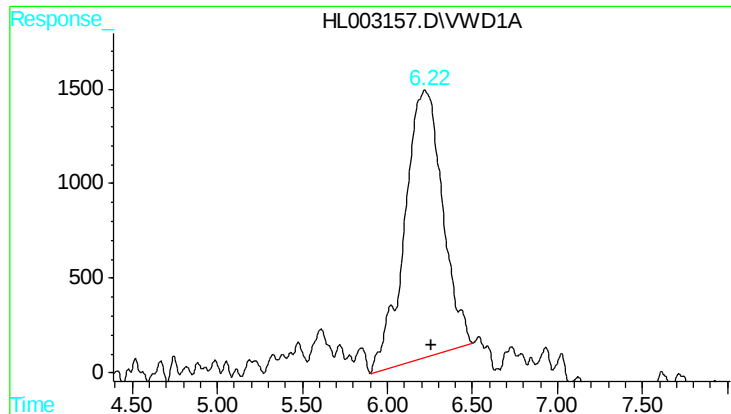


#5 Tetryl

R.T.: 6.220 min
Delta R.T.: -0.038 min
Response: 218615
Conc: 24.34 ug/L

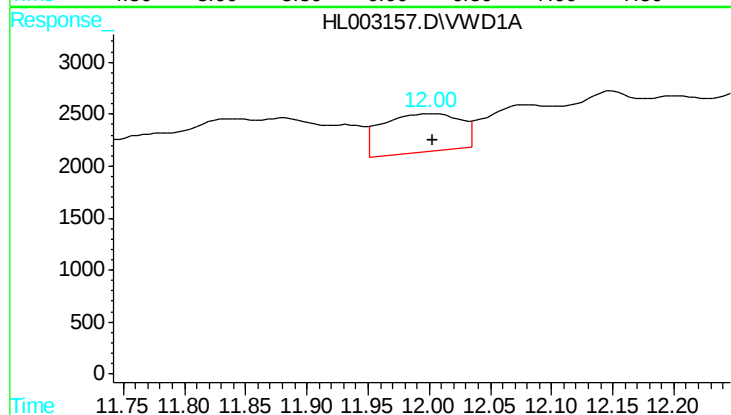

#13 2-Nitrotoluene

R.T.: 12.003 min
Delta R.T.: 0.000 min
Response: 16596
Conc: 2.39 ug/L

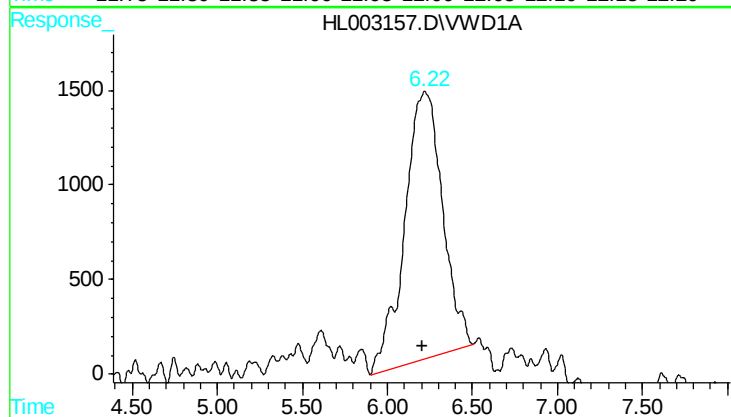

#17 Nitroglycerin

R.T.: 6.220 min
Delta R.T.: 0.012 min
Response: 218615
Conc: 3723.60 ug/L