

Data Path : X:\HPCHEM1\HPLC\_L\Data\HL060112\  
Data File : HL003162.D  
Signal(s) : VWD1A.CH  
Acq On : 02-Jun-2012, 05:05  
Operator : HLM  
Sample : D2816-05  
Misc :  
ALS Vial : 59 Sample Multiplier: 1


Instrument :  
HPLC\_L  
ClientSampleId :  
C0AA4


Manual Integrations  
APPROVED

AHPatel  
6/6/2012 3:43:12 AM

Integration File: events.e  
Quant Time: Jun 05 04:03:12 2012  
Quant Method : H:\VOL1\HPLC\HPLC\_L\METHODS\HL050312.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Mon Jun 04 10:17:03 2012  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

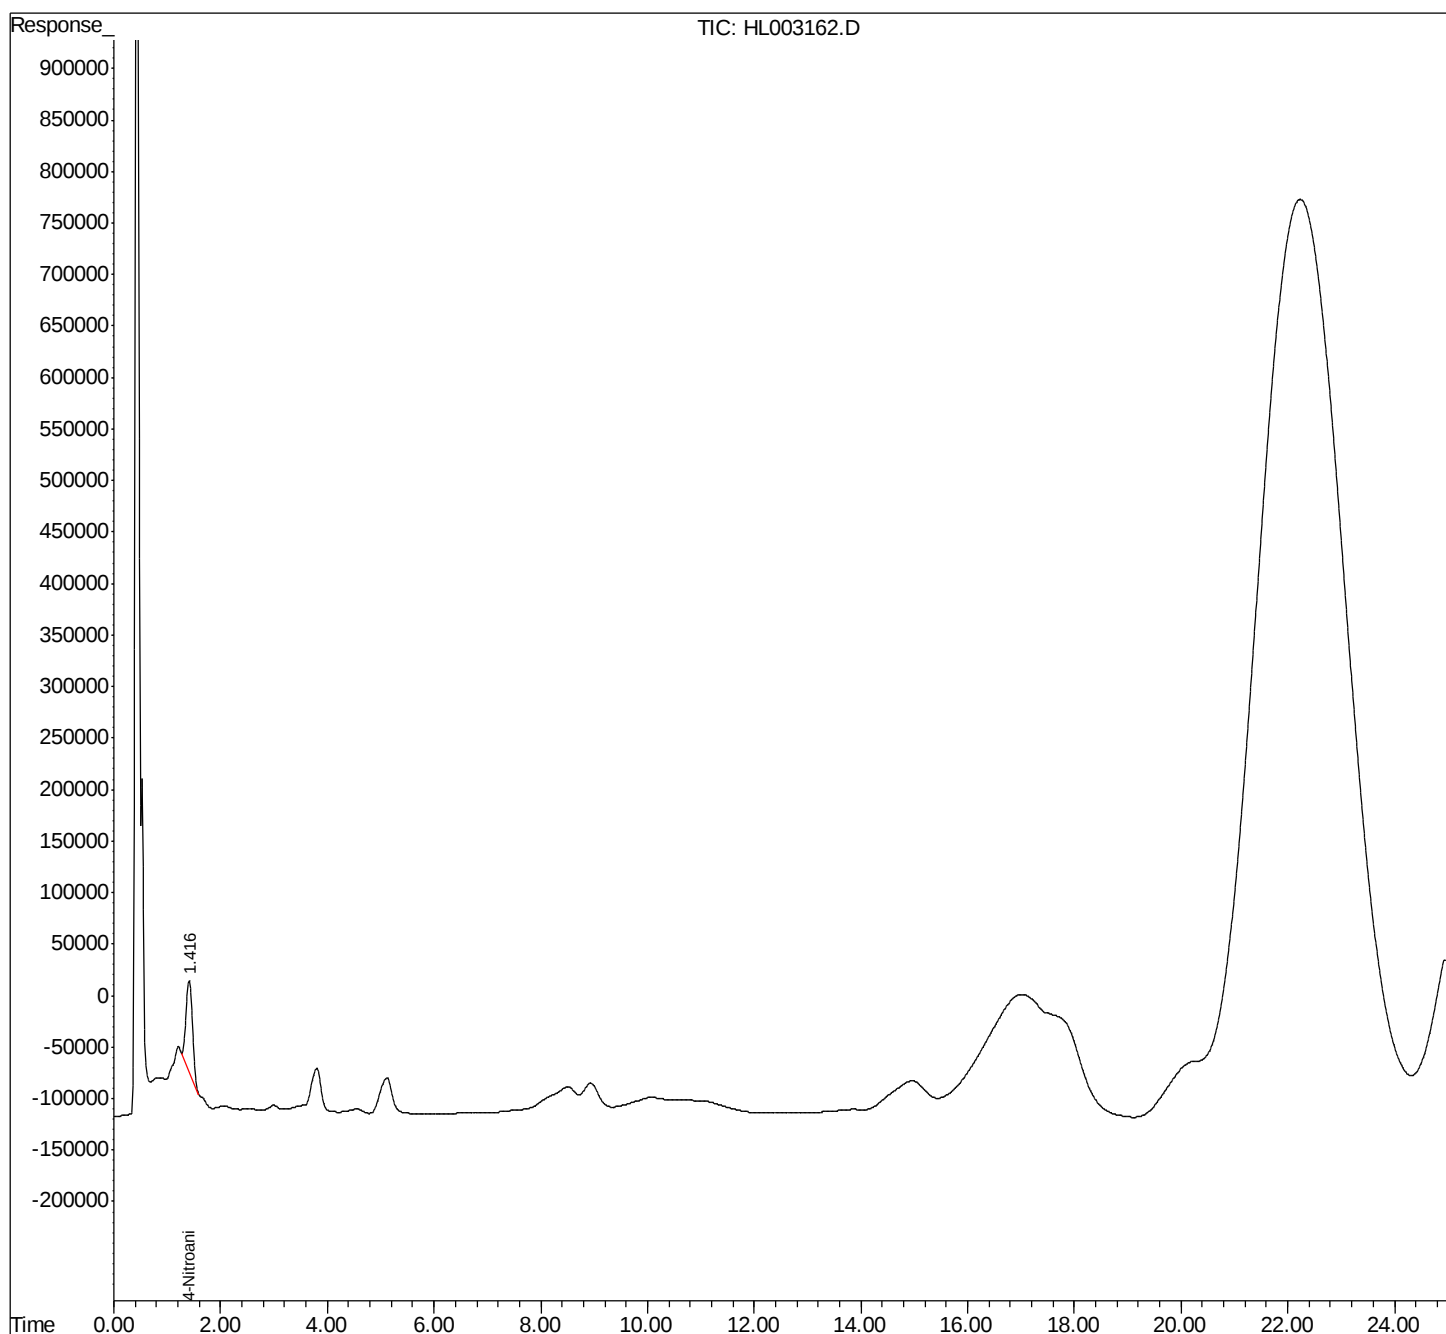

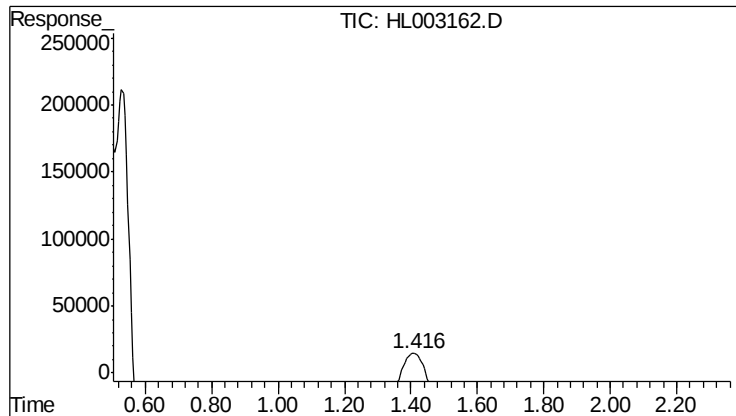

#1 4-Nitroaniline

R.T.: 1.416 min  
Delta R.T.: 0.050 min  
Response: 7416917  
Conc: 2027.11 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
C0AA4

Manual Integrations  
APPROVED

AHPatel  
6/6/2012 3:43:12 AM

Data Path : X:\HPCHEM1\HPLC\_L\Data\HL060112\  
Data File : HL003162.D  
Signal(s) : VWD1A.CH  
Acq On : 02-Jun-2012, 05:05  
Operator : HLM  
Sample : D2816-05  
Misc :  
ALS Vial : 59 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
C0AA4

Manual Integrations  
APPROVED

AHPatel  
6/6/2012 3:43:12 AM

Integration File: events.e  
Quant Time: Jun 05 04:03:12 2012  
Quant Method : H:\VOL1\HPLC\HPLC\_L\METHODS\HL050312.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Mon Jun 04 10:17:03 2012  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

| Compound                    | R.T.           | Response | Conc Units      |
|-----------------------------|----------------|----------|-----------------|
| -----                       |                |          |                 |
| System Monitoring Compounds |                |          |                 |
| 1) S 4-Nitroaniline         | 1.416f         | 7416917  | 2027.111 ug/L m |
| Spiked Amount 300.000       | Range 37 - 149 | Recovery | = 675.70%#      |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.