

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL060413\HL005373.D Vial: 7
Acq On : 04-Jun-2013, 21:25 Operator: QM
Sample : E2428-01MS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 7:57 2013 Quant Results File: HL060413.RES

Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL060413.M
Title :
Last Update : Tue Jun 04 17:00:19 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.34	647568	167.467 ug/L
Target Compounds			
2) T HMX	0.93	31605	7.022 ug/L
5) T 1,3-Dinitrobenzene	3.57	37568	2.444 ng/ml
6) T 3,5-Dinitroaniline	3.93	123842	9.172 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005373.D HL060413.M

Wed Jun 05 07:57:52 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL060413\HL005373.D Vial: 7
Acq On : 04-Jun-2013, 21:25 Operator: QM
Sample : E2428-01MS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 7:57 2013 Quant Results File: HL060413.RES

Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL060413.M
Title :
Last Update : Tue Jun 04 17:00:19 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

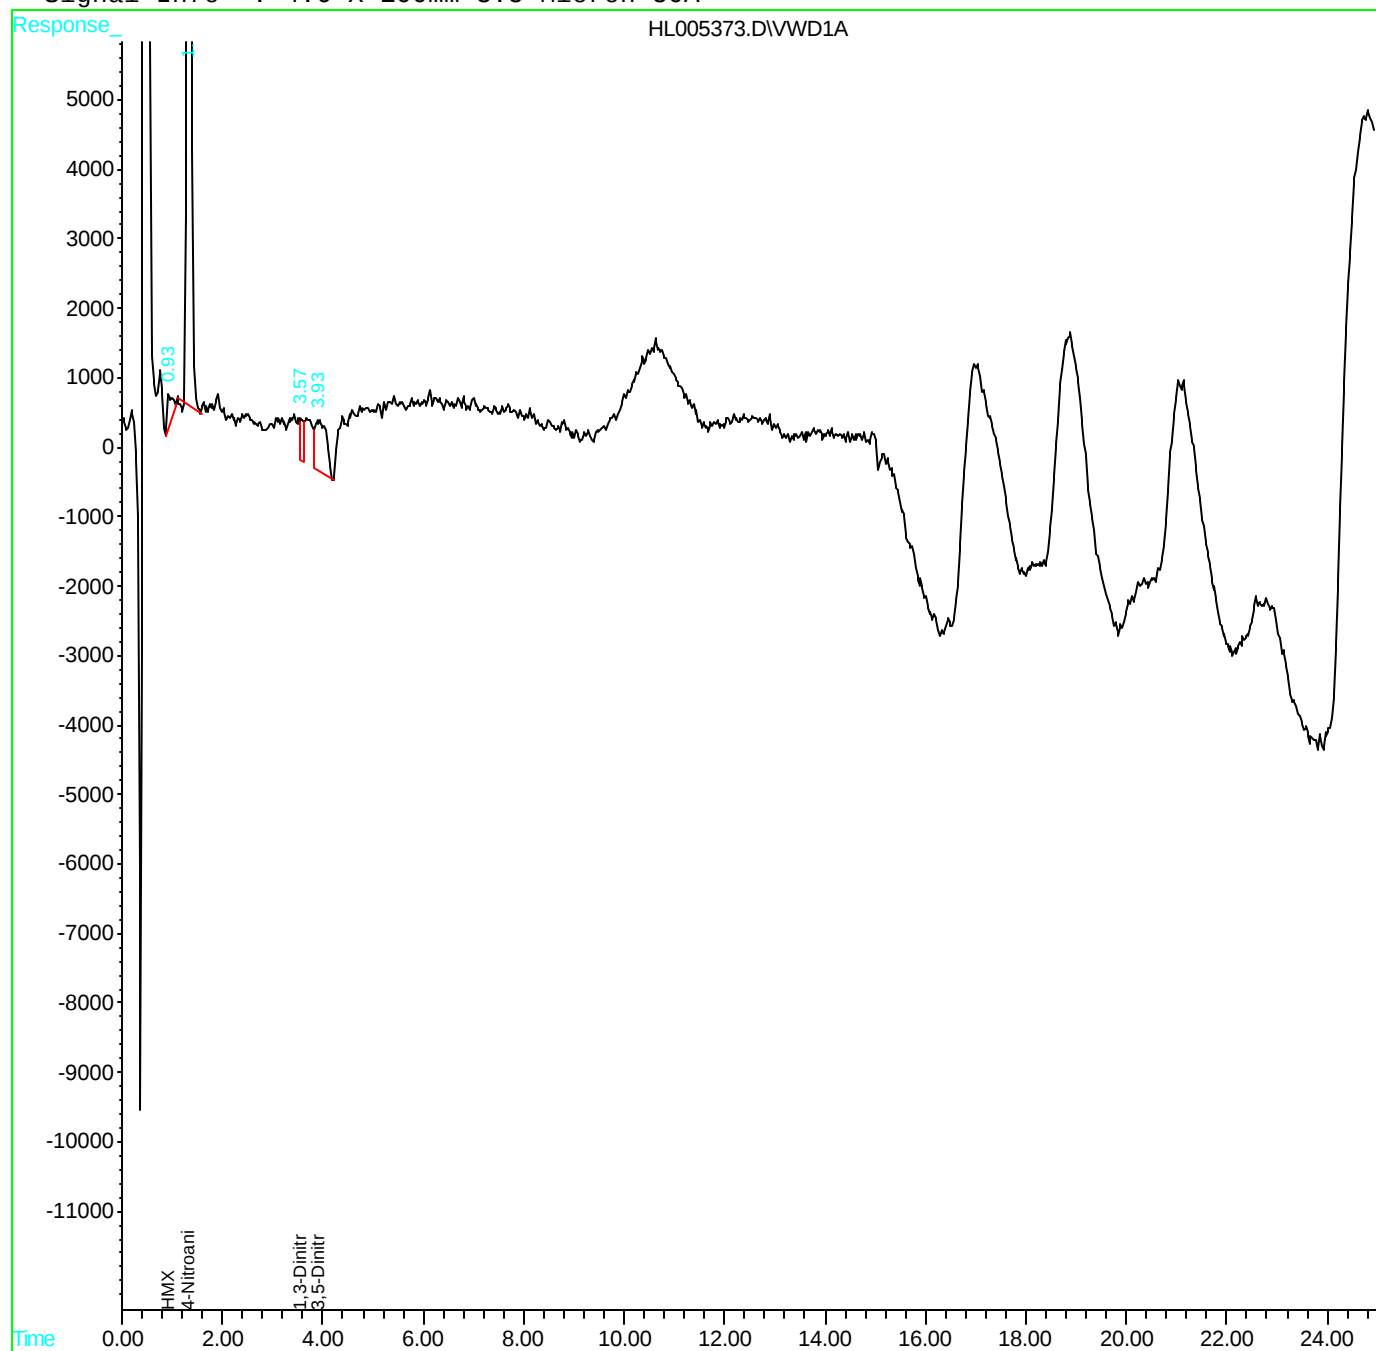


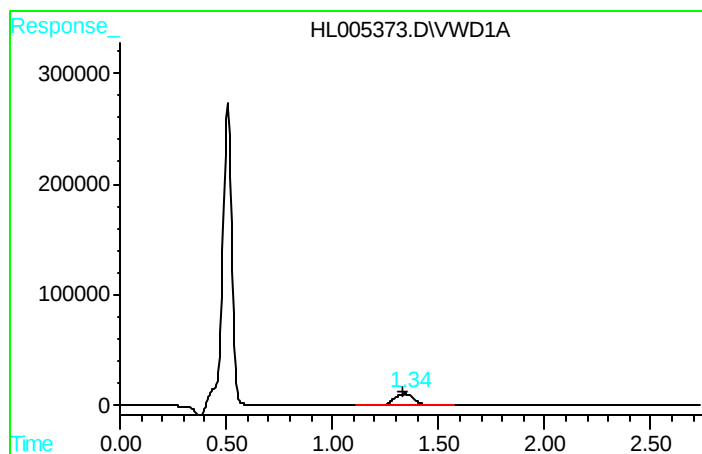

#1 4-Nitroaniline


R.T.: 1.341 min
Delta R.T.: 0.008 min
Response: 647568
Conc: 167.47 ug/L

Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS

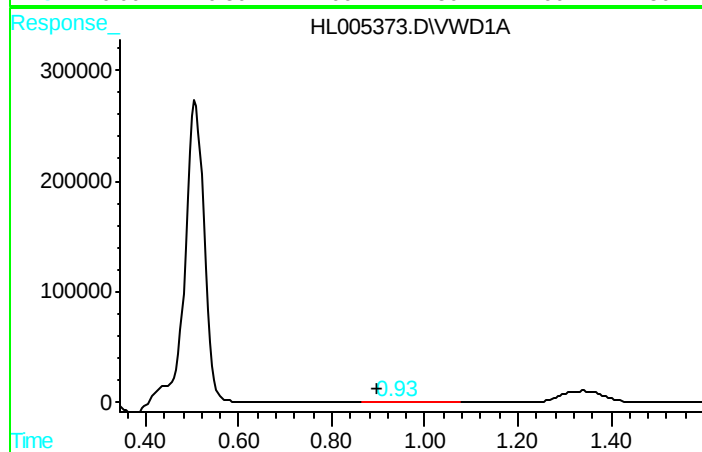


#2 HMX

R.T.: 0.934 min
Delta R.T.: 0.038 min
Response: 31605
Conc: 7.02 ug/L

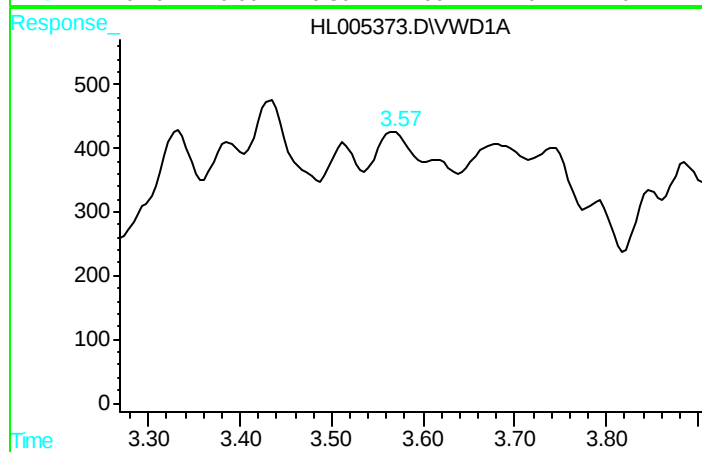

#5 1,3-Dinitrobenzene

R.T.: 3.570 min
Delta R.T.: 0.030 min
Response: 37568
Conc: 2.44 ng/ml

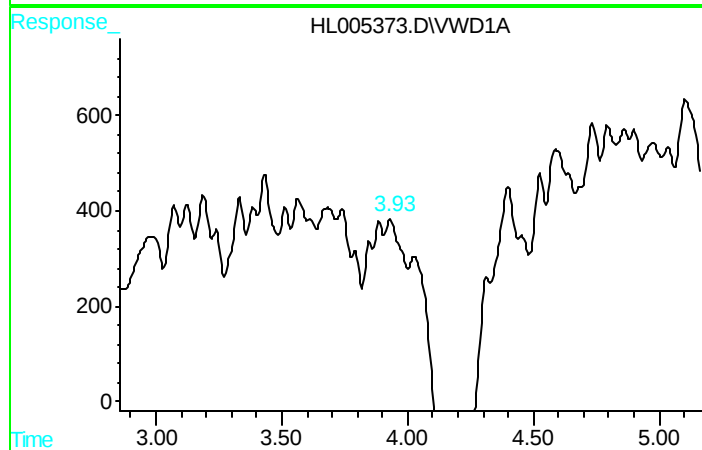

#6 3,5-Dinitroaniline

R.T.: 3.930 min
Delta R.T.: 0.020 min
Response: 123842
Conc: 9.17 ug/L