

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060413\
Data File : HL005362.D
Signal(s) : VWD1A.CH
Acq On : 04-Jun-2013, 16:01
Operator : QM
Sample : HSTDICCC0500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500

Integration File: autoint1.e
Quant Time: Jun 07 03:31:14 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL060413.M
Quant Title :
QLast Update : Thu Jun 06 16:09:39 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.326	1936162	500.707 ug/L
Target Compounds			
2) T HMX	0.894	1953346	433.976 ug/L
3) T RDX	1.723	2401290	507.575 ug/L
4) T 1,3,5-Trinitrobenzene	2.673	5371359	475.963 ug/L
9) T 2,4,6-Trinitrotoluene	6.357	3434800	302.153 ug/L
11) T 4-Amino-2,6-dinitroto...	7.164	2975618	488.892 ug/L
13) T 2,6-Dinitrotoluene	8.299	2876203	369.851 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060413\
Data File : HL005362.D
Signal(s) : VWD1A.CH
Acq On : 04-Jun-2013, 16:01
Operator : QM
Sample : HSTDICCC0500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500

Integration File: autoint1.e
Quant Time: Jun 07 03:31:14 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL060413.M
Quant Title :
QLast Update : Thu Jun 06 16:09:39 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

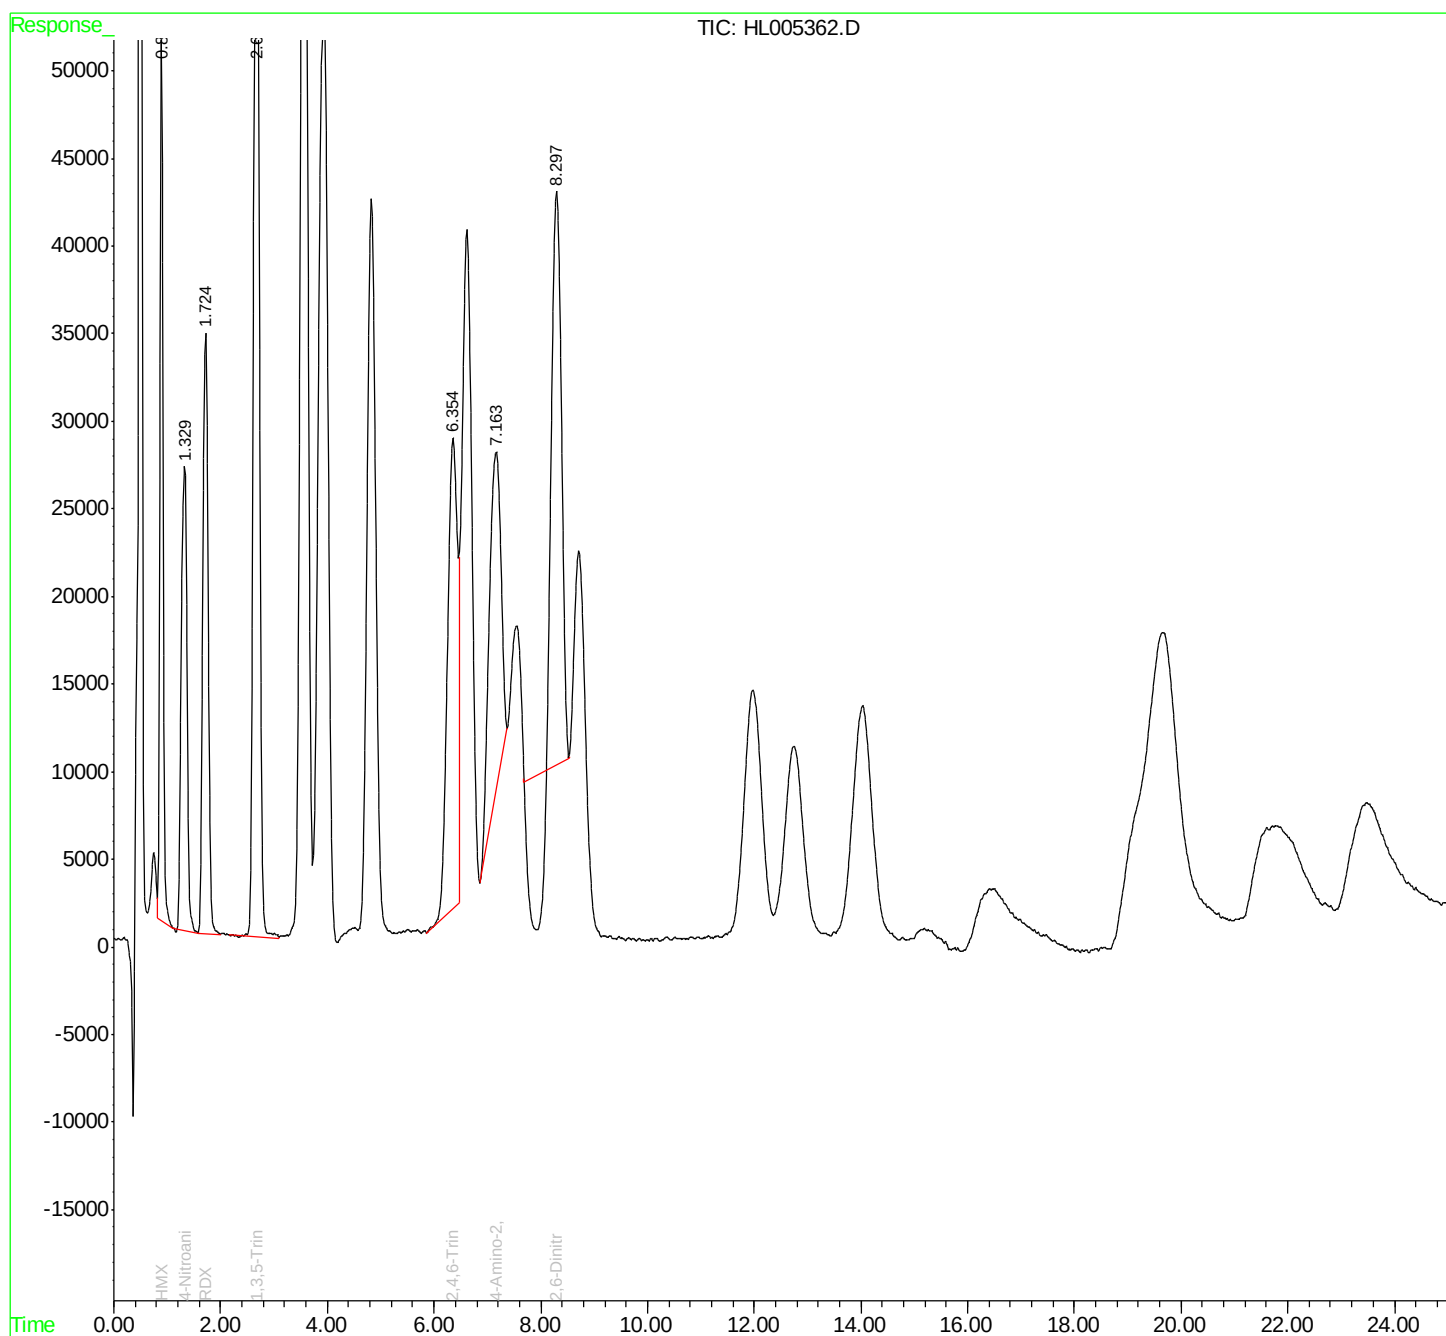


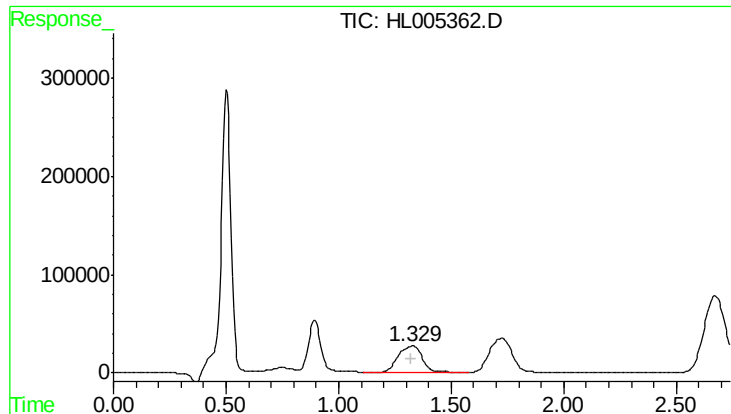

#1 4-Nitroaniline


R.T.: 1.326 min
 Delta R.T.: 0.007 min
 Response: 1936162
 Conc: 500.71 ug/L

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICC0500

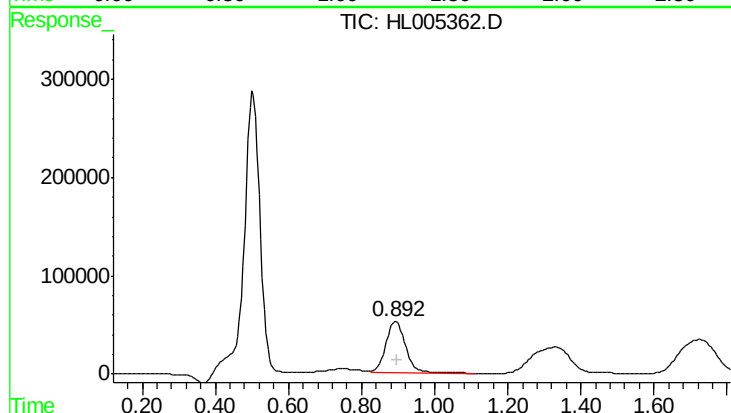


#2 HMX

R.T.: 0.894 min
 Delta R.T.: -0.001 min
 Response: 1953346
 Conc: 433.98 ug/L

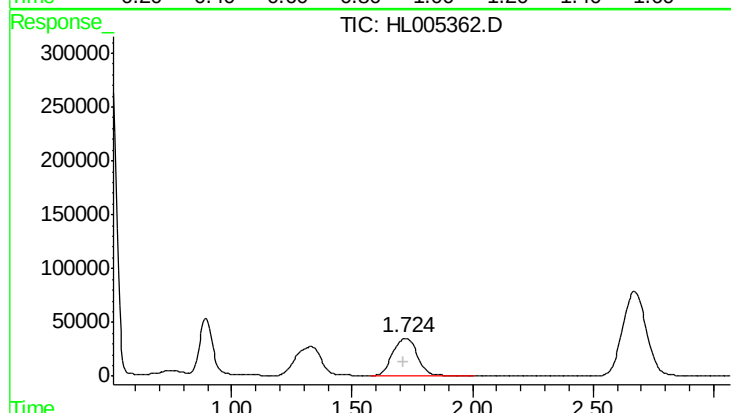


#3 RDX

R.T.: 1.723 min
 Delta R.T.: 0.009 min
 Response: 2401290
 Conc: 507.58 ug/L

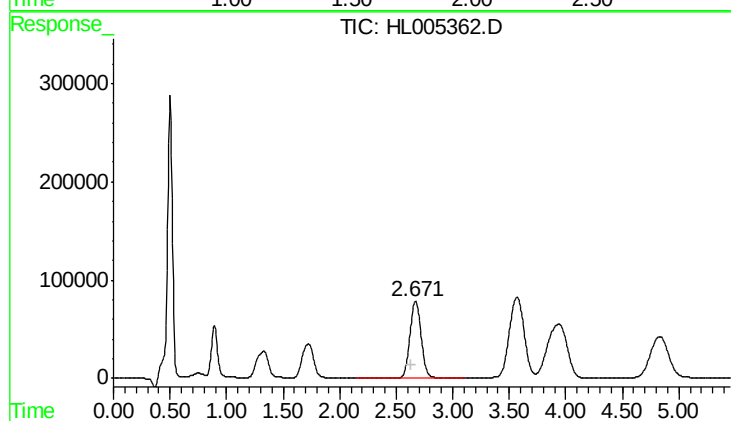

#4 1,3,5-Trinitrobenzene


R.T.: 2.673 min
 Delta R.T.: 0.039 min
 Response: 5371359
 Conc: 475.96 ug/L

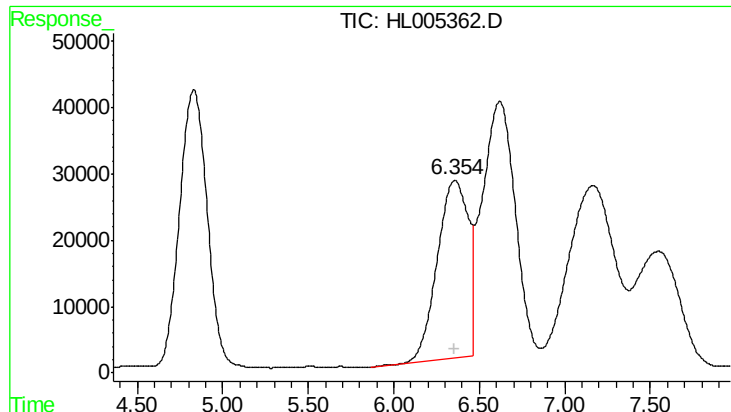

#9 2,4,6-Trinitrotoluene


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 3434800
Conc: 302.15 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0500

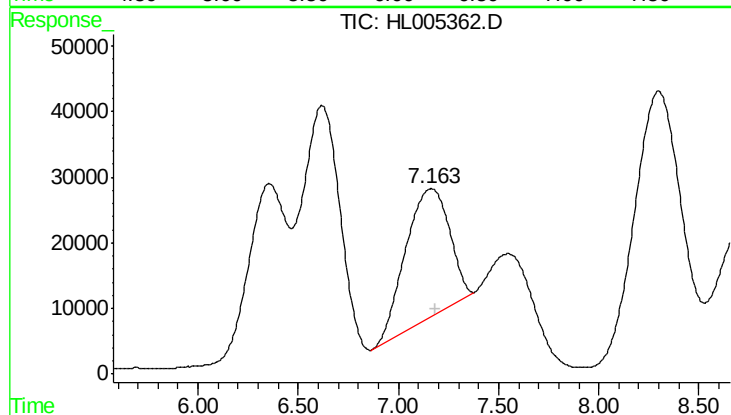

#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.164 min
Delta R.T.: -0.018 min
Response: 2975618
Conc: 488.89 ug/L

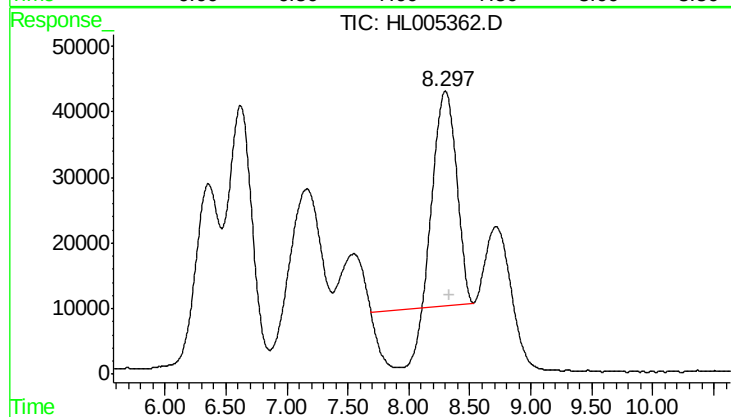

#13 2,6-Dinitrotoluene

R.T.: 8.299 min
Delta R.T.: -0.039 min
Response: 2876203
Conc: 369.85 ug/L