

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060613\
 Data File : HL005412.D
 Signal(s) : VWD1A.CH
 Acq On : 06-Jun-2013, 14:16
 Operator : QM
 Sample : E2428-01MS
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 SS26-WC15MS

Manual Integrations
 APPROVED

AHPatel
 6/7/2013 3:58:24 AM

Integration File: autoint1.e
 Quant Time: Jun 07 05:37:11 2013
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL060413.M
 Quant Title :
 QLast Update : Tue Jun 04 16:52:57 2013
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.283	642965	166.276 ug/L
Target Compounds			
2) T HMX	0.869	599030	133.087 ug/L
3) T RDX	1.674	714271	150.980 ug/L
4) T 1,3,5-Trinitrobenzene	2.623	1453685	128.813 ug/L
5) T 1,3-Dinitrobenzene	3.493	2108296	137.166 ng/mL
6) T 3,5-Dinitroaniline	3.839	1696256	125.625 ug/L
7) T Nitrobenzene	4.678	1371623	139.089 ug/L
8) T Teteryl	6.124	753399	95.058 ug/L
9) T 2,4,6-Trinitrotoluene	6.390	1396155	122.817 ug/L
10) T 2-Amino-4,6-dinitroto...	6.895	1379839	123.358 ug/L
11) T 4-Amino-2,6-dinitroto...	7.239	837407	137.585 ug/L
12) T 2,4-Dinitrotoluene	7.970	1929083	132.090 ug/L
13) T 2,6-Dinitrotoluene	8.362	1086903	139.765 ug/L
14) T 2-Nitrotoluene	11.533	956749	144.009 ug/L
15) T 4-Nitrotoluene	12.298	776361	142.971 ug/L
16) T 3-Nitrotoluene	13.548	1019075	141.484 ug/L
17) T PETN	18.905	1252372	131.739 ug/L m

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060613\
Data File : HL005412.D
Signal(s) : VWD1A.CH
Acq On : 06-Jun-2013, 14:16
Operator : QM
Sample : E2428-01MS
Misc :
ALS Vial : 43 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS


Manual Integrations
APPROVED

AHPatel
6/7/2013 3:58:24 AM

Integration File: autoint1.e
Quant Time: Jun 07 05:37:11 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL060413.M
Quant Title :
QLast Update : Tue Jun 04 16:52:57 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

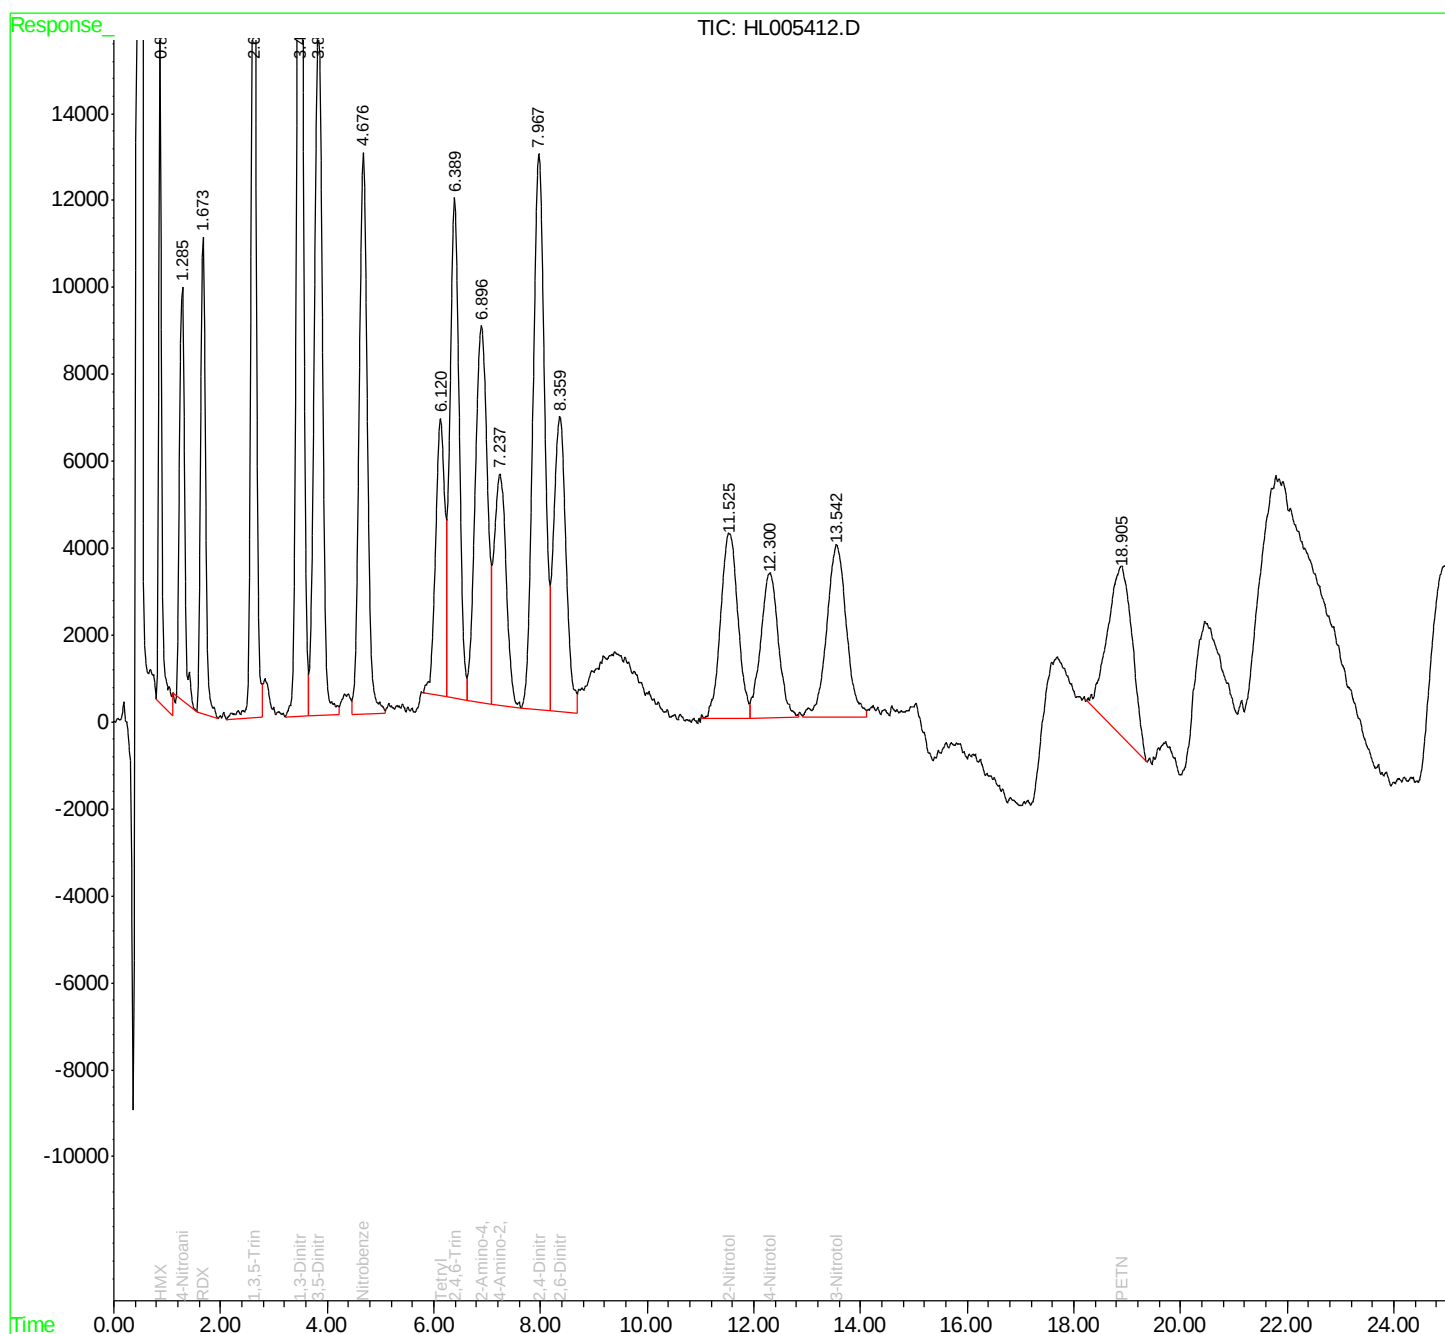

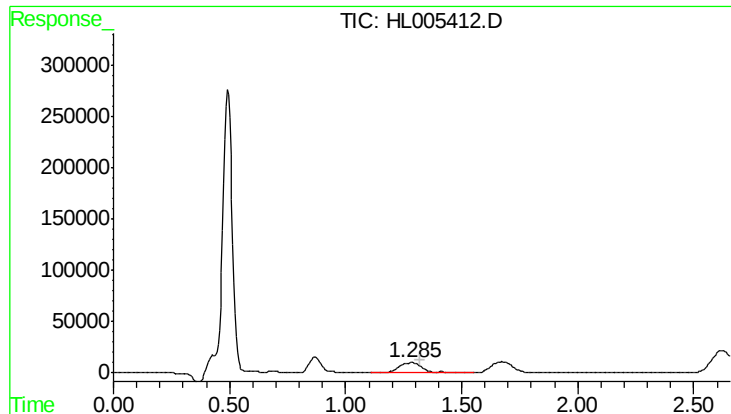


#1 4-Nitroaniline

R.T.: 1.283 min
Delta R.T.: -0.040 min
Response: 642965
Conc: 166.28 ug/L

Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS


Manual Integrations
APPROVED

AHPatel
6/7/2013 3:58:24 AM

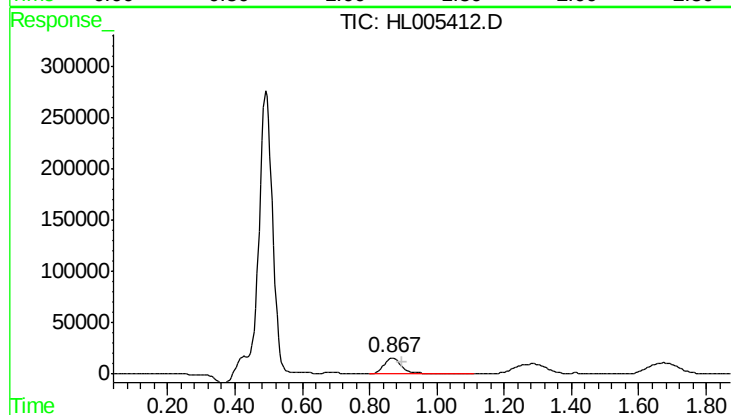


#2 HMX

R.T.: 0.869 min
Delta R.T.: -0.029 min
Response: 599030
Conc: 133.09 ug/L

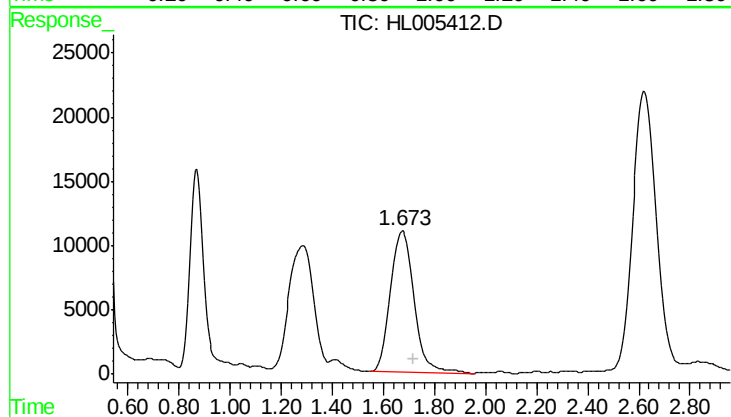


#3 RDX

R.T.: 1.674 min
Delta R.T.: -0.044 min
Response: 714271
Conc: 150.98 ug/L

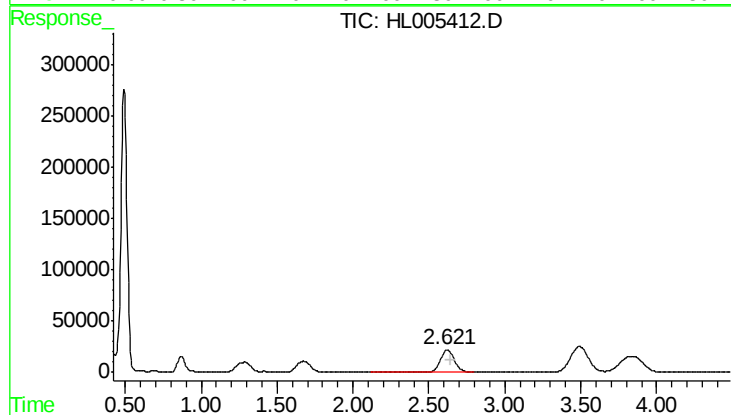

#4 1,3,5-Trinitrobenzene

R.T.: 2.623 min
Delta R.T.: -0.023 min
Response: 1453685
Conc: 128.81 ug/L

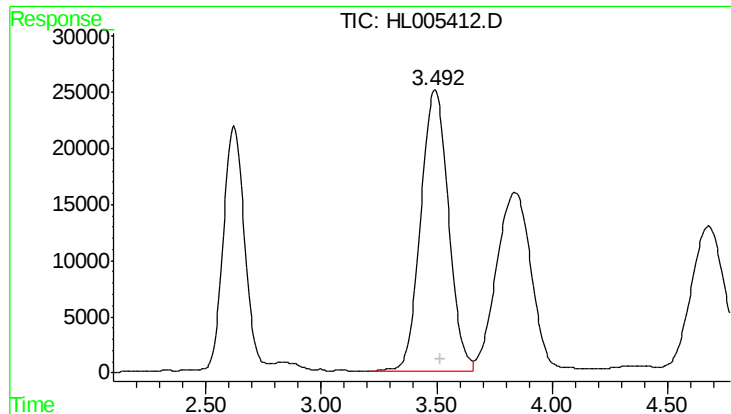


#5 1,3-Dinitrobenzene

R.T.: 3.493 min
Delta R.T.: -0.023 min
Response: 2108296
Conc: 137.17 ng/ml

Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS


Manual Integrations
APPROVED

AHPatel
6/7/2013 3:58:24 AM

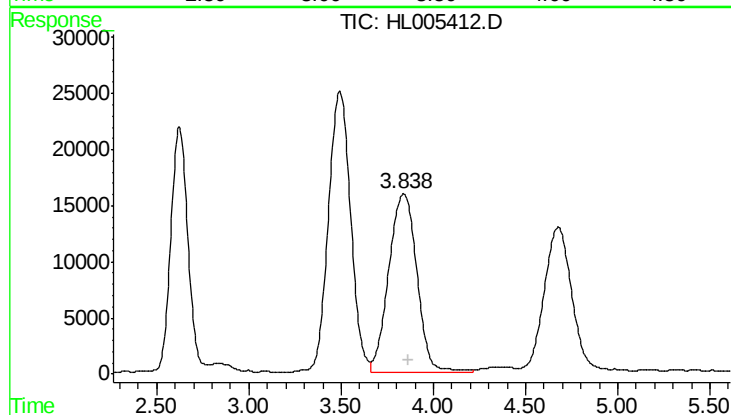


#6 3,5-Dinitroaniline

R.T.: 3.839 min
Delta R.T.: -0.028 min
Response: 1696256
Conc: 125.62 ug/L

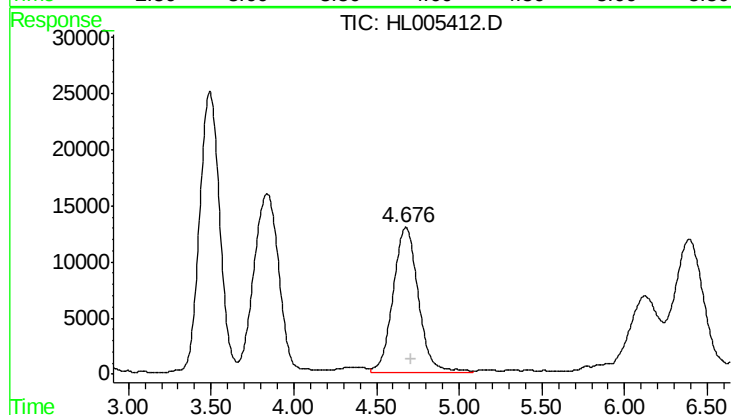


#7 Nitrobenzene

R.T.: 4.678 min
Delta R.T.: -0.031 min
Response: 1371623
Conc: 139.09 ug/L

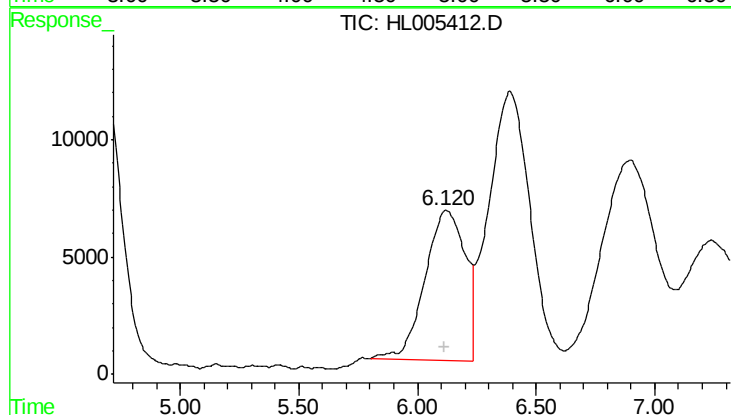

#8 Tetryl

R.T.: 6.124 min
Delta R.T.: 0.011 min
Response: 753399
Conc: 95.06 ug/L

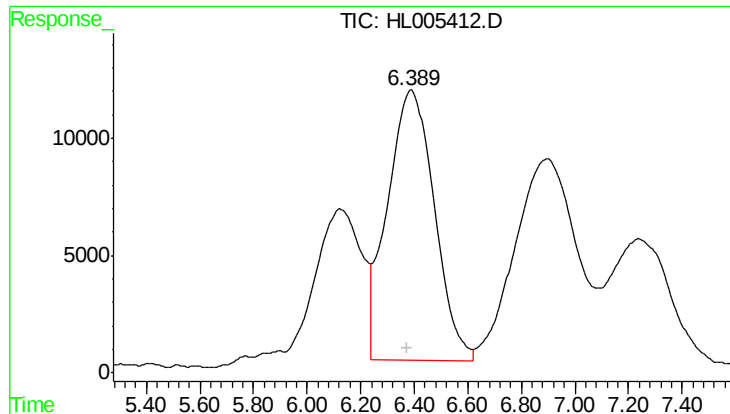


#9 2,4,6-Trinitrotoluene

R.T.: 6.390 min
Delta R.T.: 0.018 min
Response: 1396155
Conc: 122.82 ug/L

Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS


Manual Integrations
APPROVED

AHPatel
6/7/2013 3:58:24 AM

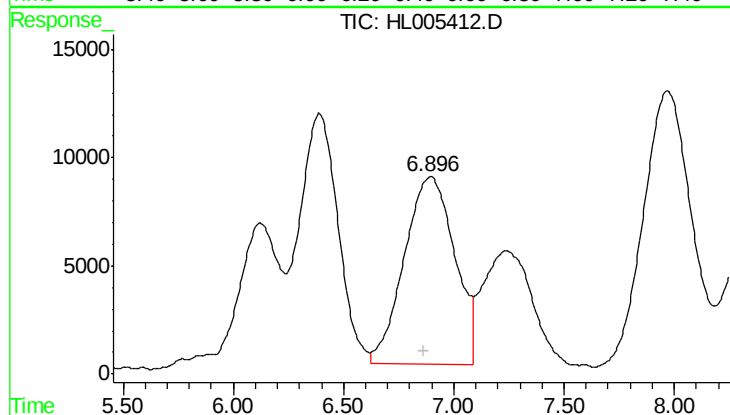


#10 2-Amino-4,6-dinitrotoluene

R.T.: 6.895 min
Delta R.T.: 0.031 min
Response: 1379839
Conc: 123.36 ug/L

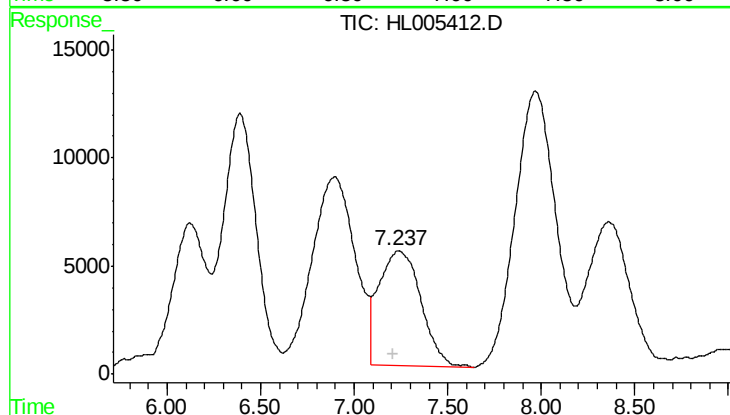


#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.239 min
Delta R.T.: 0.030 min
Response: 837407
Conc: 137.59 ug/L

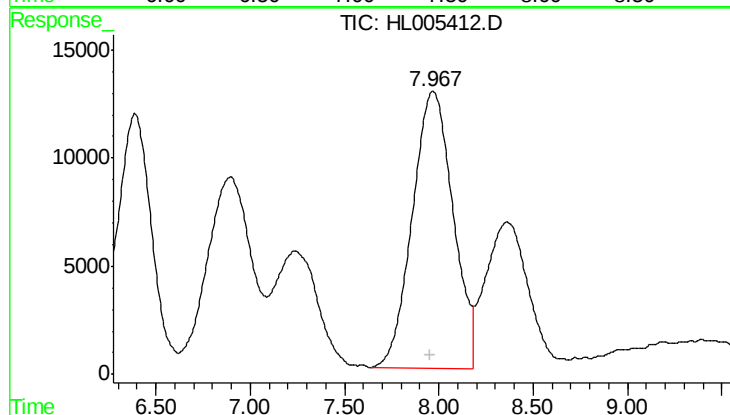

#12 2,4-Dinitrotoluene

R.T.: 7.970 min
Delta R.T.: 0.015 min
Response: 1929083
Conc: 132.09 ug/L

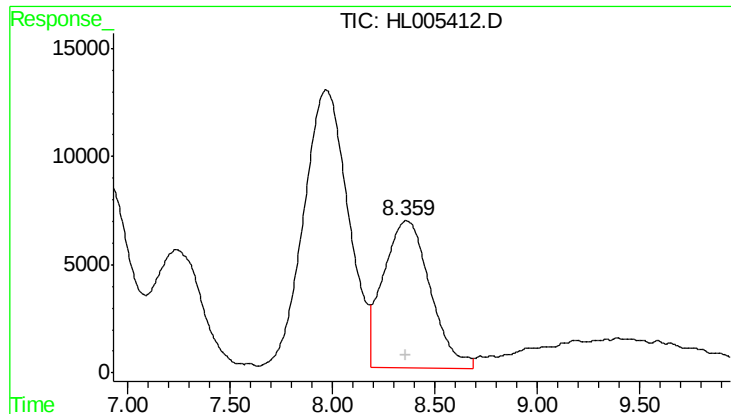


#13 2,6-Dinitrotoluene

R.T.: 8.362 min
Delta R.T.: 0.000 min
Response: 1086903
Conc: 139.76 ug/L

Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS


Manual Integrations
APPROVED

AHPatel
6/7/2013 3:58:24 AM

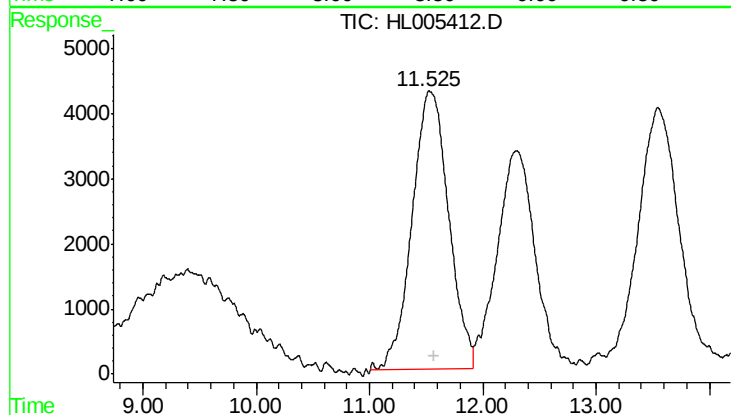


#14 2-Nitrotoluene

R.T.: 11.533 min
Delta R.T.: -0.038 min
Response: 956749
Conc: 144.01 ug/L

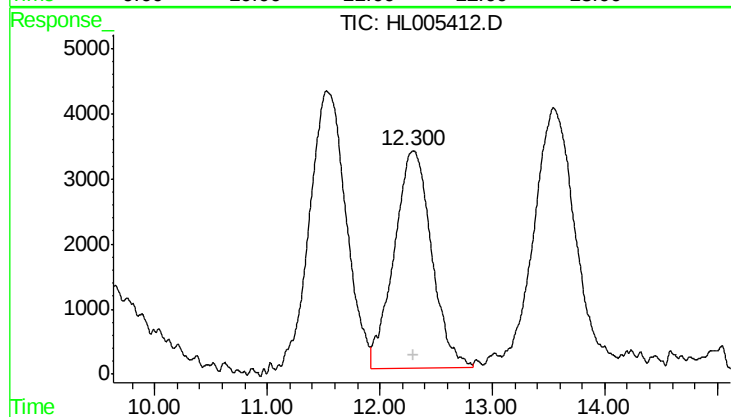


#15 4-Nitrotoluene

R.T.: 12.298 min
Delta R.T.: -0.002 min
Response: 776361
Conc: 142.97 ug/L

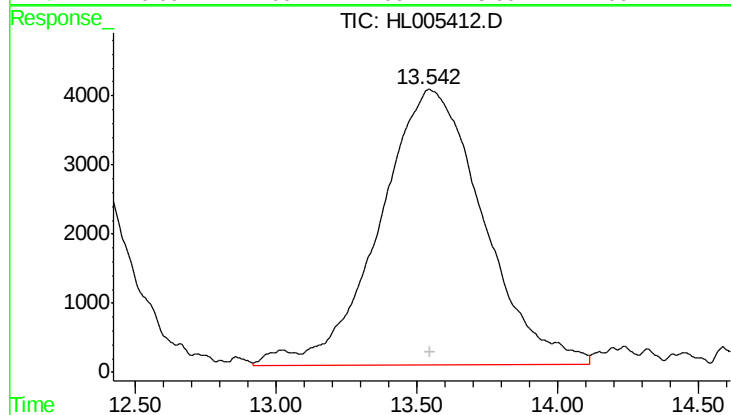

#16 3-Nitrotoluene

R.T.: 13.548 min
Delta R.T.: 0.002 min
Response: 1019075
Conc: 141.48 ug/L

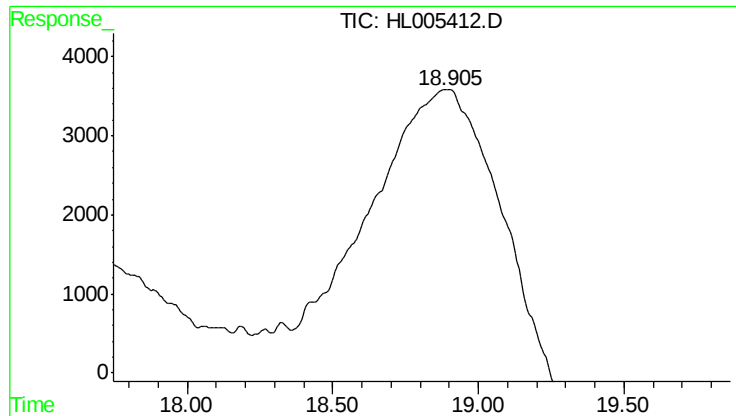

#17 PETN

R.T.: 18.905 min
Delta R.T.: -0.063 min
Response: 1252372
Conc: 131.74 ug/L m

Instrument :
HPLC_L
ClientSampleId :
SS26-WC15MS

Manual Integrations
APPROVED

AHPatel
6/7/2013 3:58:24 AM