



Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060812\
Data File : HL003218.D
Signal(s) : VWD1A.CH
Acq On : 08-Jun-2012, 16:05
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
CCAL01

Integration File: events.e
Quant Time: Jun 14 04:22:14 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL053012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu May 31 11:08:18 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

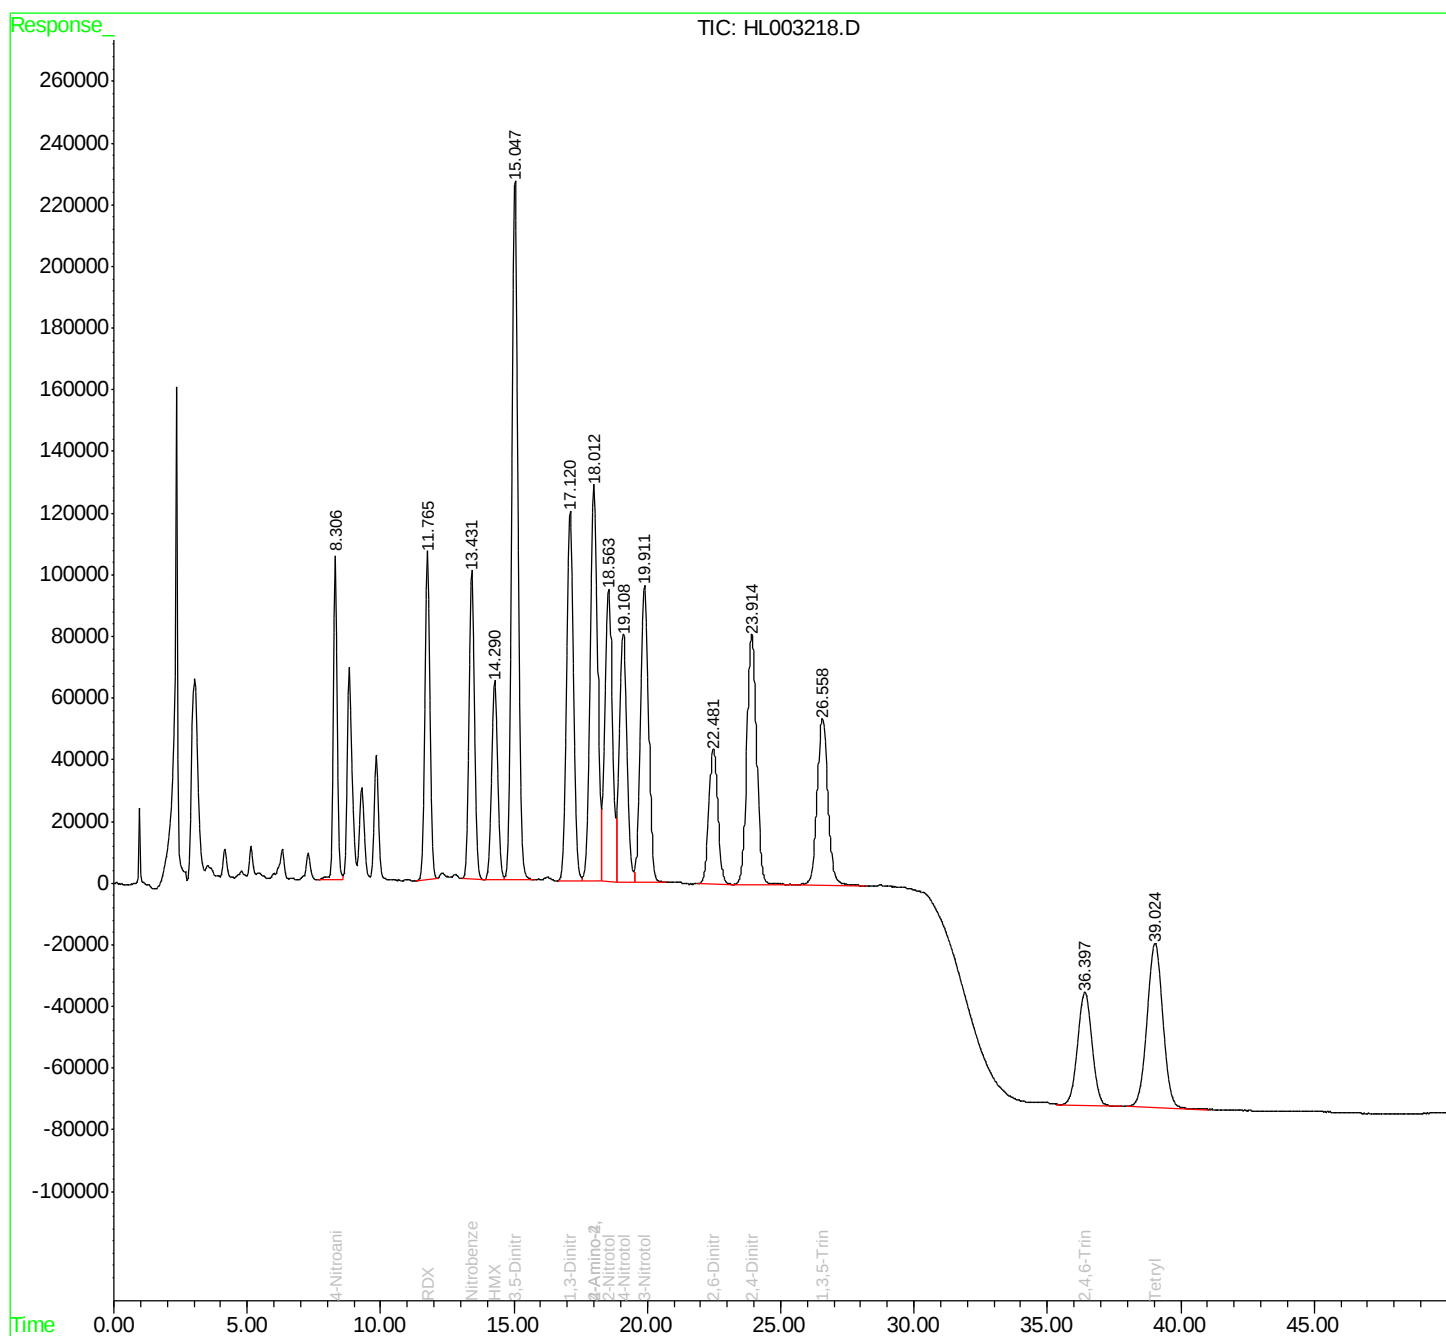


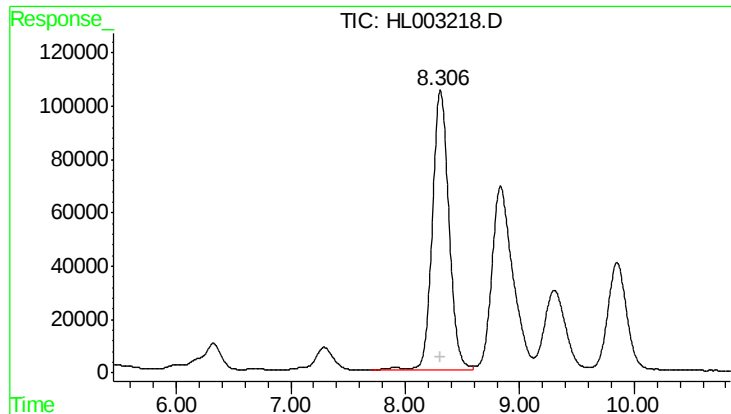

#1 4-Nitroaniline


R.T.: 8.308 min
Delta R.T.: 0.000 min
Response: 10546923
Conc: 1040.52 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL01

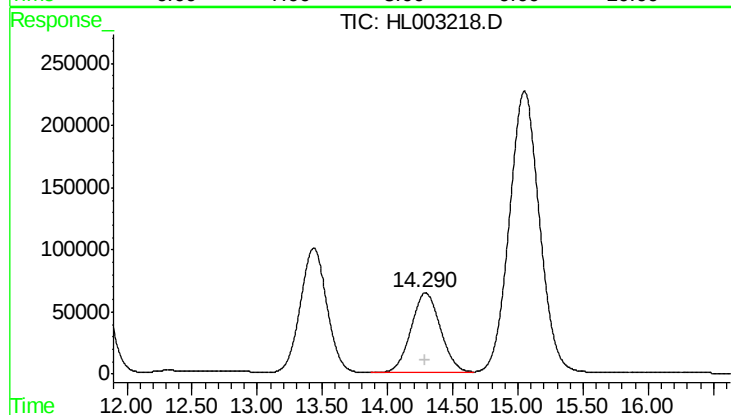


#2 HMX

R.T.: 14.292 min
Delta R.T.: 0.000 min
Response: 10260341
Conc: 1037.94 ug/L

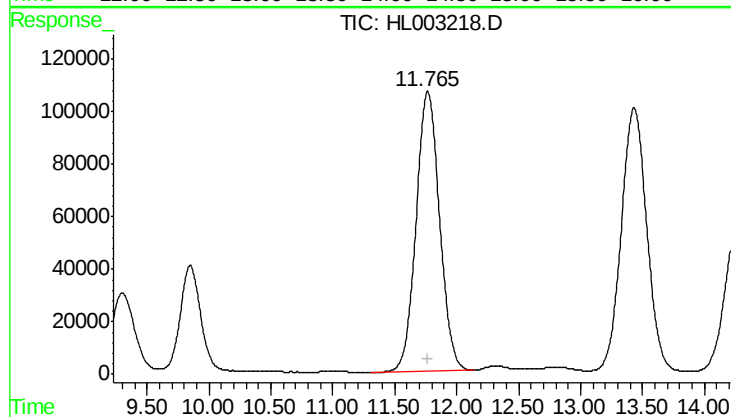


#3 RDX

R.T.: 11.767 min
Delta R.T.: 0.000 min
Response: 14018954
Conc: 1020.96 ug/L

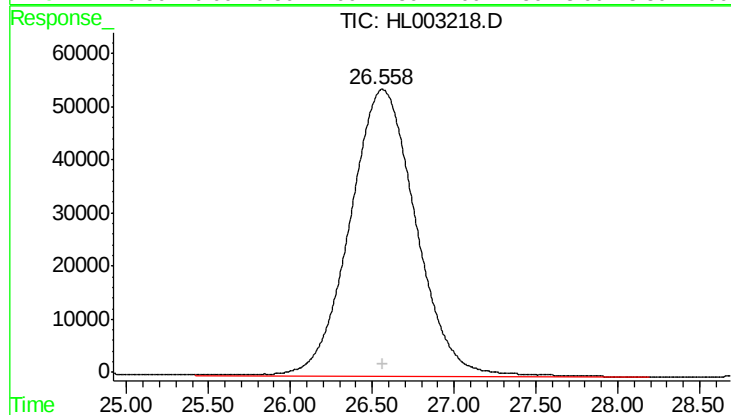

#4 1,3,5-Trinitrobenzene


R.T.: 26.562 min
Delta R.T.: 0.000 min
Response: 15409847
Conc: 553.48 ug/L

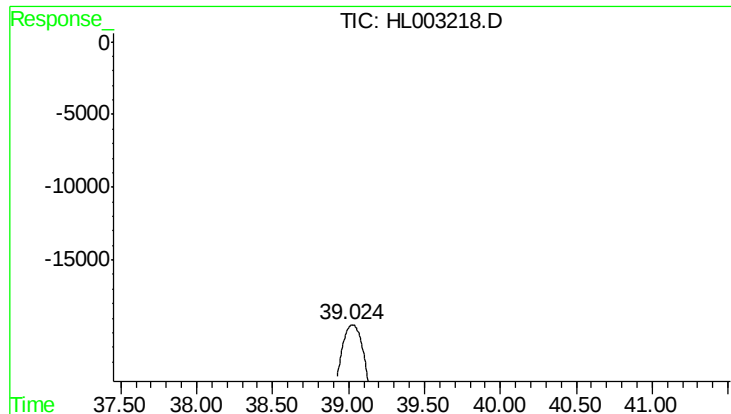

#5 Tetryl


R.T.: 39.027 min
Delta R.T.: 0.000 min
Response: 21928442
Conc: 1032.36 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL01

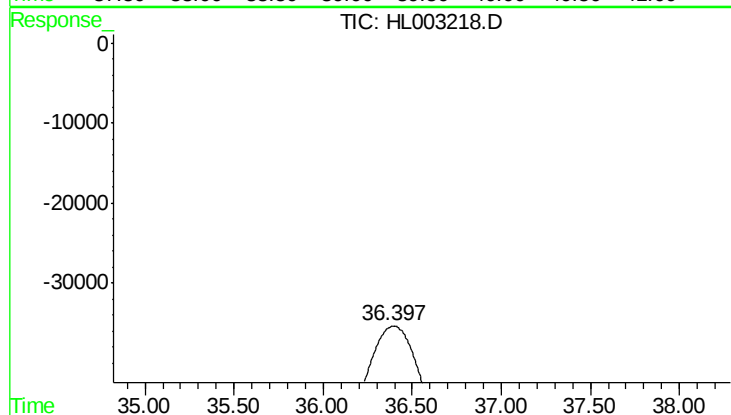


#6 2,4,6-Trinitrotoluene

R.T.: 36.395 min
Delta R.T.: 0.000 min
Response: 13729851
Conc: 509.58 ug/L

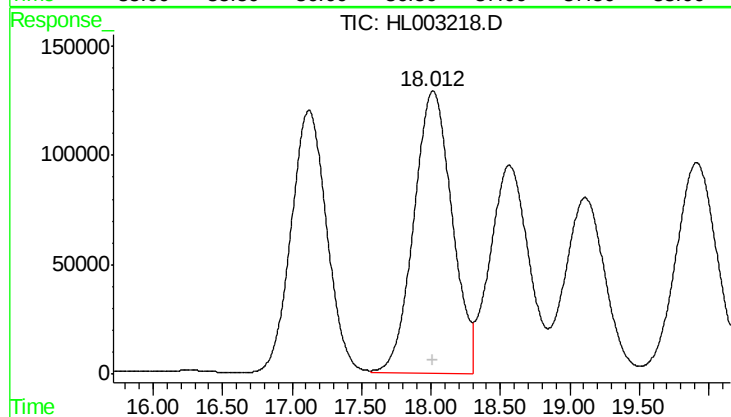


#7 2-Amino-4,6-dinitrotoluene

R.T.: 18.014 min
Delta R.T.: 0.000 min
Response: 24697240
Conc: 513.00 ug/L

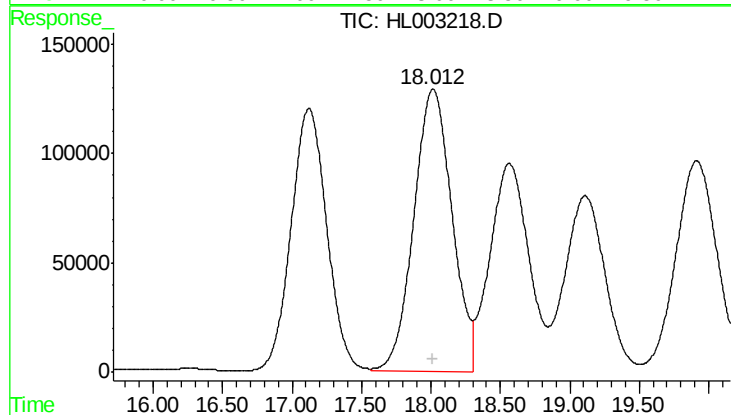

#8 4-Amino-2,6-dinitrotoluene


R.T.: 18.014 min
Delta R.T.: 0.000 min
Response: 24697240
Conc: 510.48 ug/L

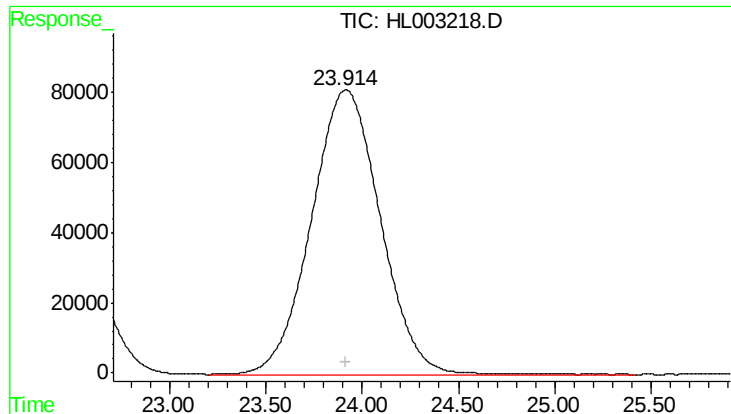

#9 2,4-Dinitrotoluene


R.T.: 23.916 min
Delta R.T.: 0.000 min
Response: 20453421
Conc: 524.81 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL01

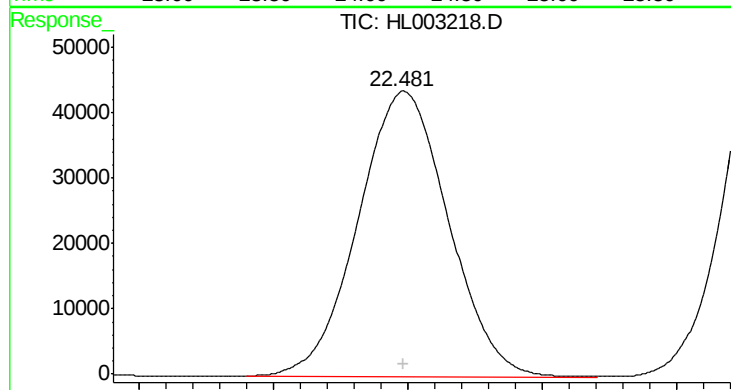


#10 2,6-Dinitrotoluene

R.T.: 22.484 min
Delta R.T.: 0.000 min
Response: 10212175
Conc: 492.90 ug/L

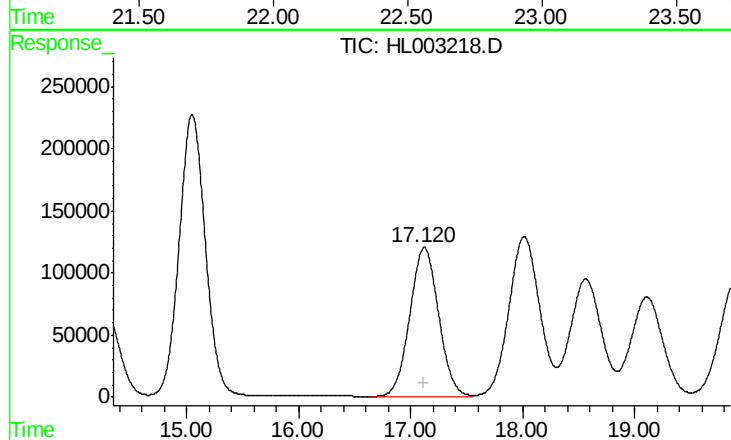


#11 1,3-Dinitrobenzene

R.T.: 17.122 min
Delta R.T.: 0.000 min
Response: 21422603
Conc: 521.23 ug/L

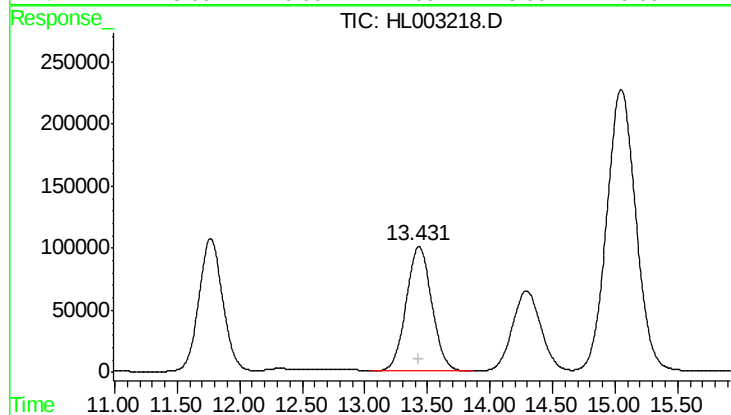

#12 Nitrobenzene


R.T.: 13.433 min
Delta R.T.: 0.000 min
Response: 14261408
Conc: 508.48 ug/L

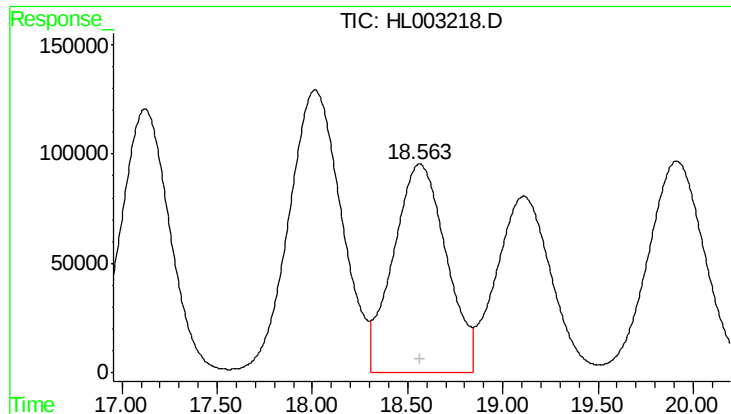

#13 2-Nitrotoluene


R.T.: 18.565 min
Delta R.T.: 0.000 min
Response: 18396024
Conc: 1009.12 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL01

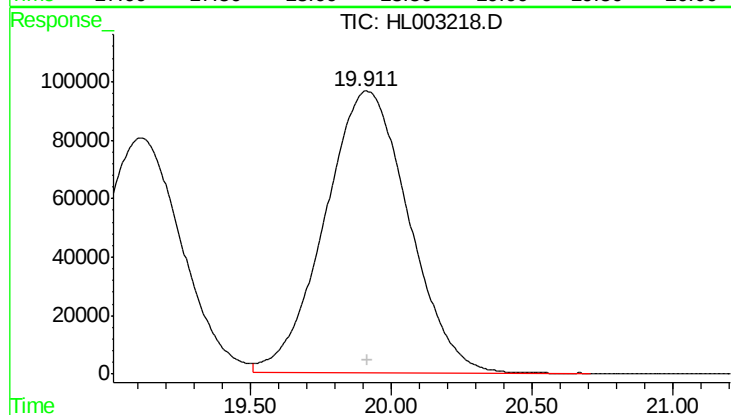


#14 3-Nitrotoluene

R.T.: 19.913 min
Delta R.T.: 0.000 min
Response: 20102850
Conc: 1010.92 ug/L

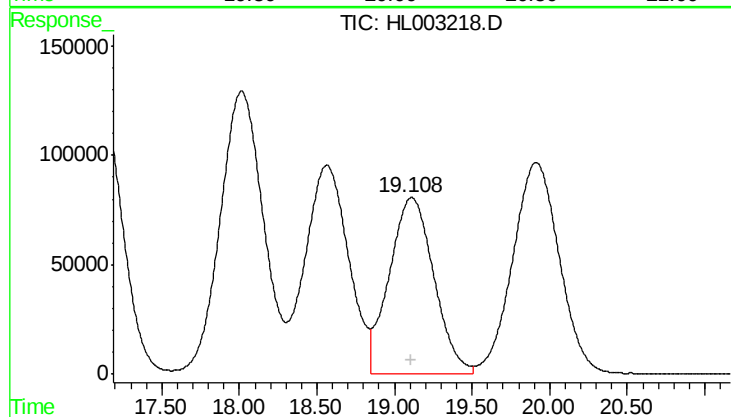

#15 4-Nitrotoluene

R.T.: 19.110 min
Delta R.T.: 0.000 min
Response: 16073484
Conc: 1000.09 ug/L

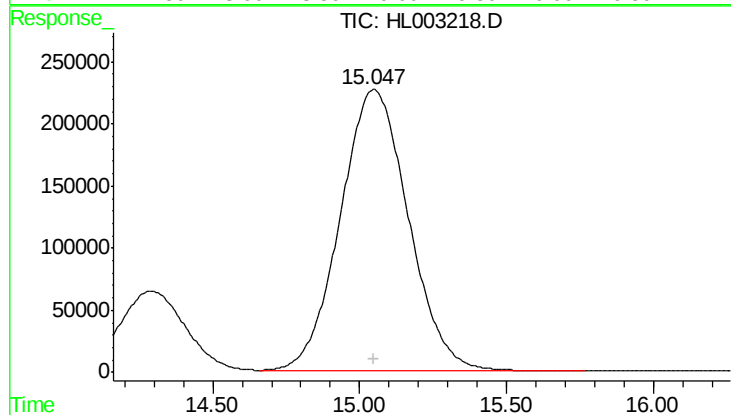

#16 3,5-Dinitroaniline

R.T.: 15.049 min
Delta R.T.: 0.000 min
Response: 36727182
Conc: 1023.72 ug/L

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060812\
 Data File : HL003218.D
 Signal(s) : VWD1A.CH
 Acq On : 08-Jun-2012, 16:05
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 CCAL01

Integration File: events.e
 Quant Time: Jun 14 04:22:14 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL053012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Thu May 31 11:08:18 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc	Units

System Monitoring Compounds				
1) S 4-Nitroaniline	8.308	10546923	1040.521	ug/L
Target Compounds				
2) T HMX	14.292	10260341	1037.944	ug/L
3) T RDX	11.767	14018954	1020.957	ug/L
4) T 1,3,5-Trinitrobenzene	26.562	15409847	553.483	ug/L
5) T Tetryl	39.027	21928442	1032.357	ug/L
6) T 2,4,6-Trinitrotoluene	36.395	13729851	509.580	ug/L
7) T 2-Amino-4,6-dinitroto...	18.014	24697240	512.996	ug/L
8) T 4-Amino-2,6-dinitroto...	18.014	24697240	510.480	ug/L
9) T 2,4-Dinitrotoluene	23.916	20453421	524.811	ug/L
10) T 2,6-Dinitrotoluene	22.484	10212175	492.895	ug/L
11) T 1,3-Dinitrobenzene	17.122	21422603	521.225	ug/L
12) T Nitrobenzene	13.433	14261408	508.475	ug/L
13) T 2-Nitrotoluene	18.565	18396024	1009.118	ug/L
14) T 3-Nitrotoluene	19.913	20102850	1010.917	ug/L
15) T 4-Nitrotoluene	19.110	16073484	1000.085	ug/L
16) T 3,5-Dinitroaniline	15.049	36727182	1023.718	ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.