

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060812\
Data File : HL003220.D
Signal(s) : VWD1A.CH
Acq On : 08-Jun-2012, 17:49
Operator : HLM
Sample : D2921-06RE
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
B1222SD-01ARE


Manual Integrations
APPROVED

AHPatel
6/19/2012 2:20:24 AM

Integration File: events.e
Quant Time: Jun 14 04:22:21 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL053012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Mon Jun 11 13:45:56 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

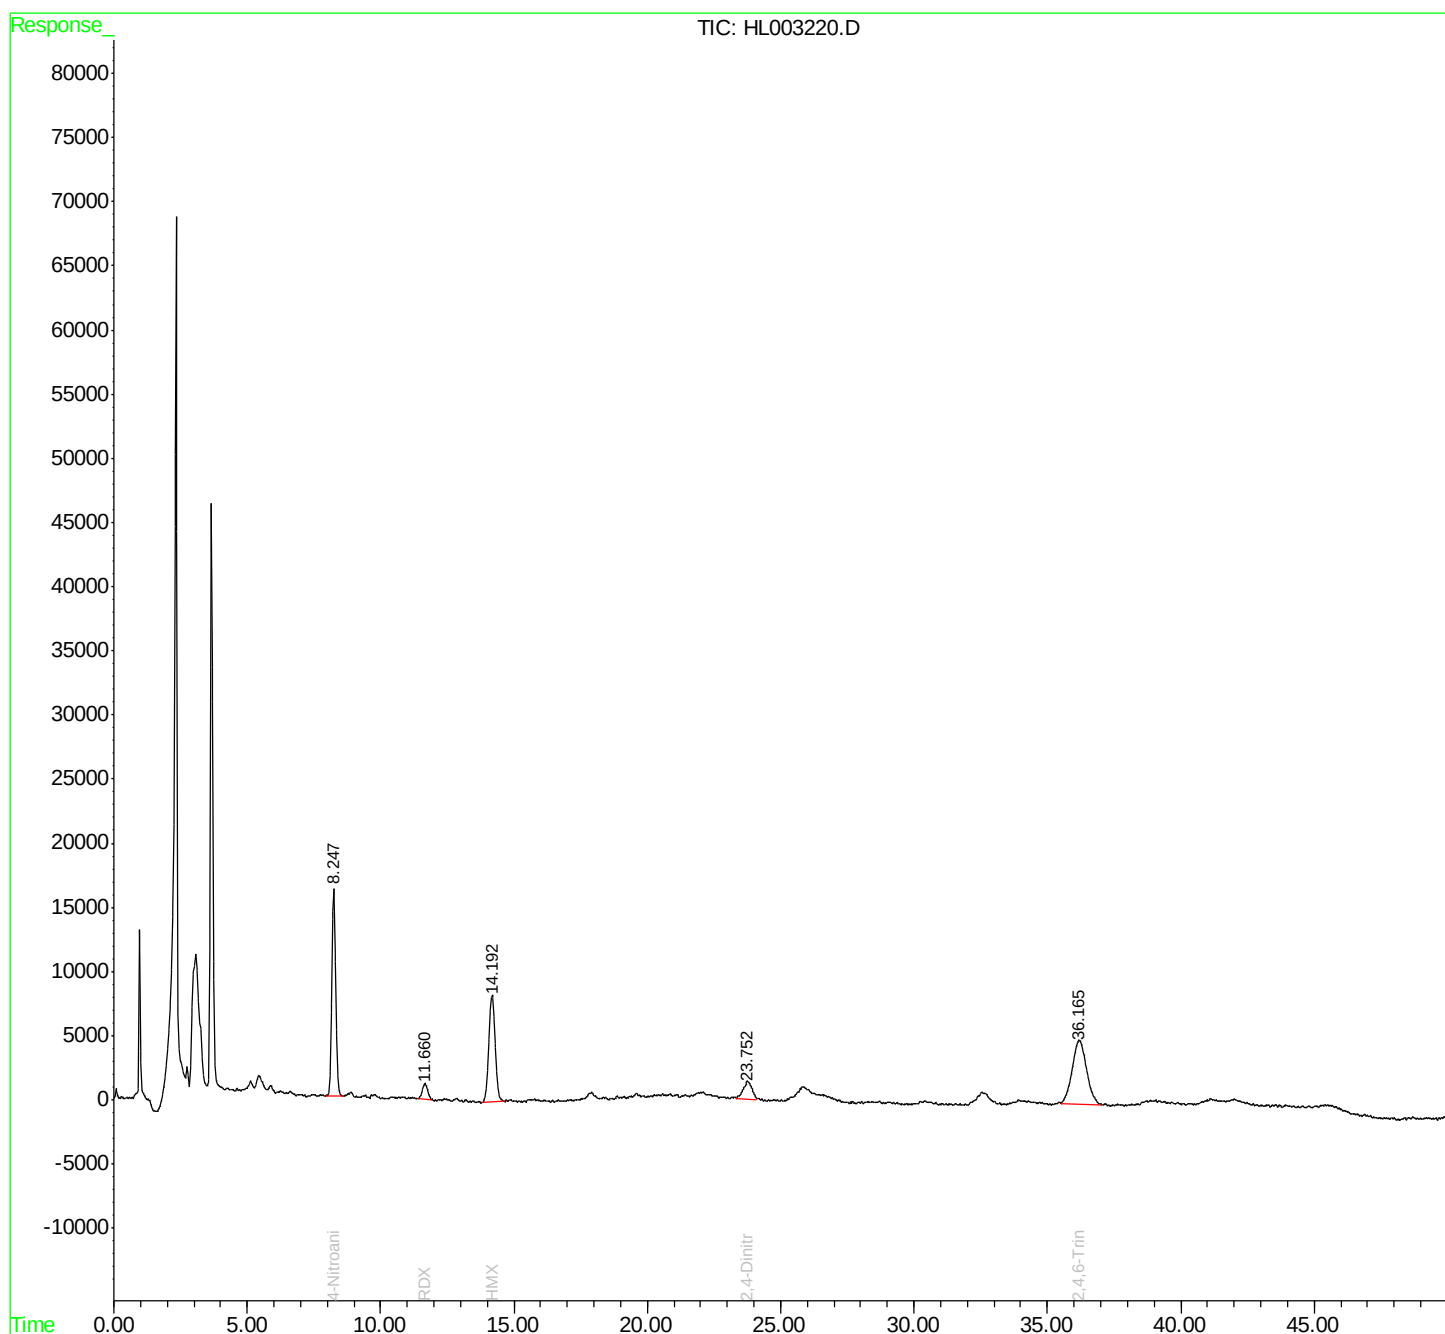

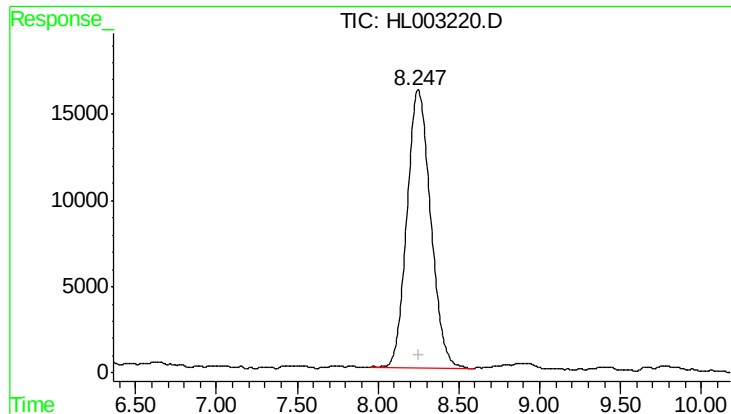


#1 4-Nitroaniline

R.T.: 8.250 min
Delta R.T.: 0.000 min
Response: 1640111
Conc: 161.81 ug/L

Instrument :
HPLC_L
ClientSampleId :
B1222SD-01ARE


Manual Integrations
APPROVED

AHPatel
6/19/2012 2:20:24 AM

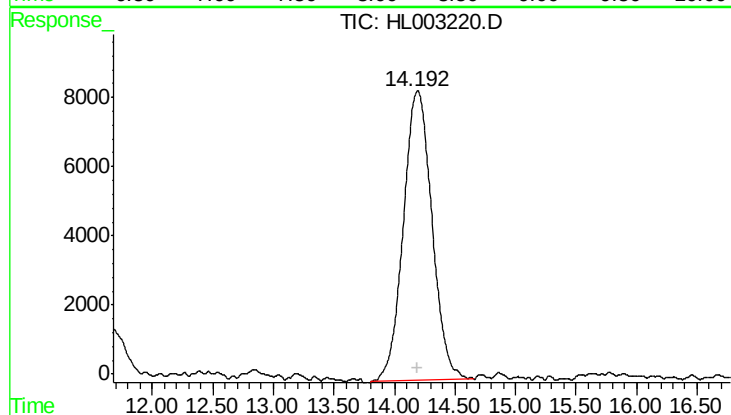


#2 HMX

R.T.: 14.194 min
Delta R.T.: 0.007 min
Response: 1376692
Conc: 139.27 ug/L

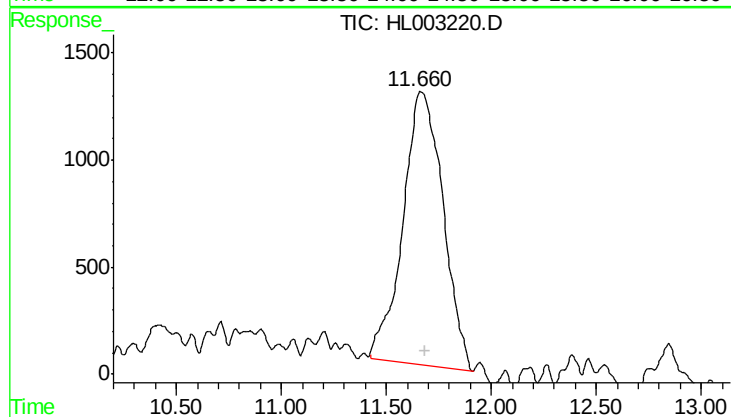


#3 RDX

R.T.: 11.660 min
Delta R.T.: -0.025 min
Response: 169757
Conc: 12.36 ug/L m

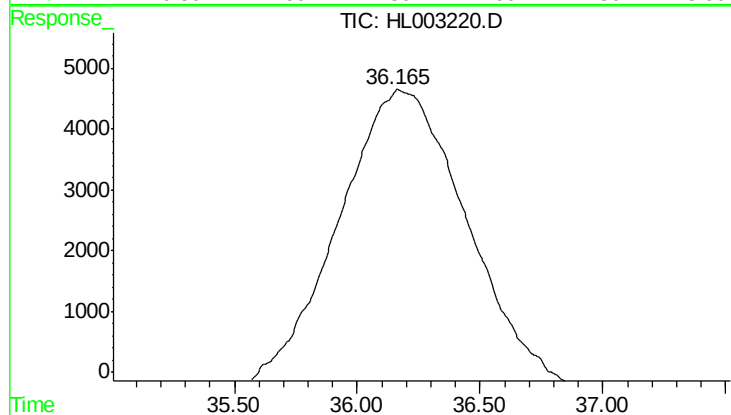

#6 2,4,6-Trinitrotoluene

R.T.: 36.169 min
Delta R.T.: 0.000 min
Response: 1852653
Conc: 68.76 ug/L

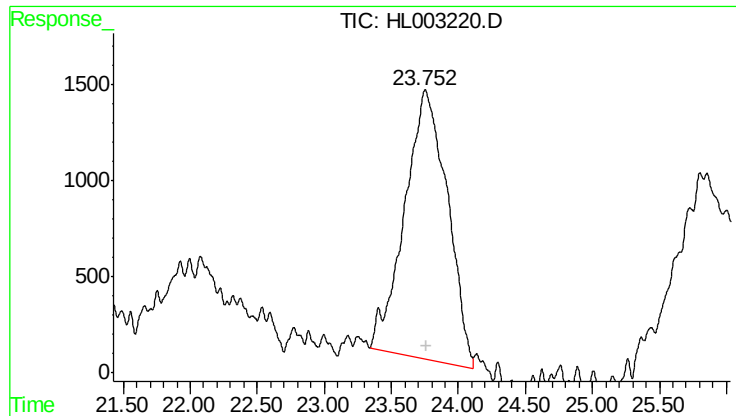

#9 2,4-Dinitrotoluene

R.T.: 23.752 min
Delta R.T.: -0.009 min
Response: 312676
Conc: 8.02 ug/L m

Instrument :
HPLC_L
ClientSampleId :
B1222SD-01ARE

Manual Integrations
APPROVED

AHPatel
6/19/2012 2:20:24 AM

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060812\
Data File : HL003220.D
Signal(s) : VWD1A.CH
Acq On : 08-Jun-2012, 17:49
Operator : HLM
Sample : D2921-06RE
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
B1222SD-01ARE

Manual Integrations
APPROVED

AHPatel
6/19/2012 2:20:24 AM

Integration File: events.e
Quant Time: Jun 14 04:22:21 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL053012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Mon Jun 11 13:45:56 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	8.250	1640111	161.807 ug/L
Target Compounds			
2) T HMX	14.194	1376692	139.267 ug/L
3) T RDX	11.660	169757	12.363 ug/L m
6) T 2,4,6-Trinitrotoluene	36.169	1852653	68.761 ug/L
9) T 2,4-Dinitrotoluene	23.752	312676	8.023 ug/L m

(f)=RT Delta > 1/2 Window

(m)=manual int.