



Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060812\
Data File : HL003231.D
Signal(s) : VWD1A.CH
Acq On : 09-Jun-2012, 03:21
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
CCAL03

Integration File: events.e
Quant Time: Jun 14 04:23:19 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL053012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Mon Jun 11 13:45:56 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

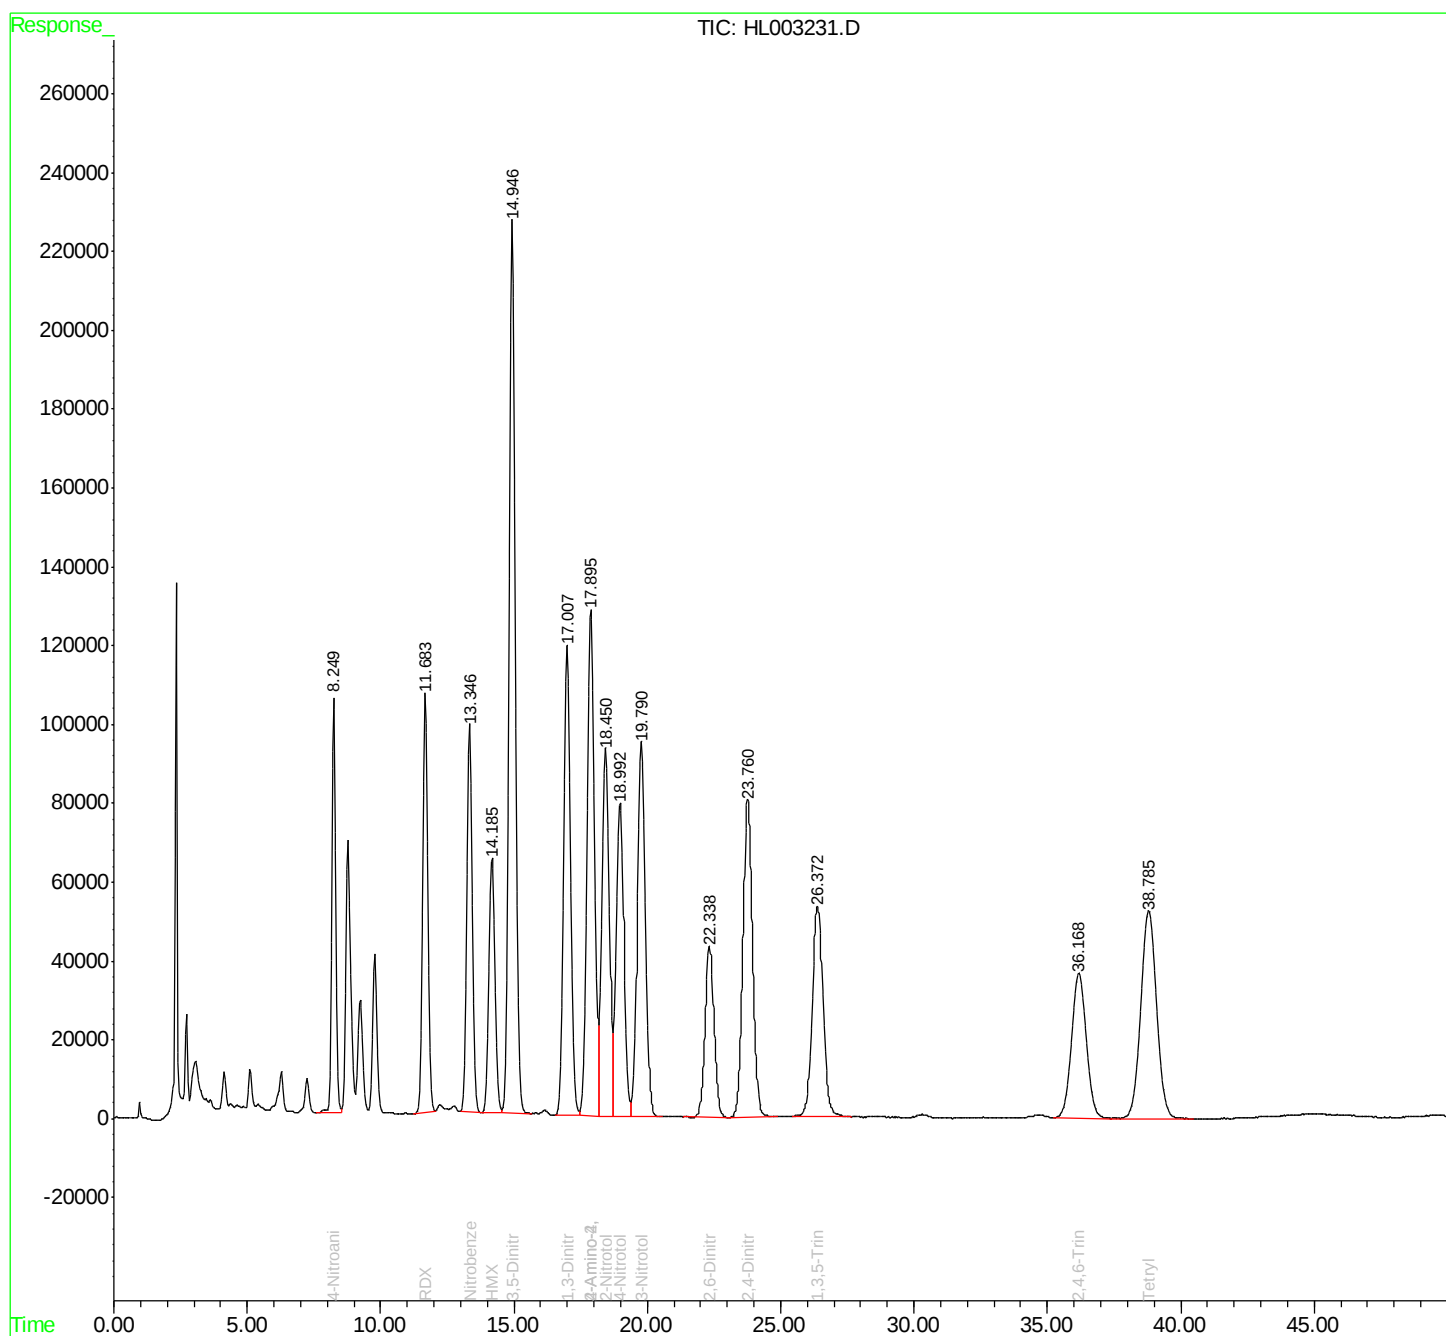


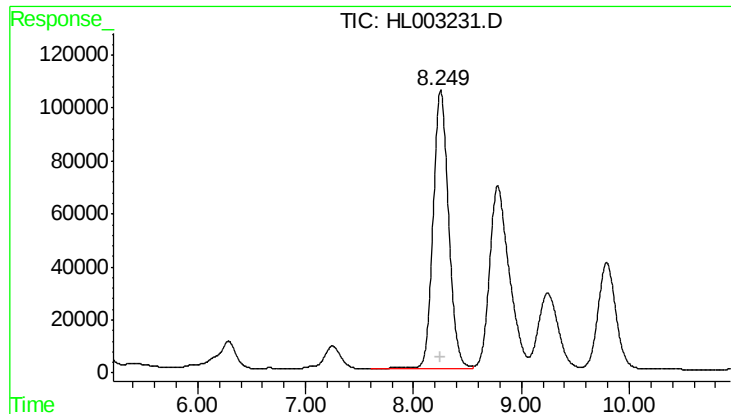

#1 4-Nitroaniline


R.T.: 8.251 min
Delta R.T.: 0.002 min
Response: 10535913
Conc: 1039.43 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL03

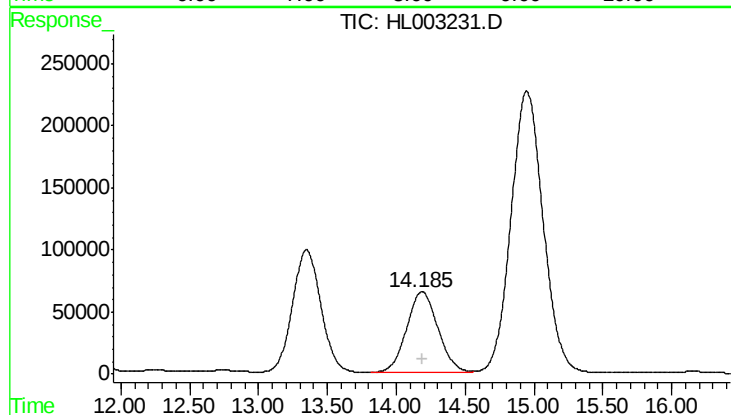


#2 HMX

R.T.: 14.187 min
Delta R.T.: 0.000 min
Response: 10269946
Conc: 1038.92 ug/L

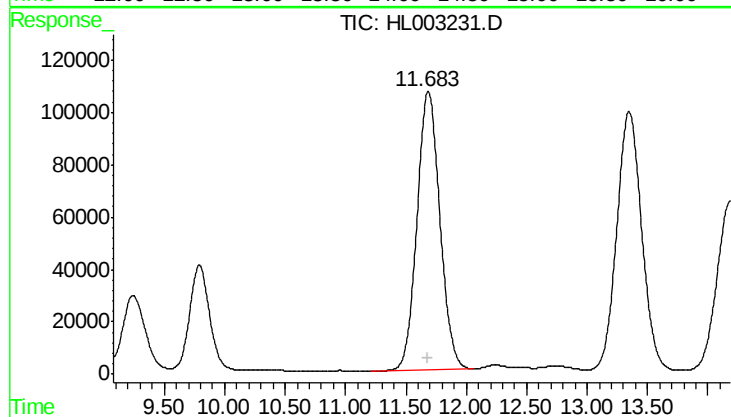


#3 RDX

R.T.: 11.685 min
Delta R.T.: 0.000 min
Response: 14016647
Conc: 1020.79 ug/L

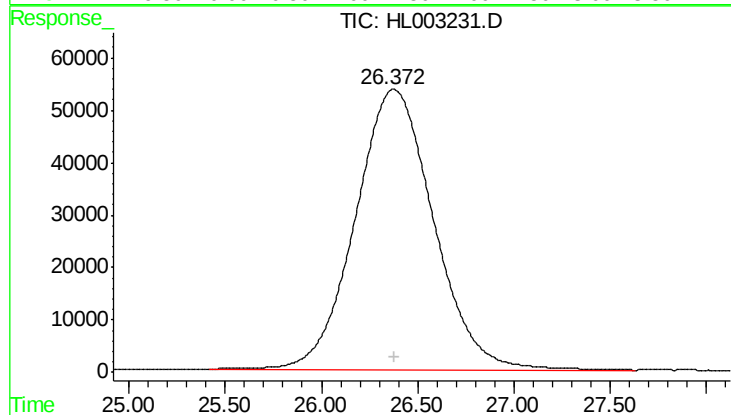

#4 1,3,5-Trinitrobenzene


R.T.: 26.377 min
Delta R.T.: 0.000 min
Response: 15155172
Conc: 544.34 ug/L

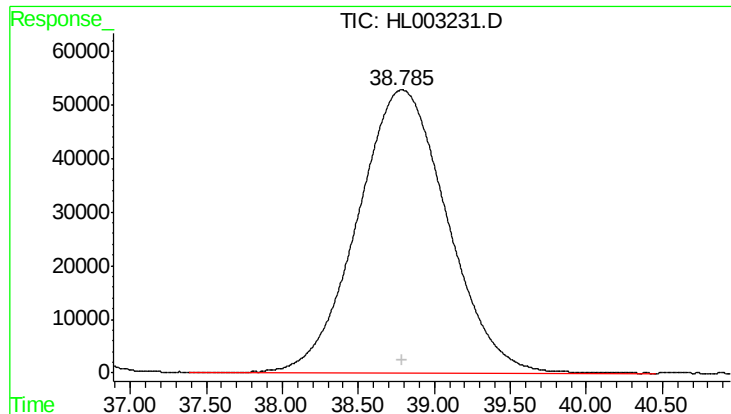

#5 Tetryl


R.T.: 38.787 min
Delta R.T.: 0.000 min
Response: 21774294
Conc: 1025.10 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL03

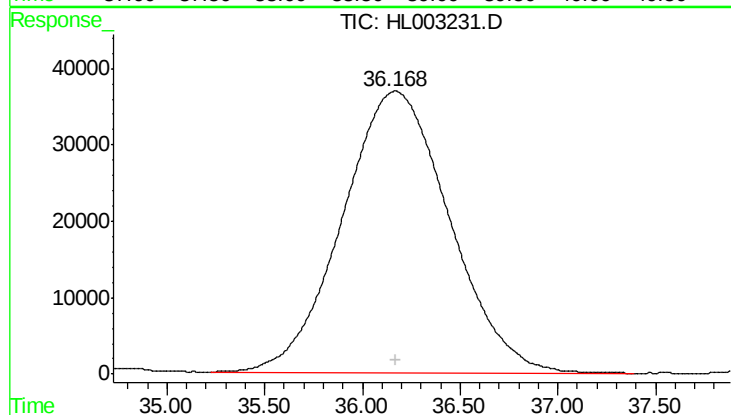


#6 2,4,6-Trinitrotoluene

R.T.: 36.169 min
Delta R.T.: 0.000 min
Response: 14134557
Conc: 524.60 ug/L

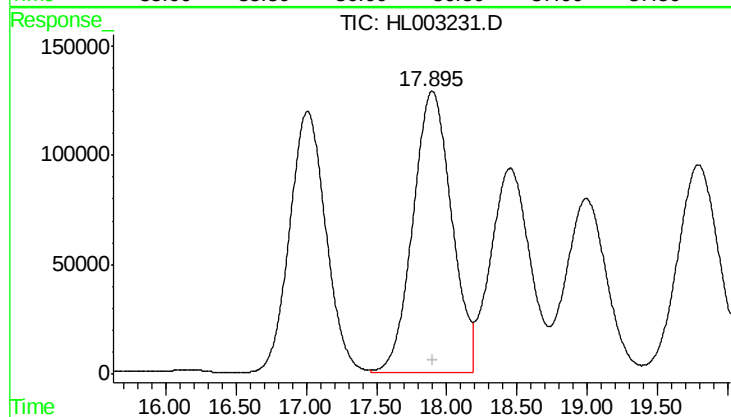


#7 2-Amino-4,6-dinitrotoluene

R.T.: 17.897 min
Delta R.T.: 0.000 min
Response: 24644301
Conc: 511.90 ug/L

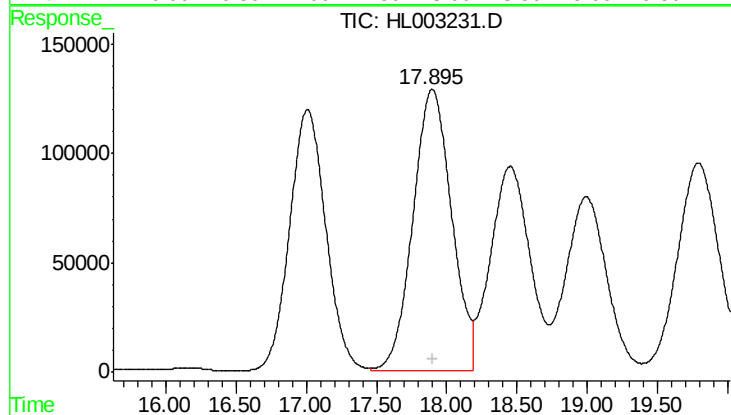

#8 4-Amino-2,6-dinitrotoluene


R.T.: 17.897 min
Delta R.T.: 0.000 min
Response: 24644301
Conc: 509.39 ug/L

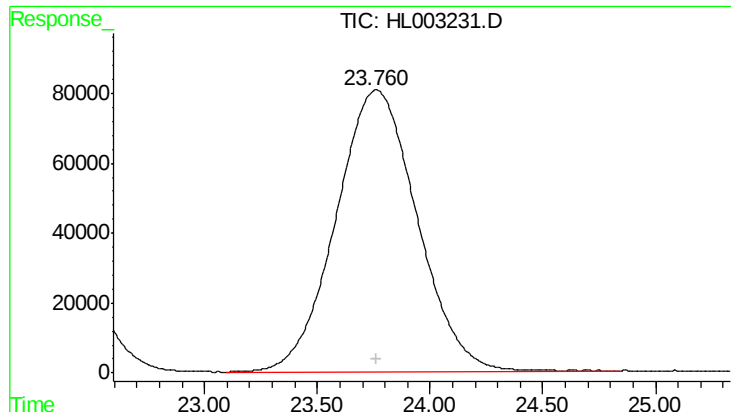

#9 2,4-Dinitrotoluene


R.T.: 23.761 min
Delta R.T.: 0.000 min
Response: 20180443
Conc: 517.81 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL03

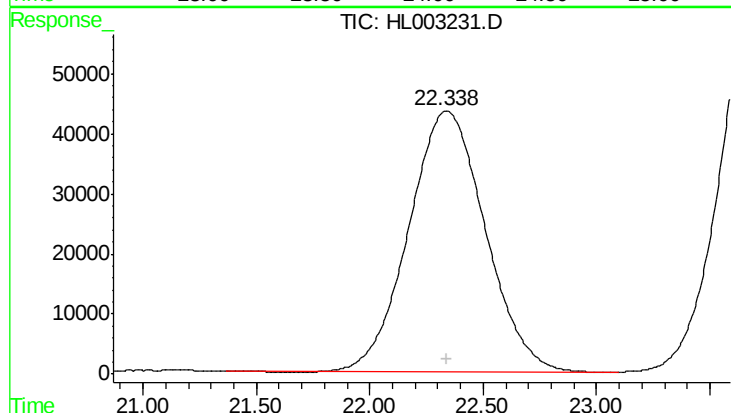


#10 2,6-Dinitrotoluene

R.T.: 22.340 min
Delta R.T.: 0.000 min
Response: 10224131
Conc: 493.47 ug/L

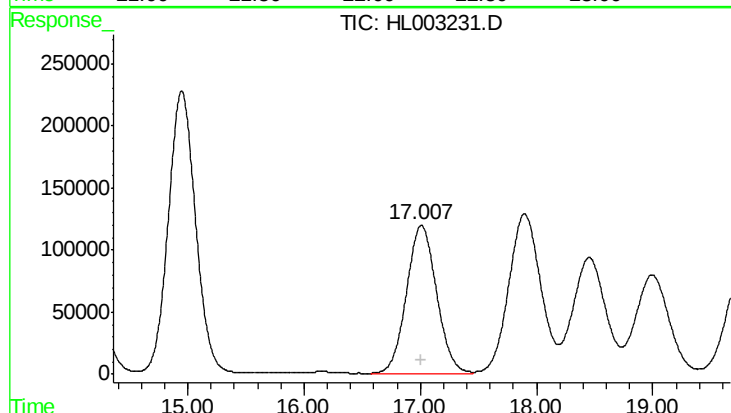


#11 1,3-Dinitrobenzene

R.T.: 17.009 min
Delta R.T.: 0.000 min
Response: 21403970
Conc: 520.77 ug/L

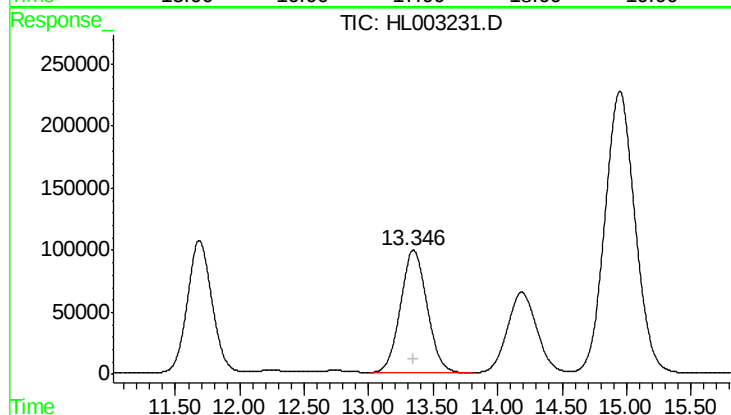

#12 Nitrobenzene


R.T.: 13.348 min
Delta R.T.: 0.000 min
Response: 14050630
Conc: 500.96 ug/L

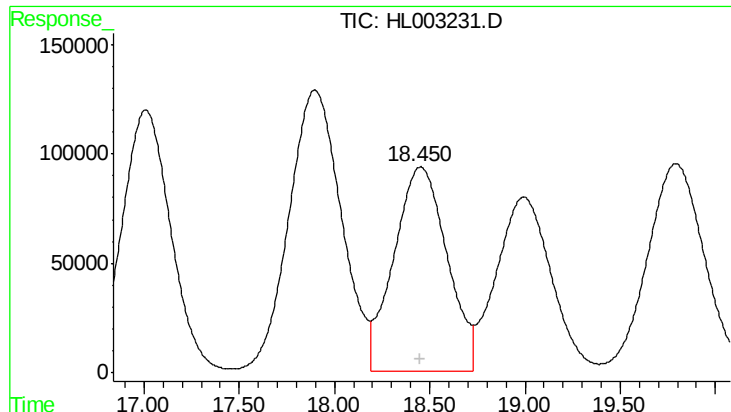

#13 2-Nitrotoluene


R.T.: 18.452 min
Delta R.T.: 0.000 min
Response: 18200561
Conc: 998.40 ug/L

Instrument :
HPLC_L
ClientSampleId :
CCAL03

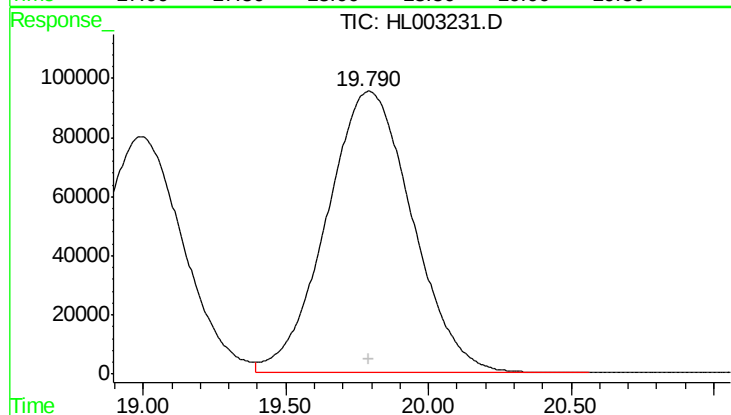


#14 3-Nitrotoluene

R.T.: 19.792 min
Delta R.T.: 0.000 min
Response: 19902703
Conc: 1000.85 ug/L

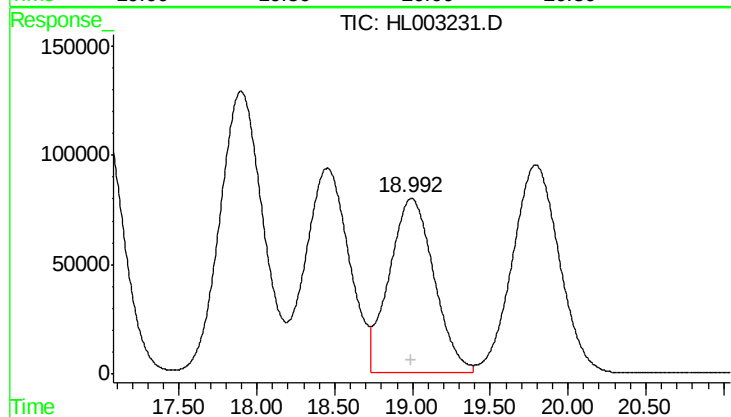

#15 4-Nitrotoluene

R.T.: 18.994 min
Delta R.T.: 0.000 min
Response: 16013785
Conc: 996.37 ug/L

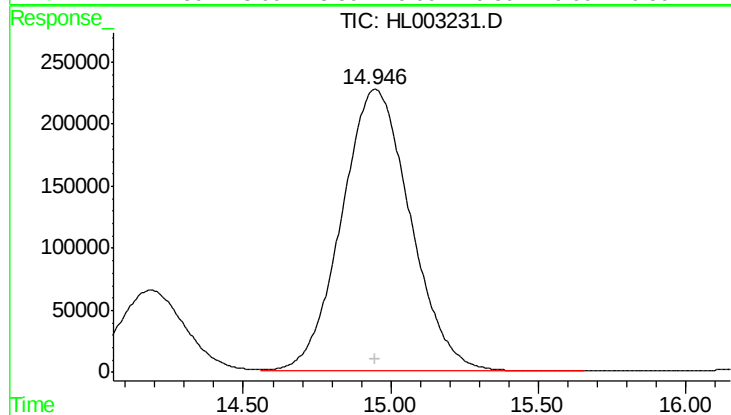

#16 3,5-Dinitroaniline

R.T.: 14.948 min
Delta R.T.: 0.000 min
Response: 36742277
Conc: 1024.14 ug/L

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL060812\
 Data File : HL003231.D
 Signal(s) : VWD1A.CH
 Acq On : 09-Jun-2012, 03:21
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 CCAL03

Integration File: events.e
 Quant Time: Jun 14 04:23:19 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL053012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Mon Jun 11 13:45:56 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc	Units

System Monitoring Compounds					
1) S	4-Nitroaniline	8.251	10535913	1039.435	ug/L
Target Compounds					
2) T	HMX	14.187	10269946	1038.915	ug/L
3) T	RDX	11.685	14016647	1020.789	ug/L
4) T	1,3,5-Trinitrobenzene	26.377	15155172	544.335	ug/L
5) T	Tetryl	38.787	21774294	1025.100	ug/L
6) T	2,4,6-Trinitrotoluene	36.169	14134557	524.601	ug/L
7) T	2-Amino-4,6-dinitroto...	17.897	24644301	511.896	ug/L
8) T	4-Amino-2,6-dinitroto...	17.897	24644301	509.385	ug/L
9) T	2,4-Dinitrotoluene	23.761	20180443	517.807	ug/L
10) T	2,6-Dinitrotoluene	22.340	10224131	493.472	ug/L
11) T	1,3-Dinitrobenzene	17.009	21403970	520.772	ug/L
12) T	Nitrobenzene	13.348	14050630	500.960	ug/L
13) T	2-Nitrotoluene	18.452	18200561	998.396	ug/L
14) T	3-Nitrotoluene	19.792	19902703	1000.852	ug/L
15) T	4-Nitrotoluene	18.994	16013785	996.371	ug/L
16) T	3,5-Dinitroaniline	14.948	36742277	1024.139	ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.