

Data File : H:\VOL1\HPLC\HPLC L\120615\HL003291.D Vial: 14
Acq On : 15-Jun-2012, 15:13 Operator: HLM
Sample : D3002-01 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jun 22 17:39 2012 Quant Results File: HL060712.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL060712.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Fri Jun 22 17:39:50 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.38	1273708	350.221 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 116.74%


Target Compounds


16) T	3,5-Dinitroaniline	4.08	831980	43.748 ug/L
-------	--------------------	------	--------	-------------

Data File : H:\VOL1\HPLC\HPLC L\120615\HL003291.D Vial: 14
Acq On : 15-Jun-2012, 15:13 Operator: HLM
Sample : D3002-01 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jun 22 17:39 2012 Quant Results File: HL060712.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL060712.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Fri Jun 22 17:39:50 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

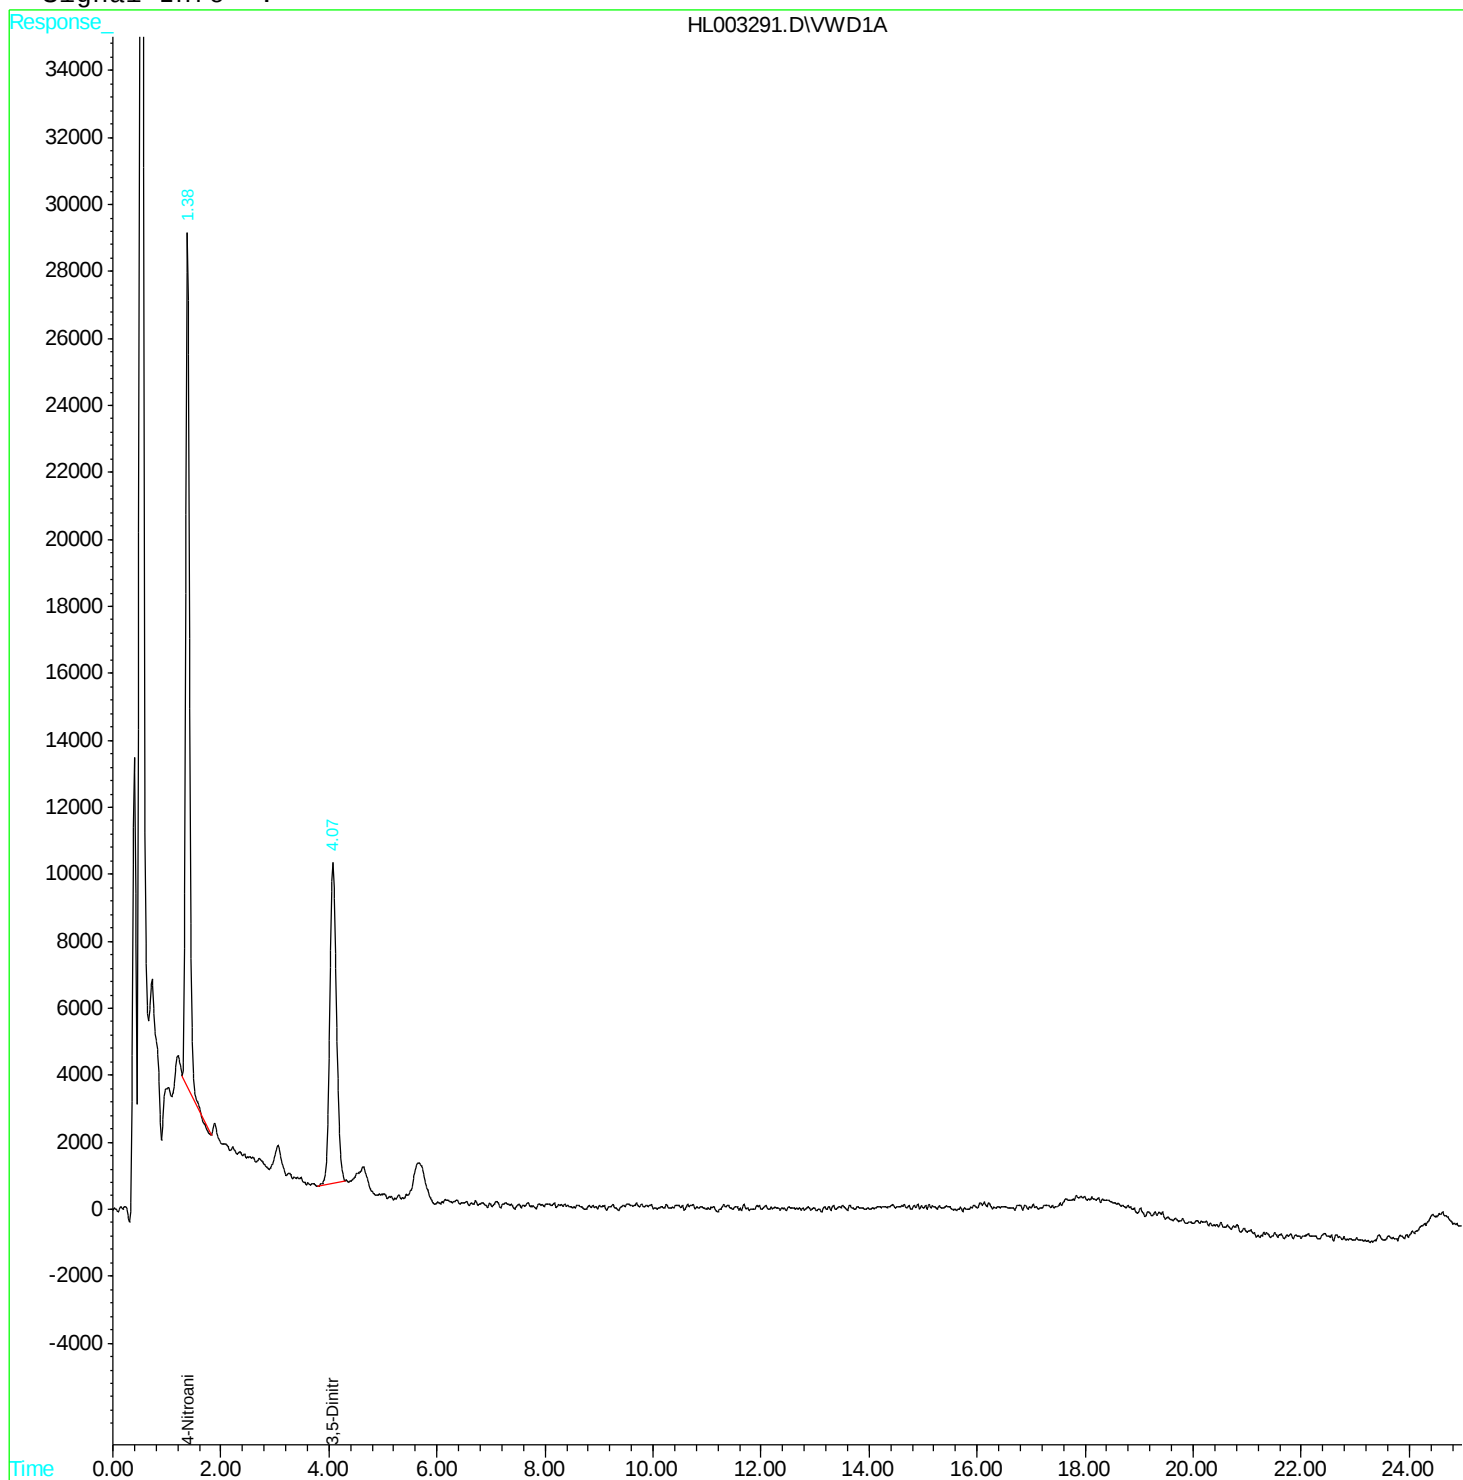

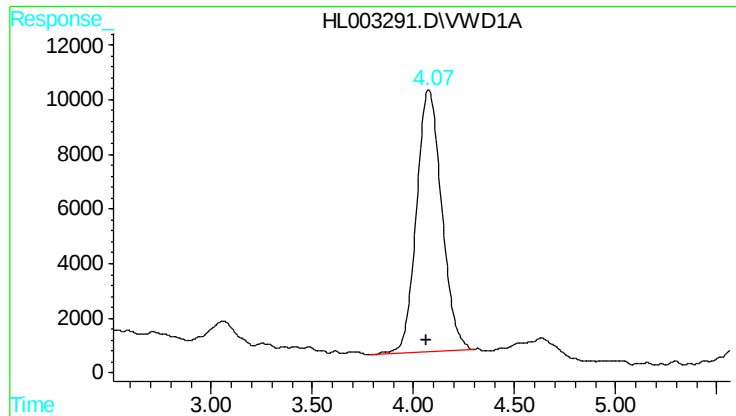

#16 3,5-Dinitroaniline

R.T.: 4.076 min
Delta R.T.: 0.011 min
Response: 831980
Conc: 43.75 ug/L