

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL061813\
 Data File : HL005432.D
 Signal(s) : VWD1A.CH
 Acq On : 18-Jun-2013, 23:20
 Operator : QM
 Sample : E1570-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 38172

Integration File: autoint1.e
 Quant Time: Jun 20 07:29:21 2013
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL061813.M
 Quant Title :
 QLast Update : Wed Jun 19 15:50:10 2013
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	5.514	2882767	290.111 ug/L m
Target Compounds				
2) T	HMX	4.109	5609803	618.236 ug/L
3) T	RDX	6.660	6204047	525.703 ug/L
4) T	1,3,5-Trinitrobenzene	9.288	21340658	852.044 ug/L
6) T	3,5-Dinitroaniline	12.258f	37373033	1155.364 ug/L m
7) T	Tetryl	13.347	6937748	333.985 ug/L m
8) T	Nitrobenzene	14.601	19527395	815.742 ug/L
9) T	2,4,6-Trinitrotoluene	15.947	10273666	403.465 ug/L m
11) T	2-Amino-4,6-dinitroto...	17.372	19457389	668.652 ug/L m
13) T	2,4-Dinitrotoluene	20.278	30084145	787.249 ug/L m
14) T	2-Nitrotoluene	24.904	10469929	685.585 ug/L m
15) T	4-Nitrotoluene	26.846	5769020	431.656 ug/L m
16) T	3-Nitrotoluene	29.028	6239801	388.400 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL061813\
Data File : HL005432.D
Signal(s) : VWD1A.CH
Acq On : 18-Jun-2013, 23:20
Operator : QM
Sample : E1570-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
38172

Integration File: autoint1.e
Quant Time: Jun 20 07:29:21 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL061813.M
Quant Title :
QLast Update : Wed Jun 19 15:50:10 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

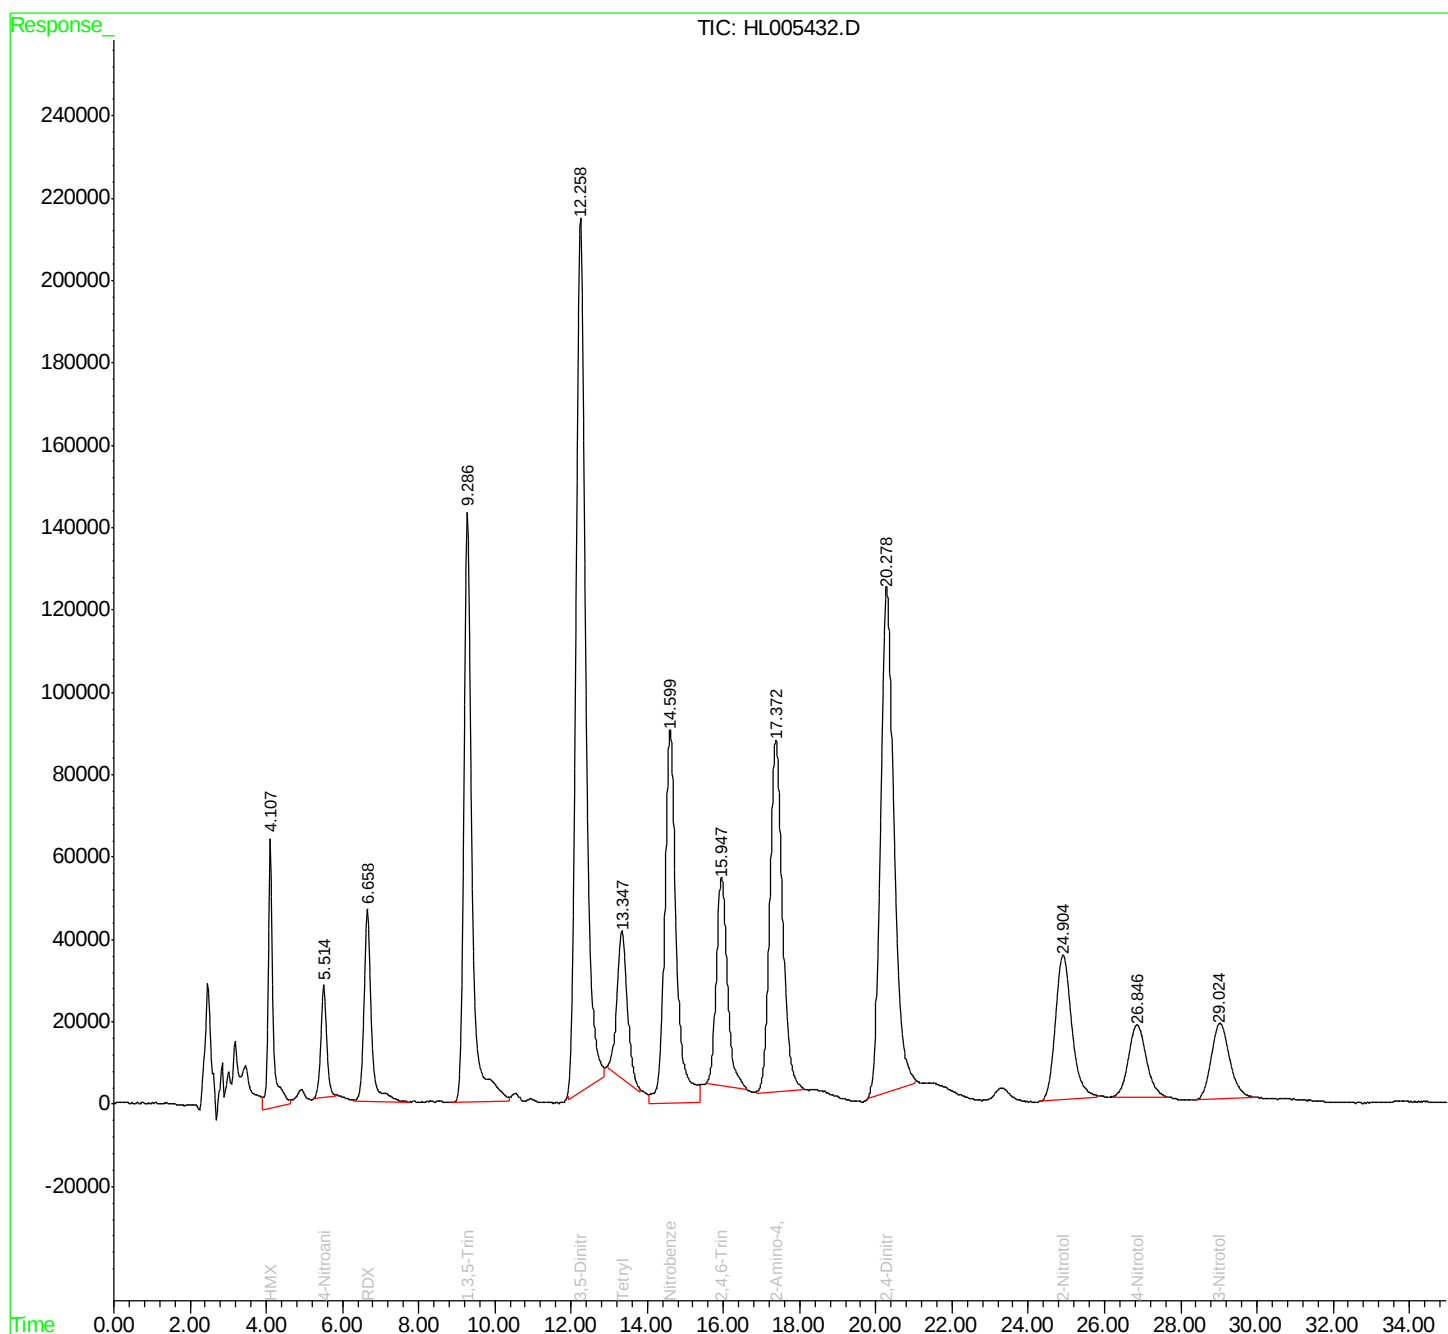


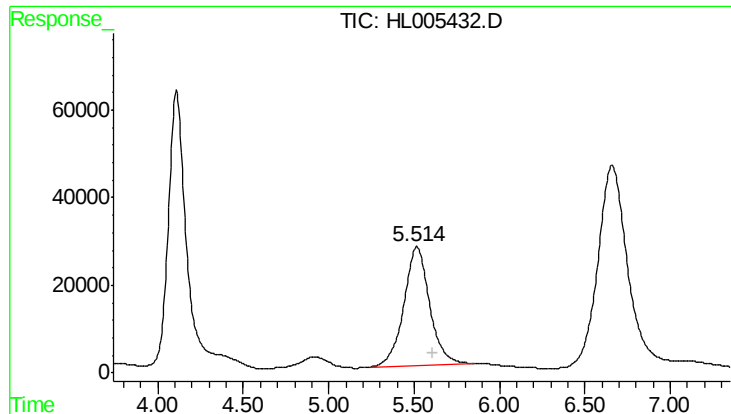

#1 4-Nitroaniline


R.T.: 5.514 min
Delta R.T.: -0.092 min
Response: 2882767
Conc: 290.11 ug/L

Instrument :
HPLC_L
ClientSampleId :
38172

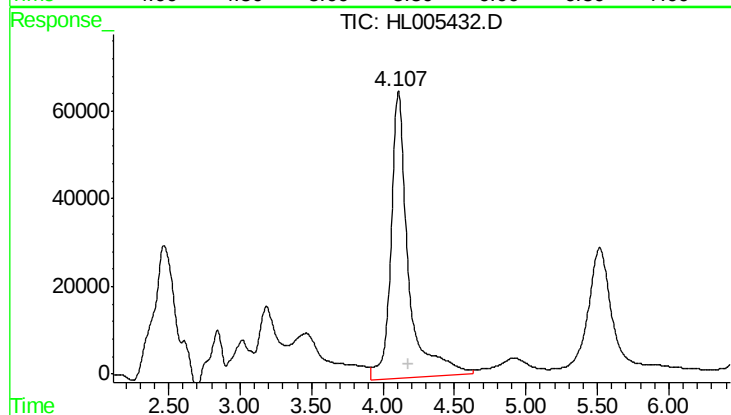


#2 HMX

R.T.: 4.109 min
Delta R.T.: -0.068 min
Response: 5609803
Conc: 618.24 ug/L

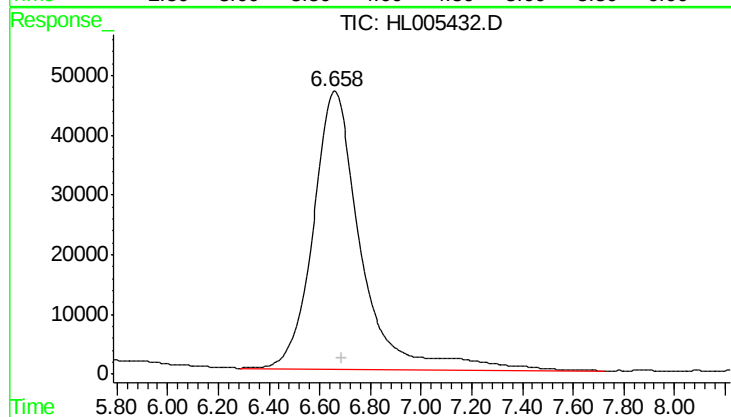


#3 RDX

R.T.: 6.660 min
Delta R.T.: -0.028 min
Response: 6204047
Conc: 525.70 ug/L

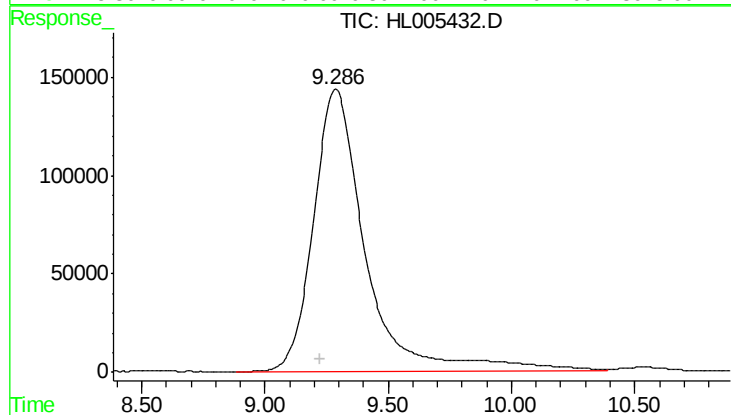

#4 1,3,5-Trinitrobenzene


R.T.: 9.288 min
Delta R.T.: 0.065 min
Response: 21340658
Conc: 852.04 ug/L

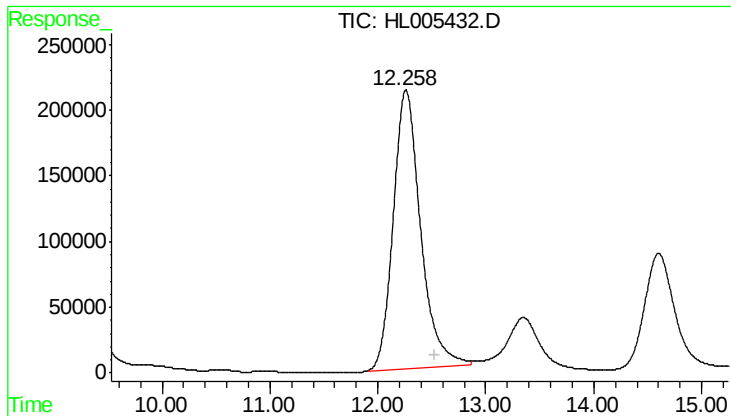

#6 3,5-Dinitroaniline


R.T.: 12.258 min
Delta R.T.: -0.262 min
Response: 37373033
Conc: 1155.36 ug/L

Instrument :
HPLC_L
ClientSampleId :
38172

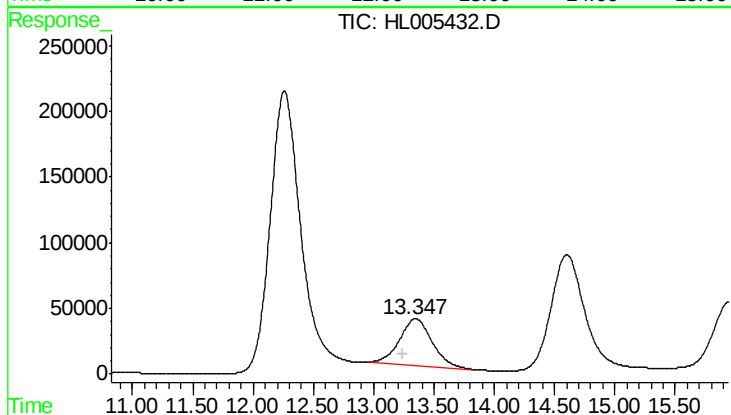


#7 Tetryl

R.T.: 13.347 min
Delta R.T.: 0.109 min
Response: 6937748
Conc: 333.98 ug/L m

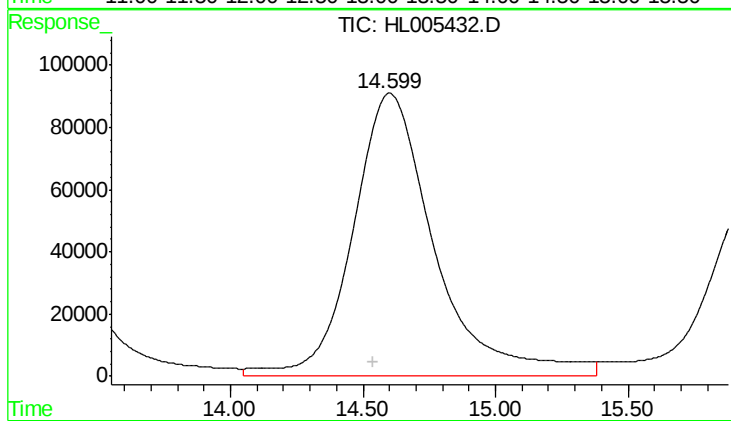


#8 Nitrobenzene

R.T.: 14.601 min
Delta R.T.: 0.061 min
Response: 19527395
Conc: 815.74 ug/L

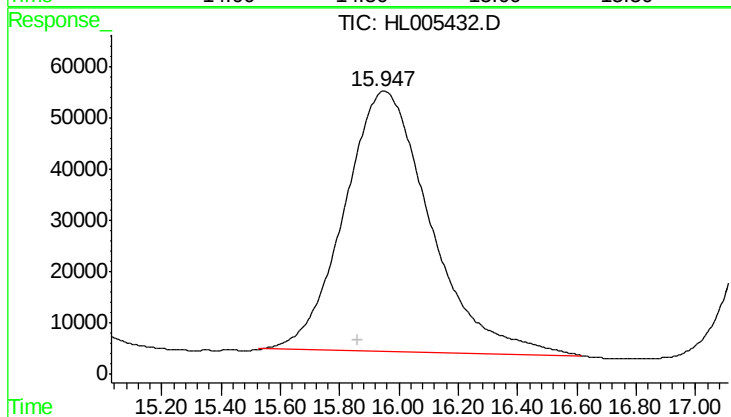

#9 2,4,6-Trinitrotoluene


R.T.: 15.947 min
Delta R.T.: 0.087 min
Response: 10273666
Conc: 403.47 ug/L m

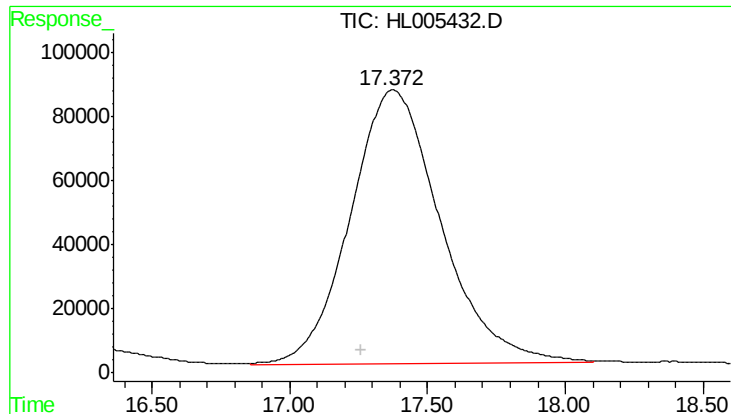

#11 2-Amino-4,6-dinitrotoluene


R.T.: 17.372 min
Delta R.T.: 0.112 min
Response: 19457389
Conc: 668.65 ug/L m

Instrument :
HPLC_L
ClientSampleId :
38172

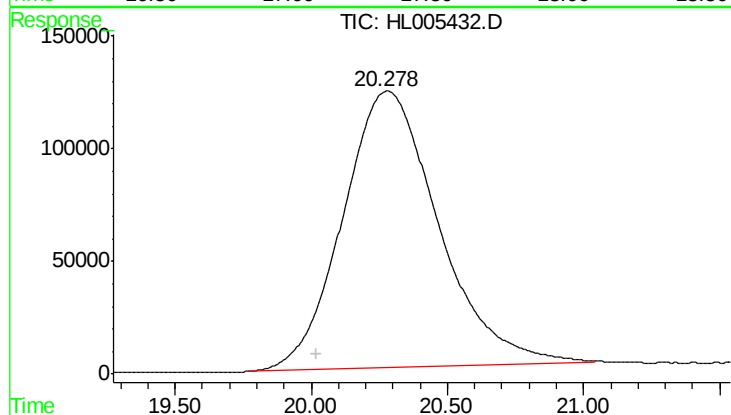


#13 2,4-Dinitrotoluene

R.T.: 20.278 min
Delta R.T.: 0.258 min
Response: 30084145
Conc: 787.25 ug/L m

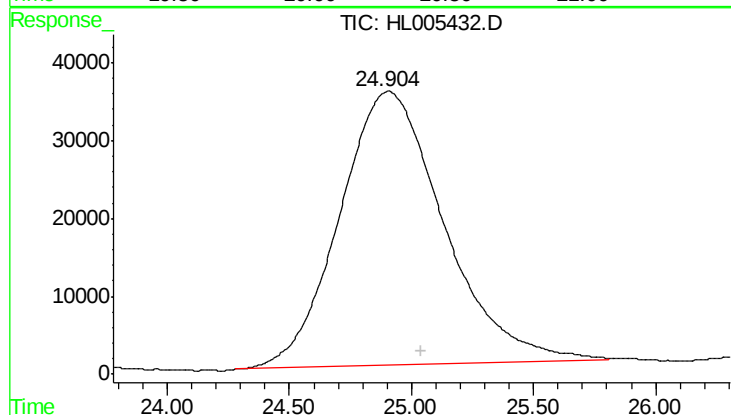


#14 2-Nitrotoluene

R.T.: 24.904 min
Delta R.T.: -0.136 min
Response: 10469929
Conc: 685.58 ug/L m

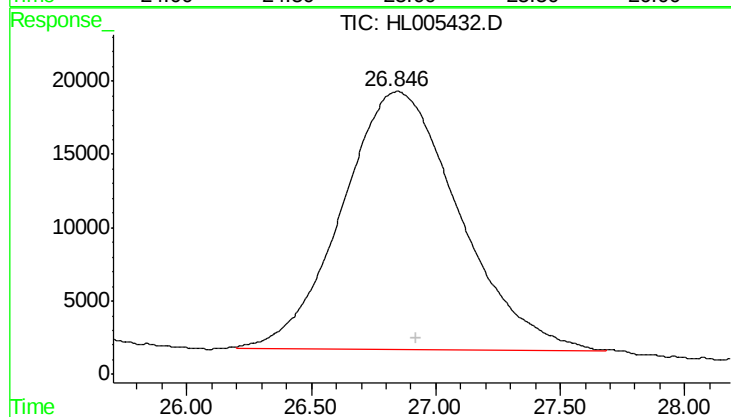

#15 4-Nitrotoluene

R.T.: 26.846 min
Delta R.T.: -0.074 min
Response: 5769020
Conc: 431.66 ug/L m

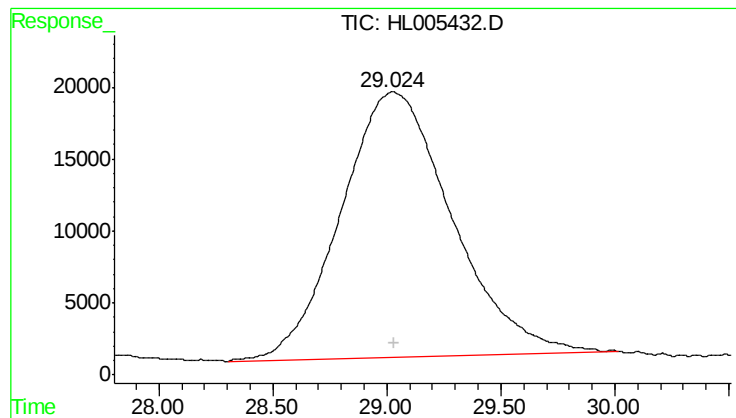

#16 3-Nitrotoluene

R.T.: 29.028 min
Delta R.T.: -0.002 min
Response: 6239801
Conc: 388.40 ug/L

Instrument :
HPLC_L
ClientSampleId :
38172