

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL061813\
 Data File : HL005434.D
 Signal(s) : VWD1A.CH
 Acq On : 19-Jun-2013, 00:34
 Operator : QM
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 HPLC_L
 LabSampleId :
 HSTDCCC0500

Integration File: autoint1.e
 Quant Time: Jun 20 07:28:01 2013
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL061813.M
 Quant Title :
 QLast Update : Wed Jun 19 16:03:01 2013
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	5.694	4935163	496.657 ug/L
Target Compounds			
2) T HMX	4.263	4513052	497.367 ug/L
3) T RDX	6.781	5755577	487.702 ug/L
4) T 1,3,5-Trinitrobenzene	9.304	13981244	558.213 ug/L
5) T 1,3-Dinitrobenzene	12.358	18180360	531.002 ng/ml
6) T 3,5-Dinitroaniline	12.748	17343403	536.160 ug/L
7) T Tetryl	13.398	11007324	529.895 ug/L
8) T Nitrobenzene	14.604	12341922	515.575 ug/L
9) T 2,4,6-Trinitrotoluene	15.917	12632779	496.112 ug/L
10) T 4-Amino-2,6-dinitroto...	16.540	9443247	528.376 ug/L
11) T 2-Amino-4,6-dinitroto...	17.301	14937691	513.333 ug/L
12) T 2,6-Dinitrotoluene	19.648	7235428	504.160 ug/L
13) T 2,4-Dinitrotoluene	20.161	19272967	504.339 ug/L
14) T 2-Nitrotoluene	24.779	7725263	505.860 ug/L
15) T 4-Nitrotoluene	26.782	6956656	520.518 ug/L
16) T 3-Nitrotoluene	29.015	8004368	498.236 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL061813\
Data File : HL005434.D
Signal(s) : VWD1A.CH
Acq On : 19-Jun-2013, 00:34
Operator : QM
Sample : HSTDCCC0500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
HSTDCCC0500

Integration File: autoint1.e
Quant Time: Jun 20 07:28:01 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL061813.M
Quant Title :
QLast Update : Wed Jun 19 16:03:01 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

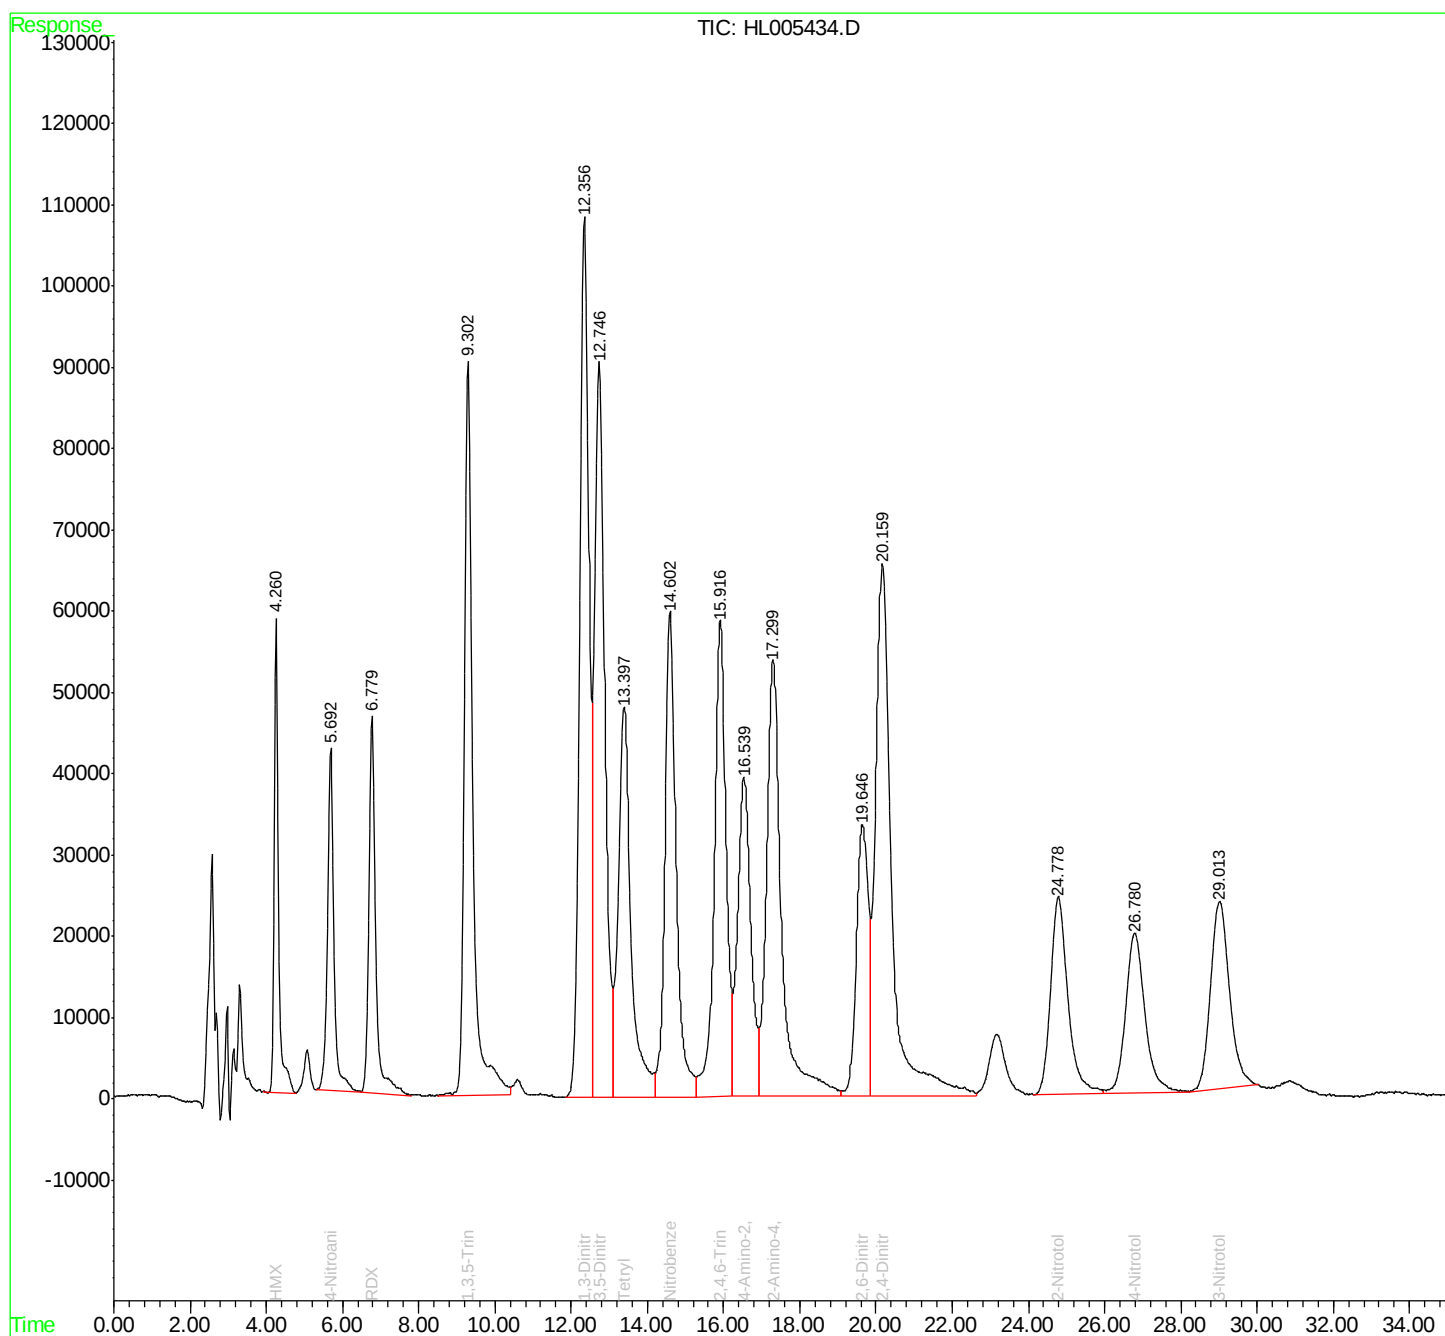


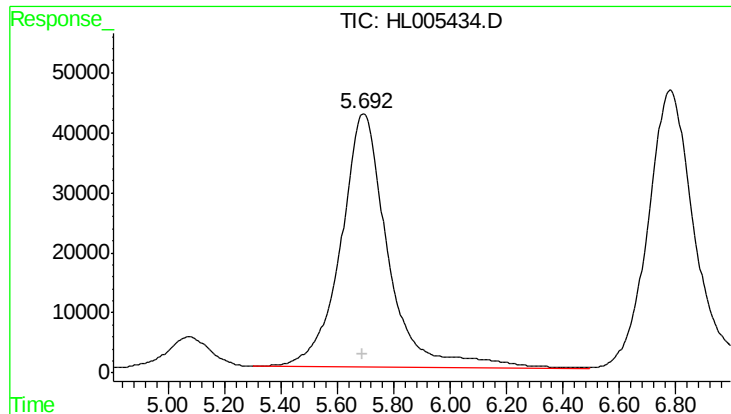

#1 4-Nitroaniline


R.T.: 5.694 min
Delta R.T.: 0.004 min
Response: 4935163
Conc: 496.66 ug/L

Instrument :
HPLC_L
LabSampleId :
HSTDCCC0500

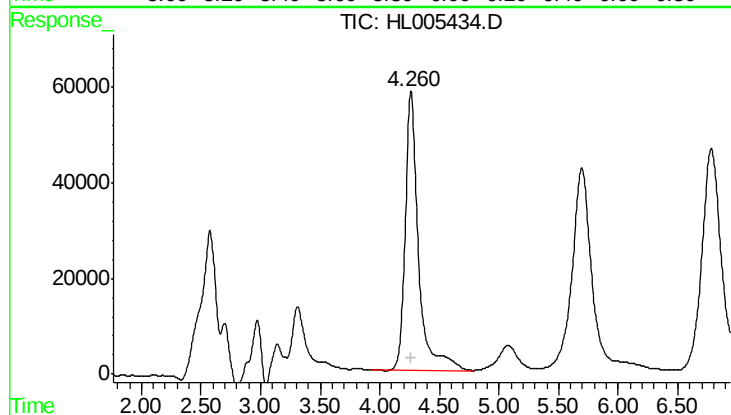


#2 HMX

R.T.: 4.263 min
Delta R.T.: 0.003 min
Response: 4513052
Conc: 497.37 ug/L

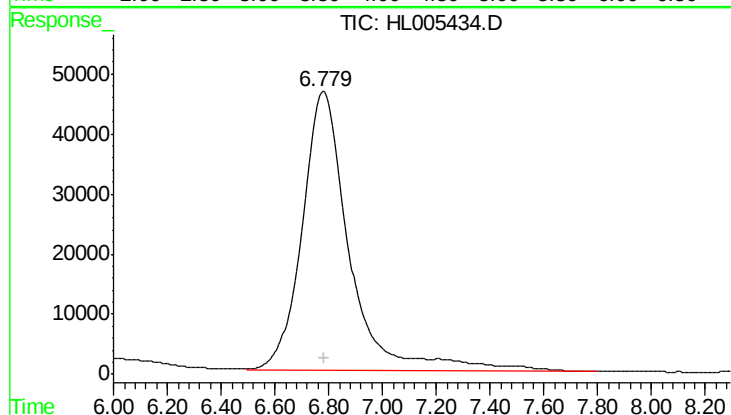


#3 RDX

R.T.: 6.781 min
Delta R.T.: 0.001 min
Response: 5755577
Conc: 487.70 ug/L

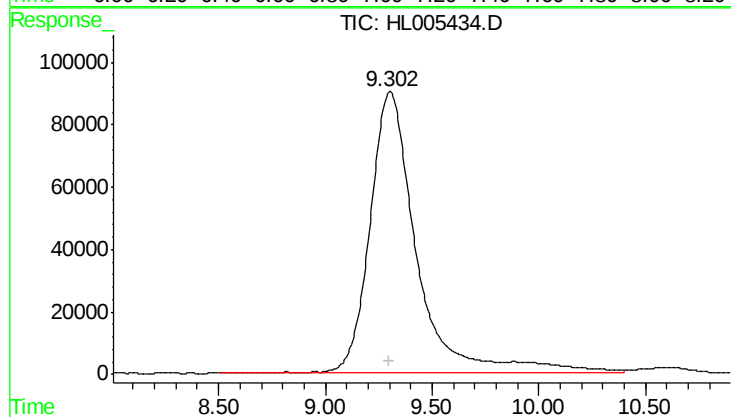

#4 1,3,5-Trinitrobenzene


R.T.: 9.304 min
Delta R.T.: 0.004 min
Response: 13981244
Conc: 558.21 ug/L

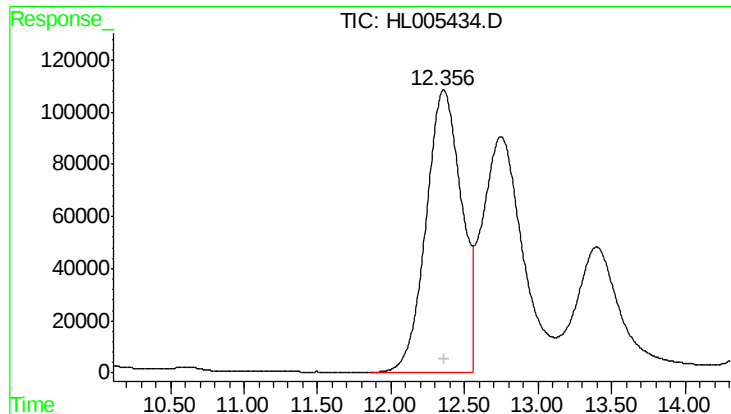

#5 1,3-Dinitrobenzene


R.T.: 12.358 min
 Delta R.T.: -0.002 min
 Response: 18180360
 Conc: 531.00 ng/ml

Instrument :
 HPLC_L
 LabSampleId :
 HSTDCCC0500

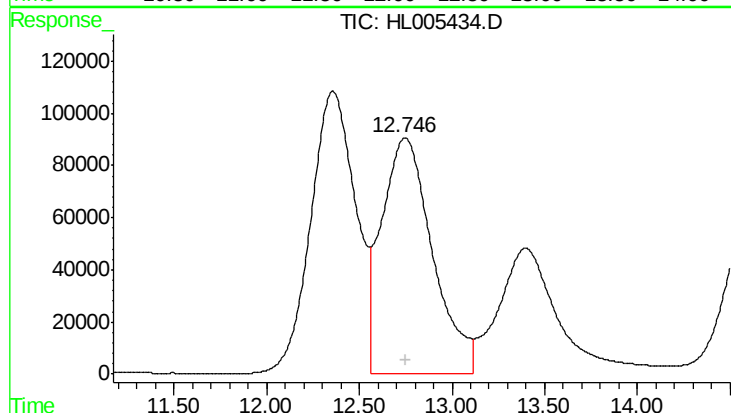


#6 3,5-Dinitroaniline

R.T.: 12.748 min
 Delta R.T.: -0.002 min
 Response: 17343403
 Conc: 536.16 ug/L

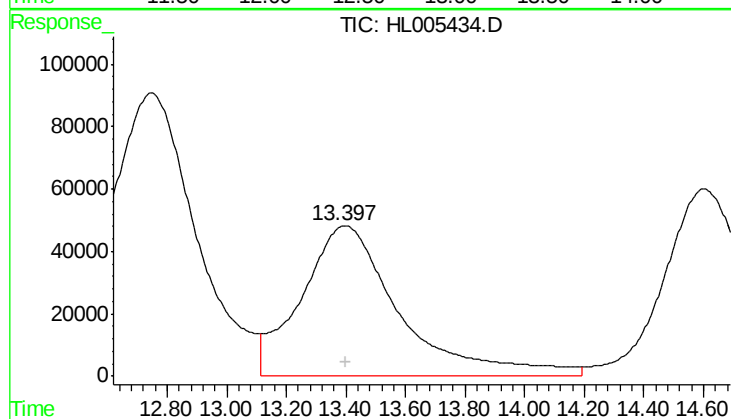


#7 Tetryl

R.T.: 13.398 min
 Delta R.T.: -0.002 min
 Response: 11007324
 Conc: 529.89 ug/L

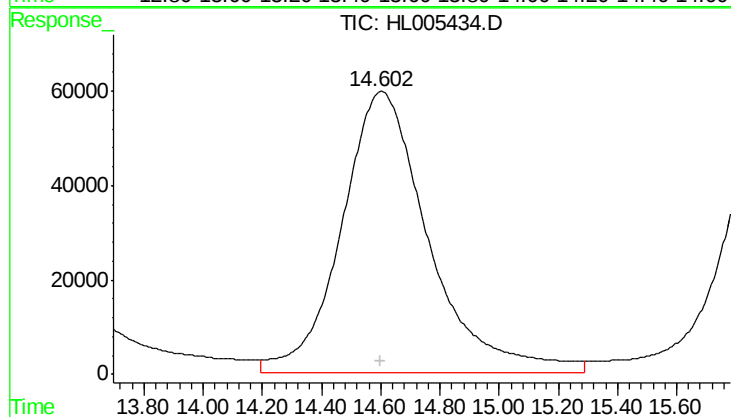

#8 Nitrobenzene


R.T.: 14.604 min
 Delta R.T.: 0.004 min
 Response: 12341922
 Conc: 515.57 ug/L

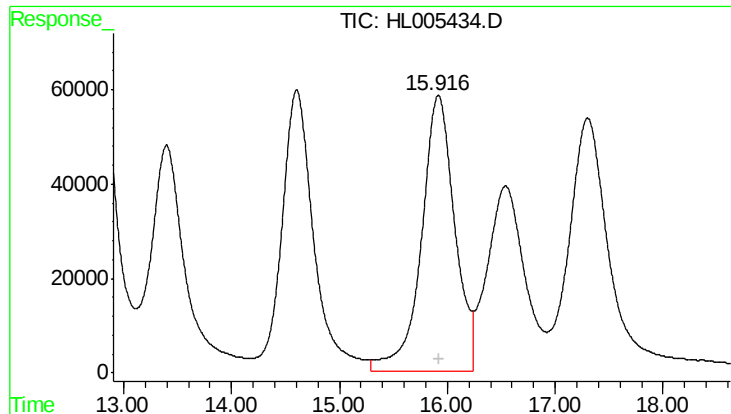

#9 2,4,6-Trinitrotoluene


R.T.: 15.917 min
Delta R.T.: -0.003 min
Response: 12632779
Conc: 496.11 ug/L

Instrument :
HPLC_L
LabSampleId :
HSTDCCC0500

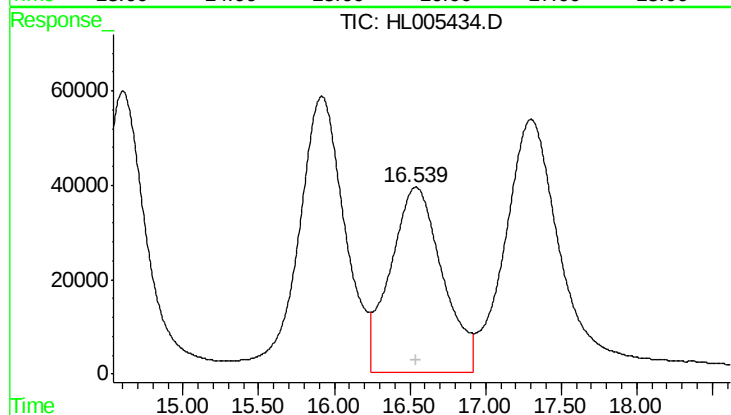


#10 4-Amino-2,6-dinitrotoluene

R.T.: 16.540 min
Delta R.T.: 0.000 min
Response: 9443247
Conc: 528.38 ug/L

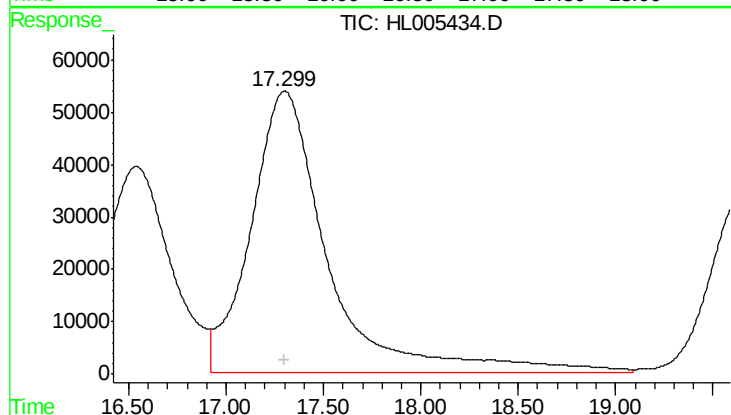


#11 2-Amino-4,6-dinitrotoluene

R.T.: 17.301 min
Delta R.T.: 0.000 min
Response: 14937691
Conc: 513.33 ug/L

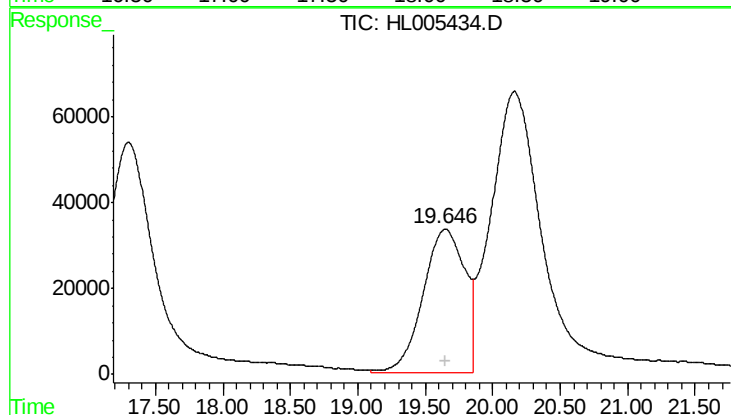

#12 2,6-Dinitrotoluene


R.T.: 19.648 min
Delta R.T.: -0.002 min
Response: 7235428
Conc: 504.16 ug/L

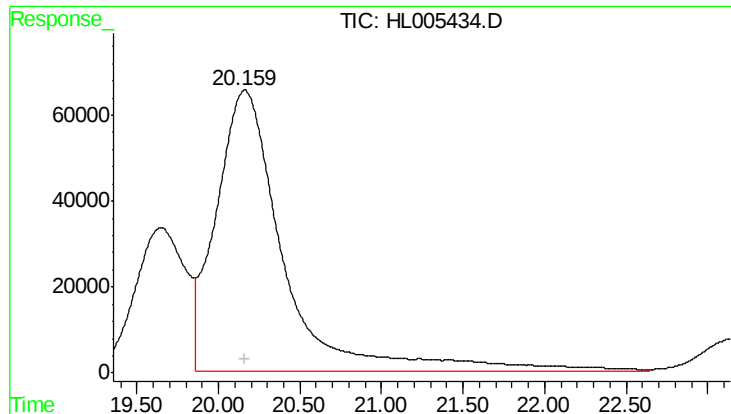

#13 2,4-Dinitrotoluene


R.T.: 20.161 min
Delta R.T.: 0.001 min
Response: 19272967
Conc: 504.34 ug/L

Instrument :
HPLC_L
LabSampleId :
HSTDCCC0500

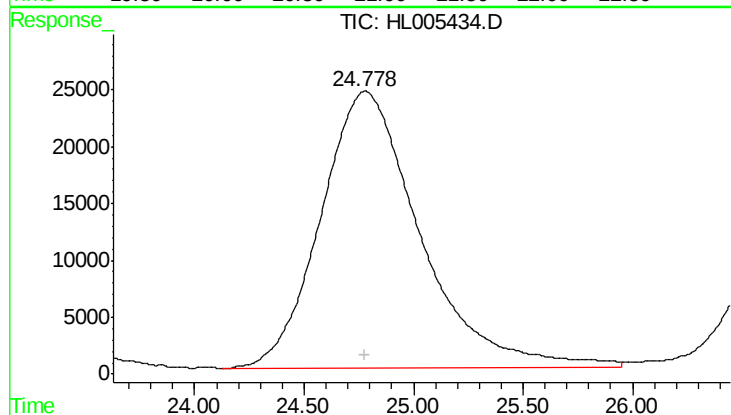


#14 2-Nitrotoluene

R.T.: 24.779 min
Delta R.T.: 0.000 min
Response: 7725263
Conc: 505.86 ug/L

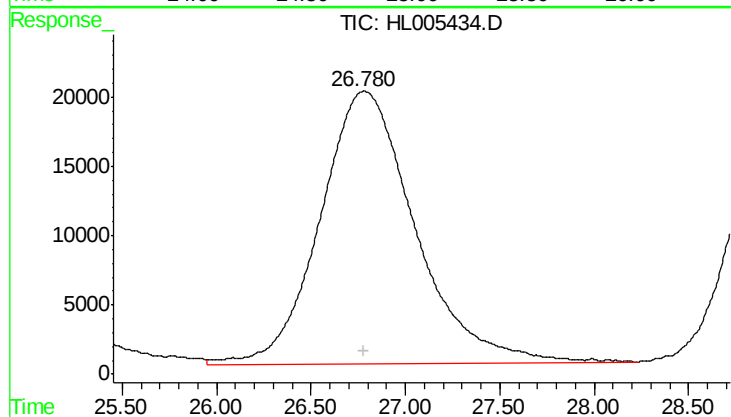

#15 4-Nitrotoluene

R.T.: 26.782 min
Delta R.T.: 0.002 min
Response: 6956656
Conc: 520.52 ug/L

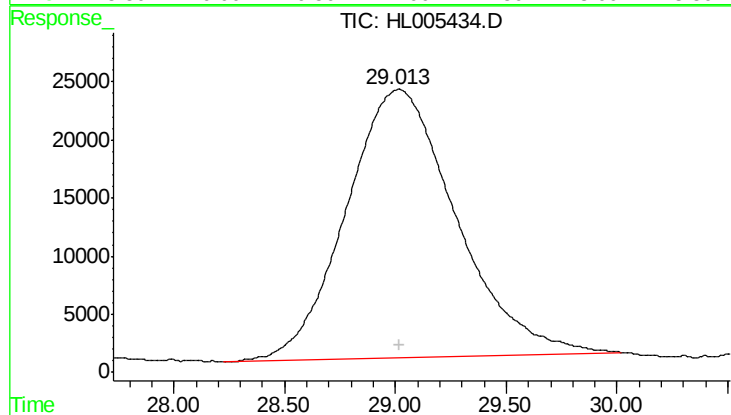

#16 3-Nitrotoluene

R.T.: 29.015 min
Delta R.T.: -0.005 min
Response: 8004368
Conc: 498.24 ug/L