

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
 Data File : HL006240.D
 Signal(s) : vwd1A.ch
 Acq On : 24-Jun-2015, 17:04
 Operator : TP/IZ
 Sample : SSTDICC0200
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :

Integration File: AUTOINT1.E
 Quant Time: Jul 10 07:51:06 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
 Quant Title :
 QLast Update : Fri Jul 10 07:50:12 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	1.408	1345669	212.022 ug/L
3) T RDX	2.460	2960569	225.284 ug/L
4) T 1,3,5-Trinitrobenzene	3.948	3438173	212.321 ug/L
5) T 1,3-Dinitrobenzene	5.214	5130188	212.175 ng/ml
6) T 3,5-Dinitroaniline	5.997	3940288	211.234 ug/L
7) T Nitrobenzene	6.732	2870040	207.714 ug/L
8) T Tetryl	8.919	2404678	219.422 ug/L
9) T 2,4,6-Trinitrotoluene	9.449	3881179	230.072 ug/L
10) T 2-Amino-4,6-dinitroto...	10.725	3765103	216.078 ug/L
11) T 4-Amino-2,6-dinitroto...	11.239	2437593	223.249 ug/L
12) T 2,4-Dinitrotoluene	12.087	4735359	210.000 ug/L
13) T 2,6-Dinitrotoluene	12.472	2367462	213.915 ug/L
14) T 2-Nitrotoluene	16.865	5240758	203.363 ug/L
15) T 4-Nitrotoluene	18.343	4516422	208.882 ug/L
16) T 3-Nitrotoluene	19.856	6188660	212.974 ug/L
17) T PETN	21.061	2747915	212.949 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
Data File : HL006240.D
Signal(s) : vwd1A.ch
Acq On : 24-Jun-2015, 17:04
Operator : TP/IZ
Sample : SSTDICC0200
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: AUTOINT1.E
Quant Time: Jul 10 07:51:06 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
Quant Title :
QLast Update : Fri Jul 10 07:50:12 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

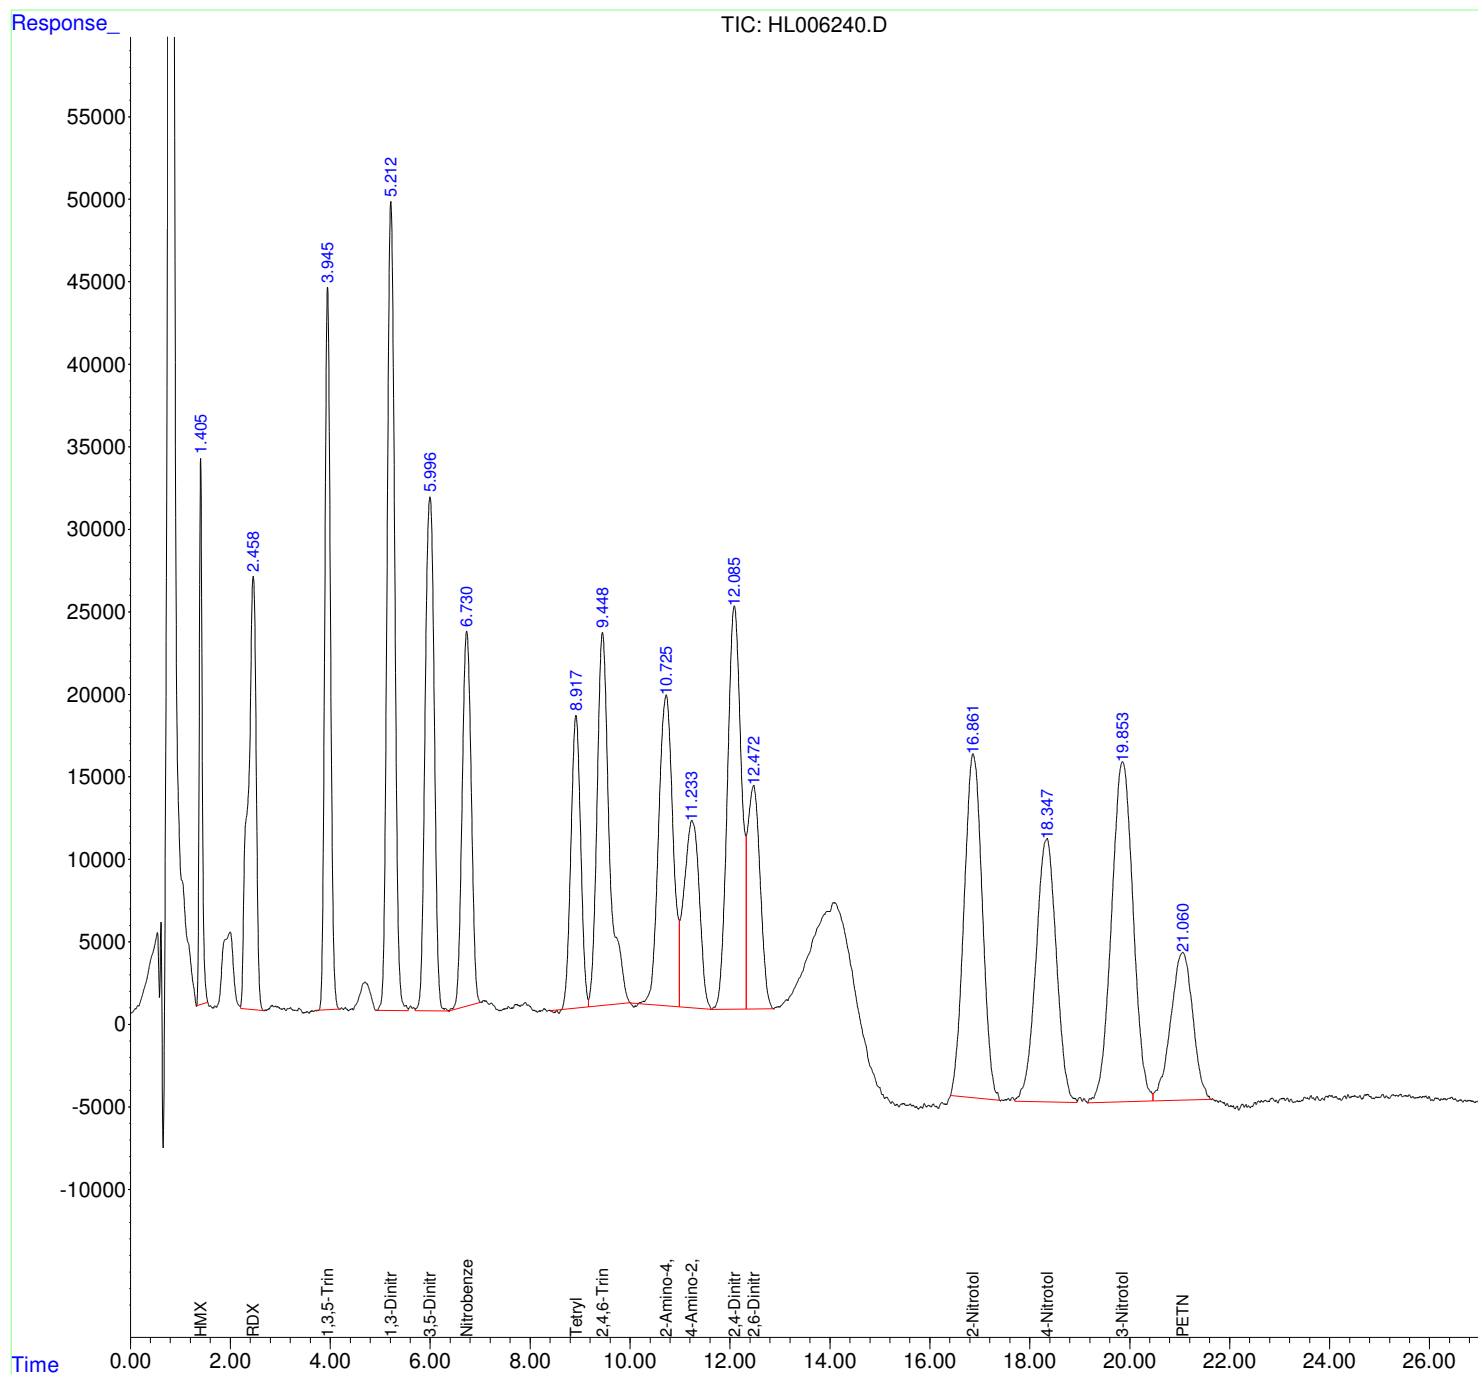


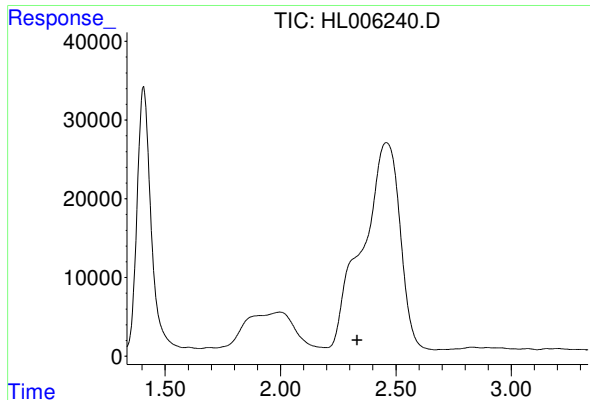

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.333 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :

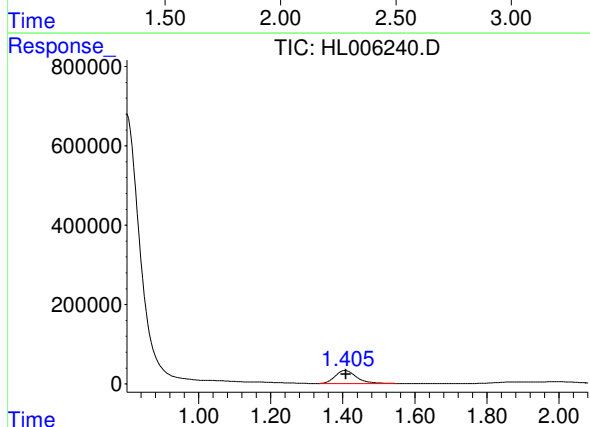


#2 HMX

R.T.: 1.408 min
Delta R.T.: 0.000 min
Response: 1345669
Conc: 212.02 ug/L

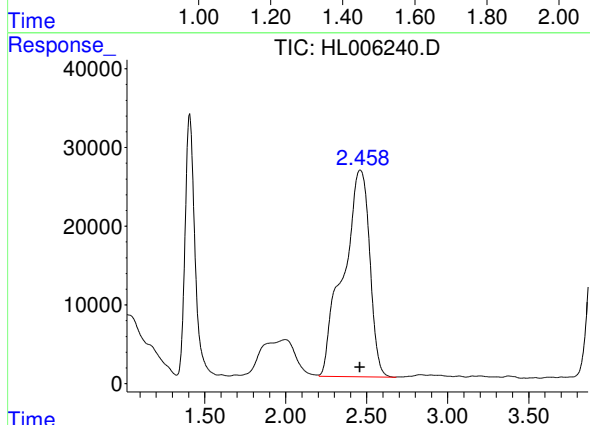


#3 RDX

R.T.: 2.460 min
Delta R.T.: 0.002 min
Response: 2960569
Conc: 225.28 ug/L

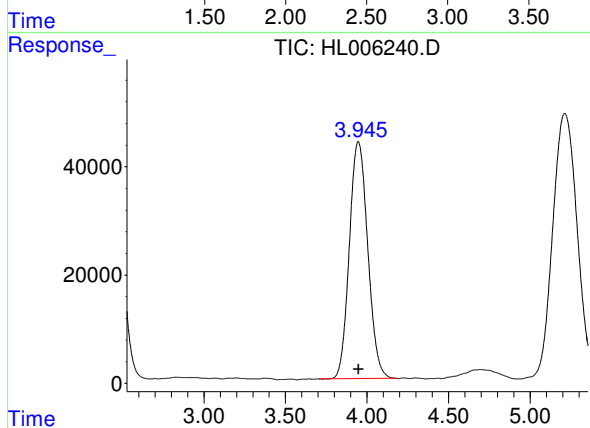

#4 1,3,5-Trinitrobenzene


R.T.: 3.948 min
Delta R.T.: 0.000 min
Response: 3438173
Conc: 212.32 ug/L

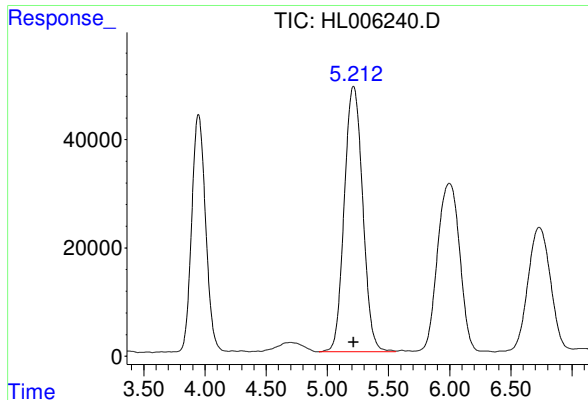

#5 1,3-Dinitrobenzene


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 5130188
Conc: 212.17 ng/ml

Instrument :
HPLC_L
ClientSampleId :

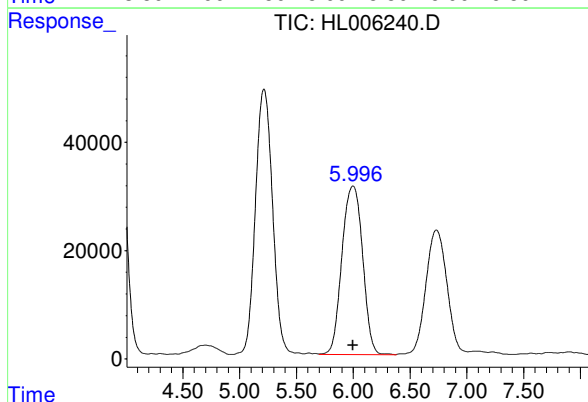


#6 3,5-Dinitroaniline

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 3940288
Conc: 211.23 ug/L

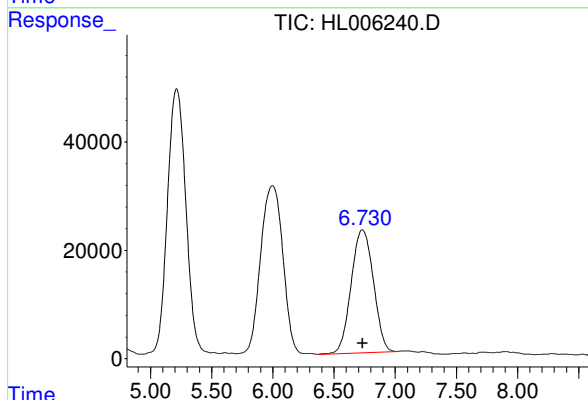


#7 Nitrobenzene

R.T.: 6.732 min
Delta R.T.: 0.000 min
Response: 2870040
Conc: 207.71 ug/L

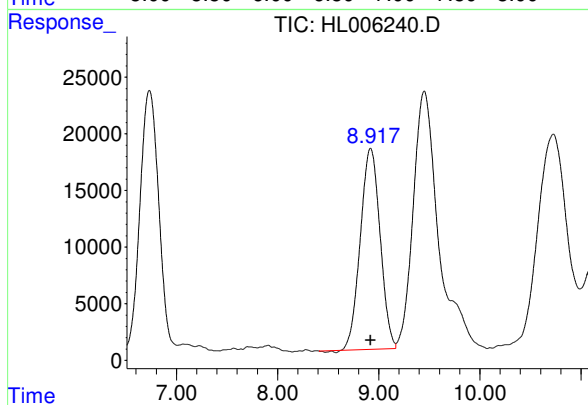

#8 Tetryl


R.T.: 8.919 min
Delta R.T.: 0.000 min
Response: 2404678
Conc: 219.42 ug/L

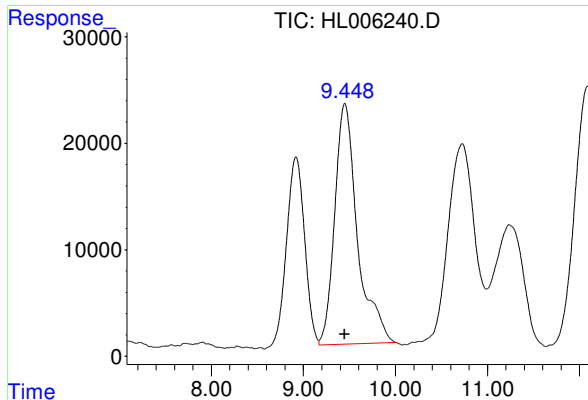

#9 2,4,6-Trinitrotoluene


R.T.: 9.449 min
Delta R.T.: 0.001 min
Response: 3881179
Conc: 230.07 ug/L

Instrument :
HPLC_L
ClientSampleId :

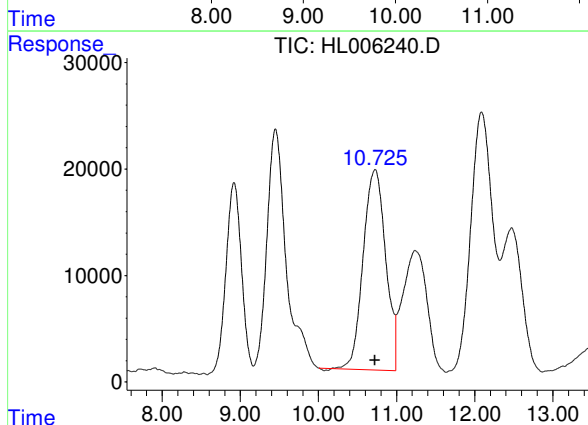


#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.725 min
Delta R.T.: 0.000 min
Response: 3765103
Conc: 216.08 ug/L

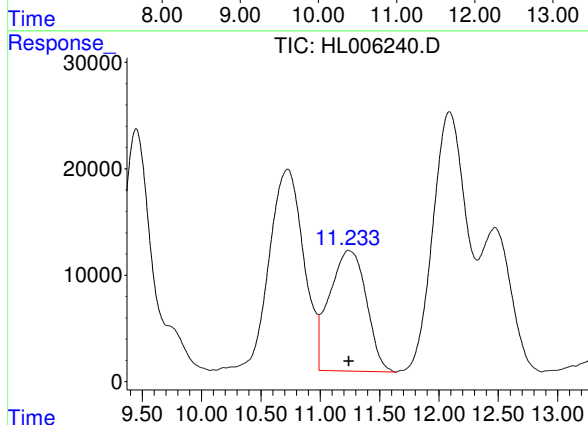


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.239 min
Delta R.T.: 0.000 min
Response: 2437593
Conc: 223.25 ug/L



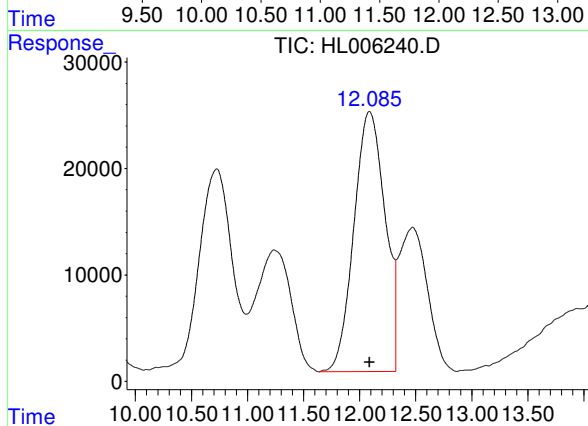



#12 2,4-Dinitrotoluene

R.T.: 12.087 min
Delta R.T.: 0.000 min
Response: 4735359
Conc: 210.00 ug/L

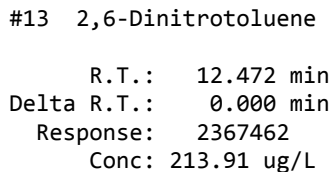

Instrument :
HPLC_L
ClientSampleId :

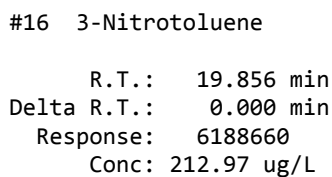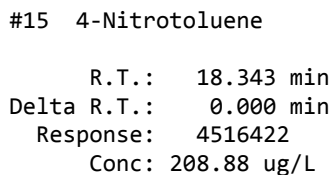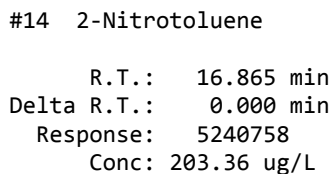

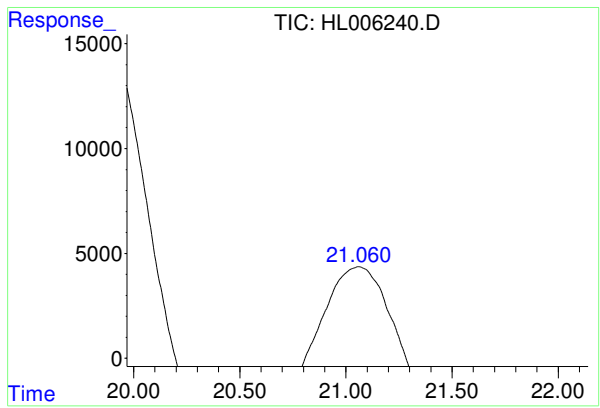

#17 PETN

R.T.: 21.061 min
Delta R.T.: 0.000 min
Response: 2747915
Conc: 212.95 ug/L

Instrument :
HPLC_L
ClientSampleId :