

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
 Data File : HL006245.D
 Signal(s) : vwd1A.ch
 Acq On : 24-Jun-2015, 19:26
 Operator : TP/IZ
 Sample : SSTDICV0500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :

Integration File: AUTOINT1.E
 Quant Time: Jun 25 05:04:49 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
 Quant Title :
 QLast Update : Thu Jun 25 05:04:10 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.440	6691642	478.899 ug/L
Target Compounds			
2) T HMX	1.398	3109728	483.632 ug/L
3) T RDX	2.440	6691642	478.899 ug/L
4) T 1,3,5-Trinitrobenzene	3.920	7807501	482.496 ug/L
5) T 1,3-Dinitrobenzene	5.178	11702020	484.448 ng/ml
6) T 3,5-Dinitroaniline	5.956	9015875	482.820 ug/L
7) T Nitrobenzene	6.685	6685280	484.331 ug/L
8) T Tetryl	8.859	5173617	475.128 ug/L
9) T 2,4,6-Trinitrotoluene	9.386	8394764	498.579 ug/L
10) T 2-Amino-4,6-dinitroto...	10.639	8248644	470.873 ug/L
11) T 4-Amino-2,6-dinitroto...	11.177	5177056	474.839 ug/L
12) T 2,4-Dinitrotoluene	12.006	10737288	477.173 ug/L
13) T 2,6-Dinitrotoluene	12.387	5271321	477.886 ug/L
14) T 2-Nitrotoluene	16.759	12402901	476.304 ug/L
15) T 4-Nitrotoluene	18.216	10474911	472.931 ug/L
16) T 3-Nitrotoluene	19.727	14166600	477.161 ug/L
17) T PETN	20.923	6435595	490.007 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
Data File : HL006245.D
Signal(s) : vwd1A.ch
Acq On : 24-Jun-2015, 19:26
Operator : TP/IZ
Sample : SSTDICV0500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: AUTOINT1.E
Quant Time: Jun 25 05:04:49 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
Quant Title :
QLast Update : Thu Jun 25 05:04:10 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

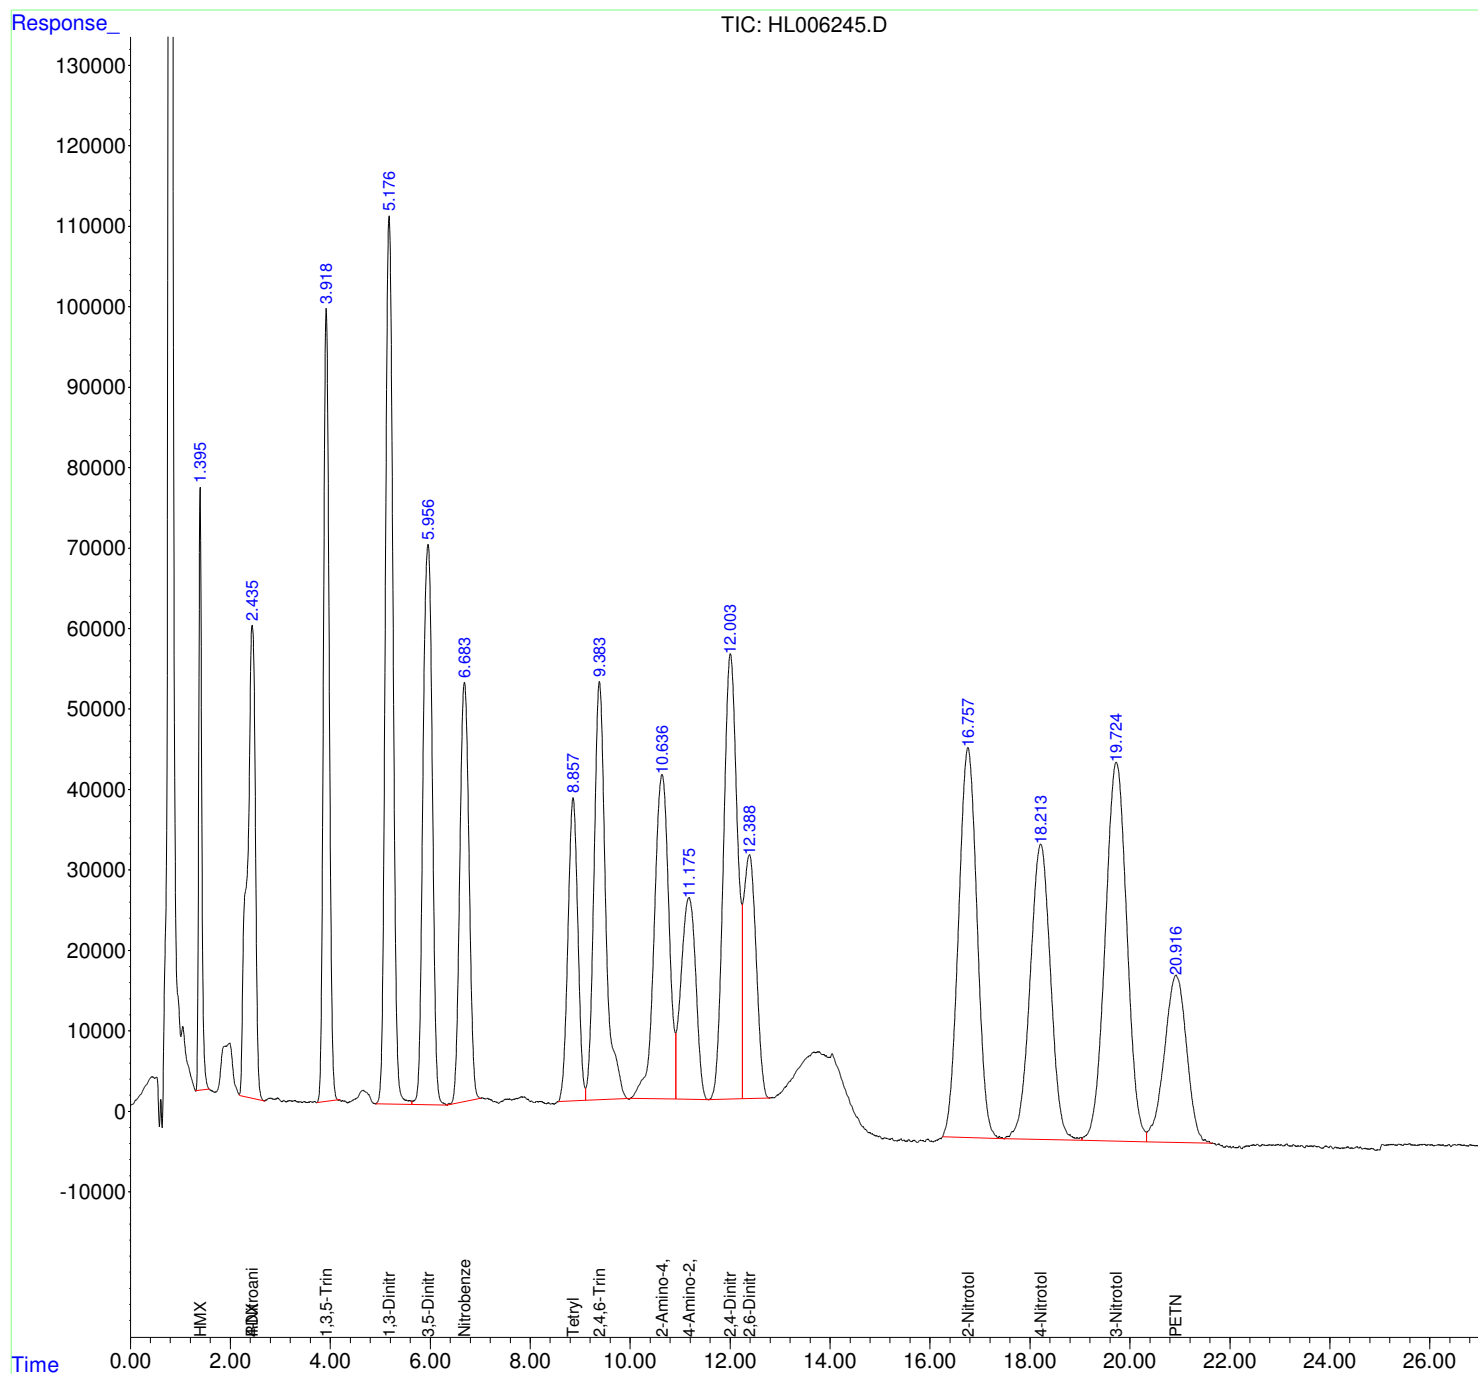


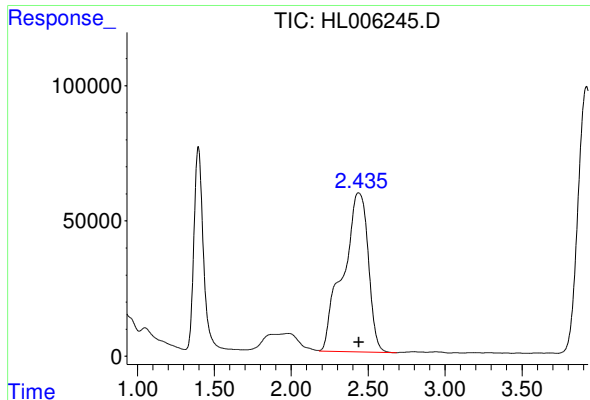

#1 4-Nitroaniline


R.T.: 2.440 min
Delta R.T.: 0.000 min
Response: 6691642
Conc: 478.90 ug/L

Instrument :
HPLC_L
ClientSampleId :

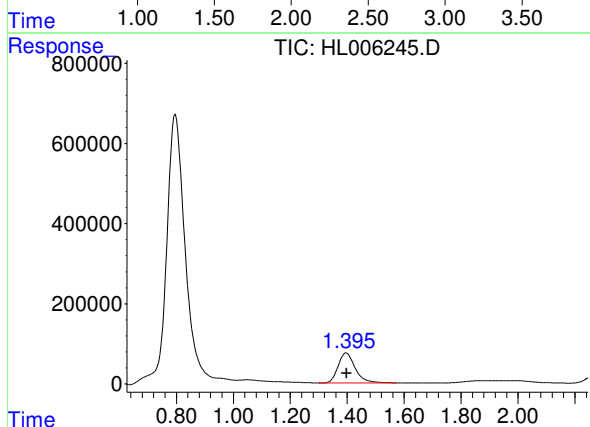


#2 HMX

R.T.: 1.398 min
Delta R.T.: 0.000 min
Response: 3109728
Conc: 483.63 ug/L

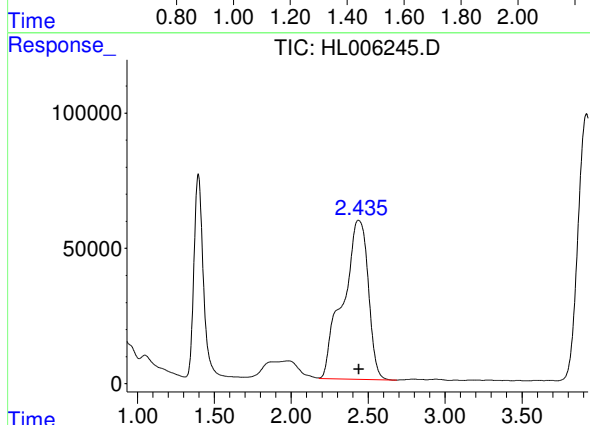


#3 RDX

R.T.: 2.440 min
Delta R.T.: 0.000 min
Response: 6691642
Conc: 478.90 ug/L

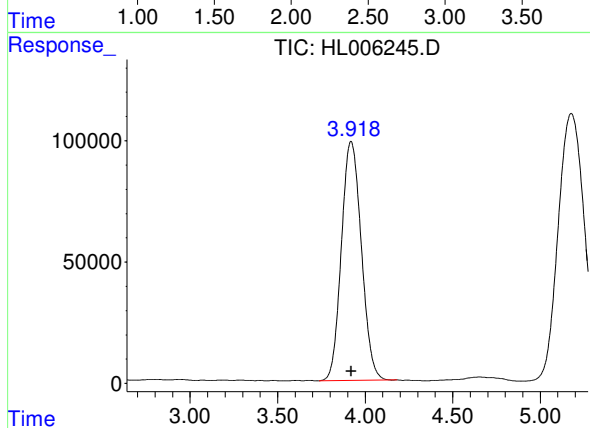

#4 1,3,5-Trinitrobenzene


R.T.: 3.920 min
Delta R.T.: 0.000 min
Response: 7807501
Conc: 482.50 ug/L

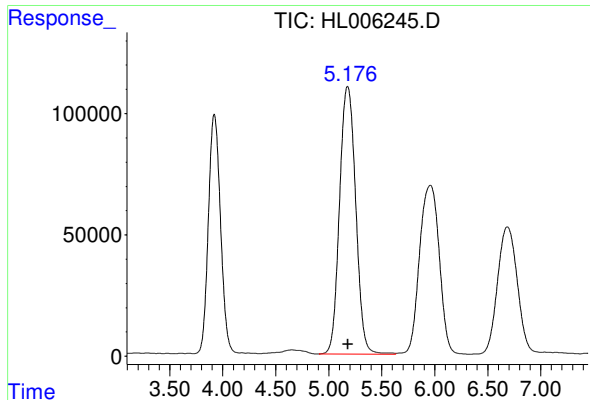

#5 1,3-Dinitrobenzene


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 11702020
Conc: 484.45 ng/ml

Instrument :
HPLC_L
ClientSampleId :

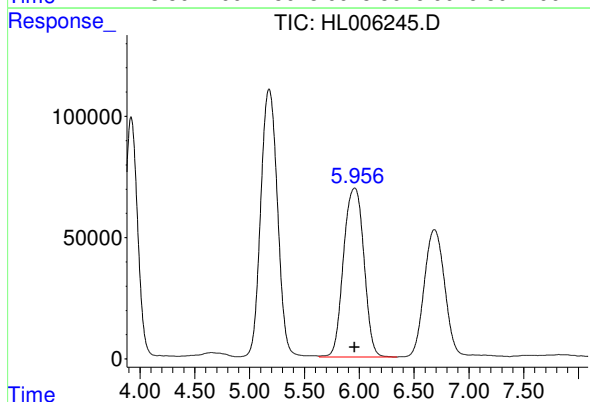


#6 3,5-Dinitroaniline

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 9015875
Conc: 482.82 ug/L

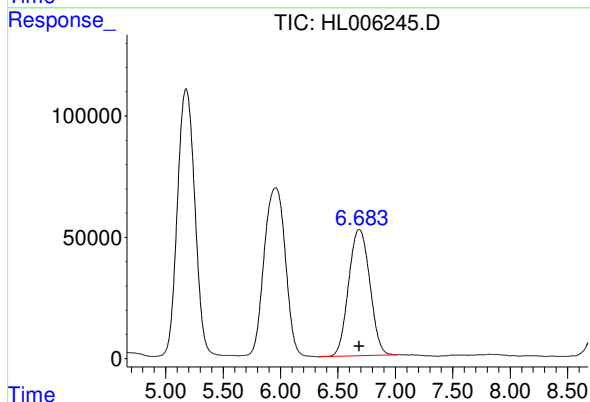


#7 Nitrobenzene

R.T.: 6.685 min
Delta R.T.: 0.000 min
Response: 6685280
Conc: 484.33 ug/L

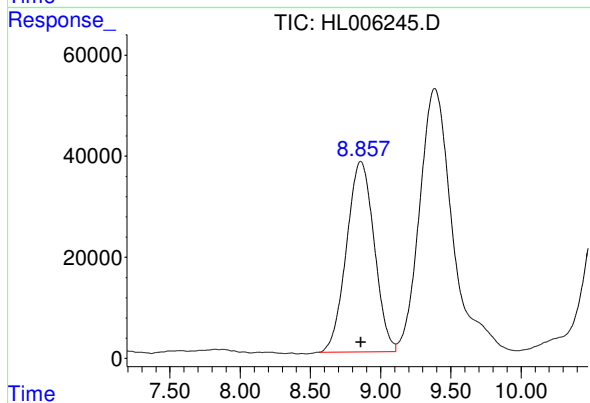

#8 Tetryl


R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 5173617
Conc: 475.13 ug/L

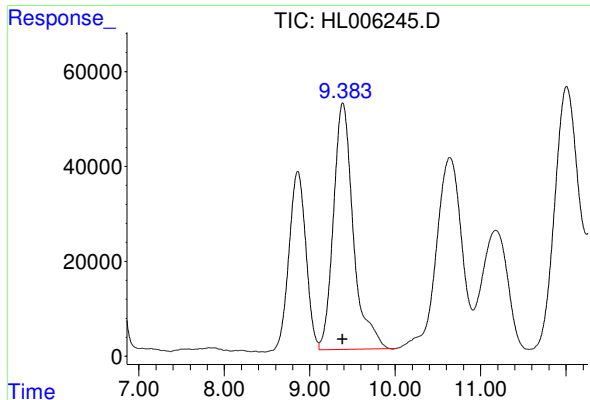

#9 2,4,6-Trinitrotoluene


R.T.: 9.386 min
Delta R.T.: 0.000 min
Response: 8394764
Conc: 498.58 ug/L

Instrument :
HPLC_L
ClientSampleId :

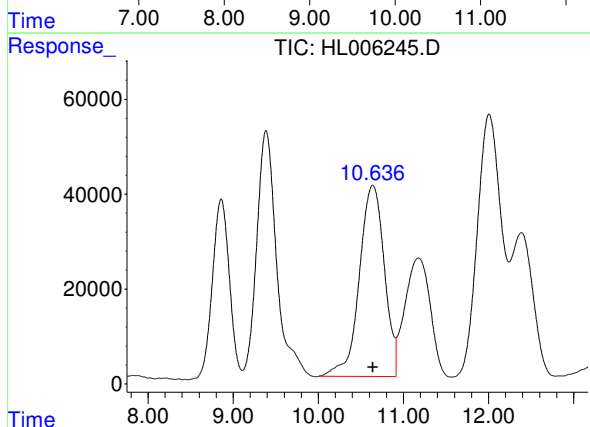


#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.639 min
Delta R.T.: 0.000 min
Response: 8248644
Conc: 470.87 ug/L

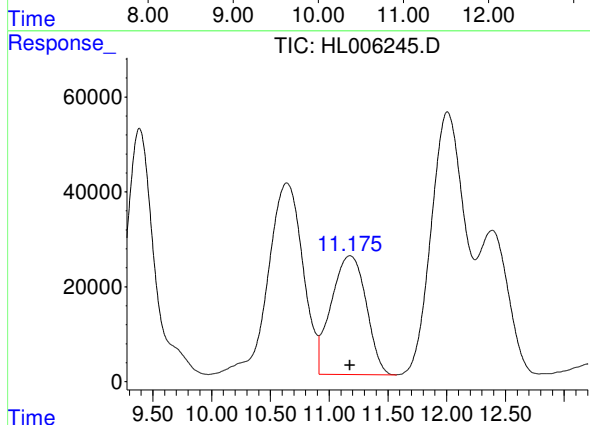


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.177 min
Delta R.T.: 0.000 min
Response: 5177056
Conc: 474.84 ug/L

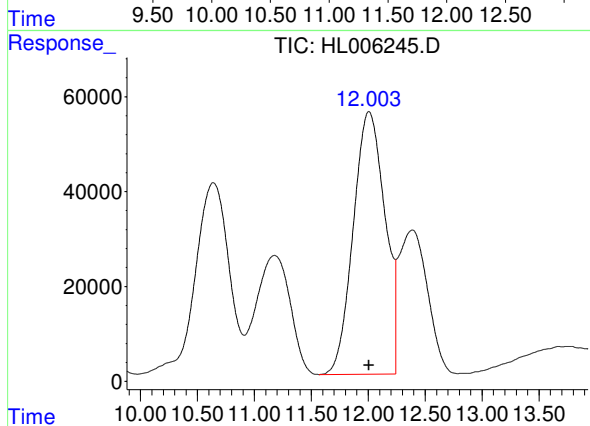

#12 2,4-Dinitrotoluene


R.T.: 12.006 min
Delta R.T.: 0.000 min
Response: 10737288
Conc: 477.17 ug/L

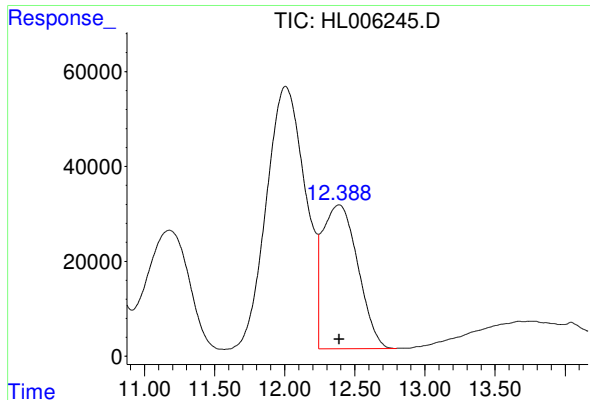

#13 2,6-Dinitrotoluene


R.T.: 12.387 min
Delta R.T.: 0.000 min
Response: 5271321
Conc: 477.89 ug/L

Instrument :
HPLC_L
ClientSampleId :

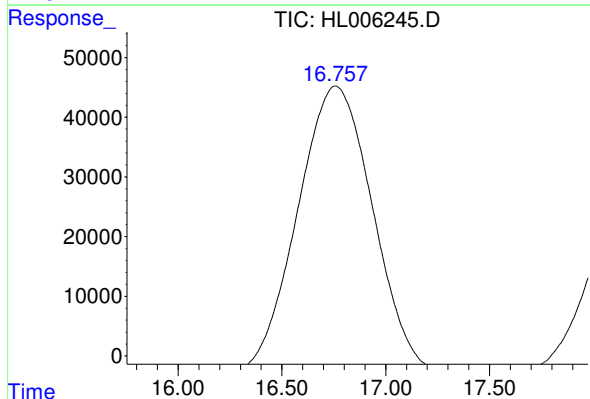


#14 2-Nitrotoluene

R.T.: 16.759 min
Delta R.T.: 0.002 min
Response: 12402901
Conc: 476.30 ug/L

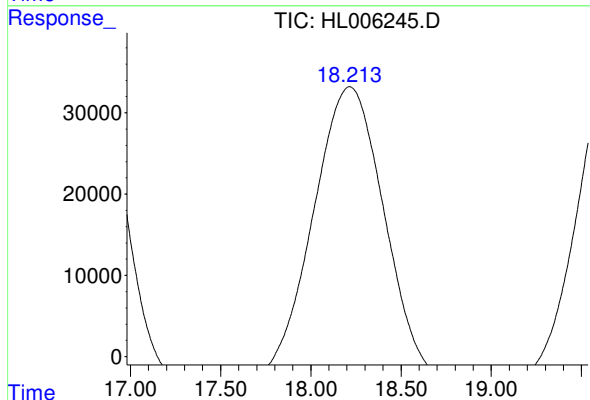


#15 4-Nitrotoluene

R.T.: 18.216 min
Delta R.T.: 0.003 min
Response: 10474911
Conc: 472.93 ug/L

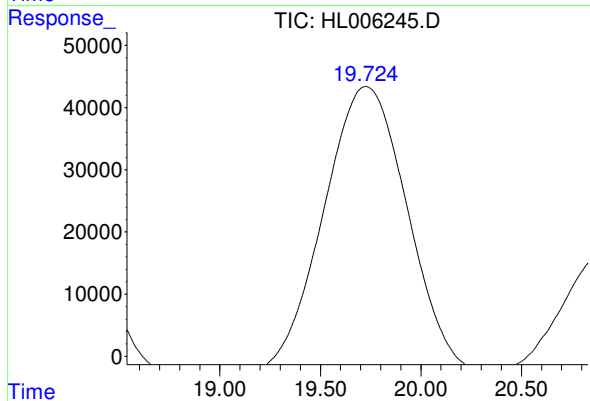

#16 3-Nitrotoluene

R.T.: 19.727 min
Delta R.T.: 0.002 min
Response: 14166600
Conc: 477.16 ug/L

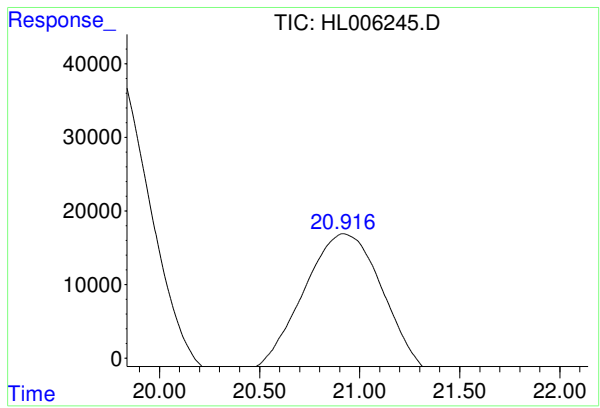

#17 PETN

R.T.: 20.923 min
Delta R.T.: 0.007 min
Response: 6435595
Conc: 490.01 ug/L

Instrument :
HPLC_L
ClientSampleId :