

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
 Data File : HL006250.D
 Signal(s) : vwd1A.ch
 Acq On : 24-Jun-2015, 21:47
 Operator : TP/IZ
 Sample : G2653-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :

Integration File: AUTOINT1.E
 Quant Time: Jun 25 08:03:37 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
 Quant Title :
 QLast Update : Thu Jun 25 08:03:31 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	2.354	3583280	256.443 ug/L
Target Compounds				
2) T	HMX	1.403	352072	54.755 ug/L
3) T	RDX	2.354	3583280	256.443 ug/L
4) T	1,3,5-Trinitrobenzene	3.915	890281	55.019 ug/L
5) T	1,3-Dinitrobenzene	5.167	1298721	53.765 ng/ml
6) T	3,5-Dinitroaniline	5.939	1028571	55.082 ug/L
7) T	Nitrobenzene	6.667	708500	51.329 ug/L
8) T	Tetryl	8.819	622395	57.159 ug/L
9) T	2,4,6-Trinitrotoluene	9.335	839548	49.862 ug/L
10) T	2-Amino-4,6-dinitroto...	10.578	834335	4.633 ug/L
11) T	4-Amino-2,6-dinitroto...	11.130	532533	48.844 ug/L
12) T	2,4-Dinitrotoluene	11.936	1051166	46.715 ug/L
13) T	2,6-Dinitrotoluene	12.329	465067	42.162 ug/L
14) T	2-Nitrotoluene	16.639	1368952	52.571 ug/L
15) T	4-Nitrotoluene	18.063	1174283	53.018 ug/L
16) T	3-Nitrotoluene	19.603	1612202	54.302 ug/L
17) T	PETN	20.751	1301755	99.116 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
Data File : HL006250.D
Signal(s) : vwd1A.ch
Acq On : 24-Jun-2015, 21:47
Operator : TP/IZ
Sample : G2653-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: AUTOINT1.E
Quant Time: Jun 25 08:03:37 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
Quant Title :
QLast Update : Thu Jun 25 08:03:31 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

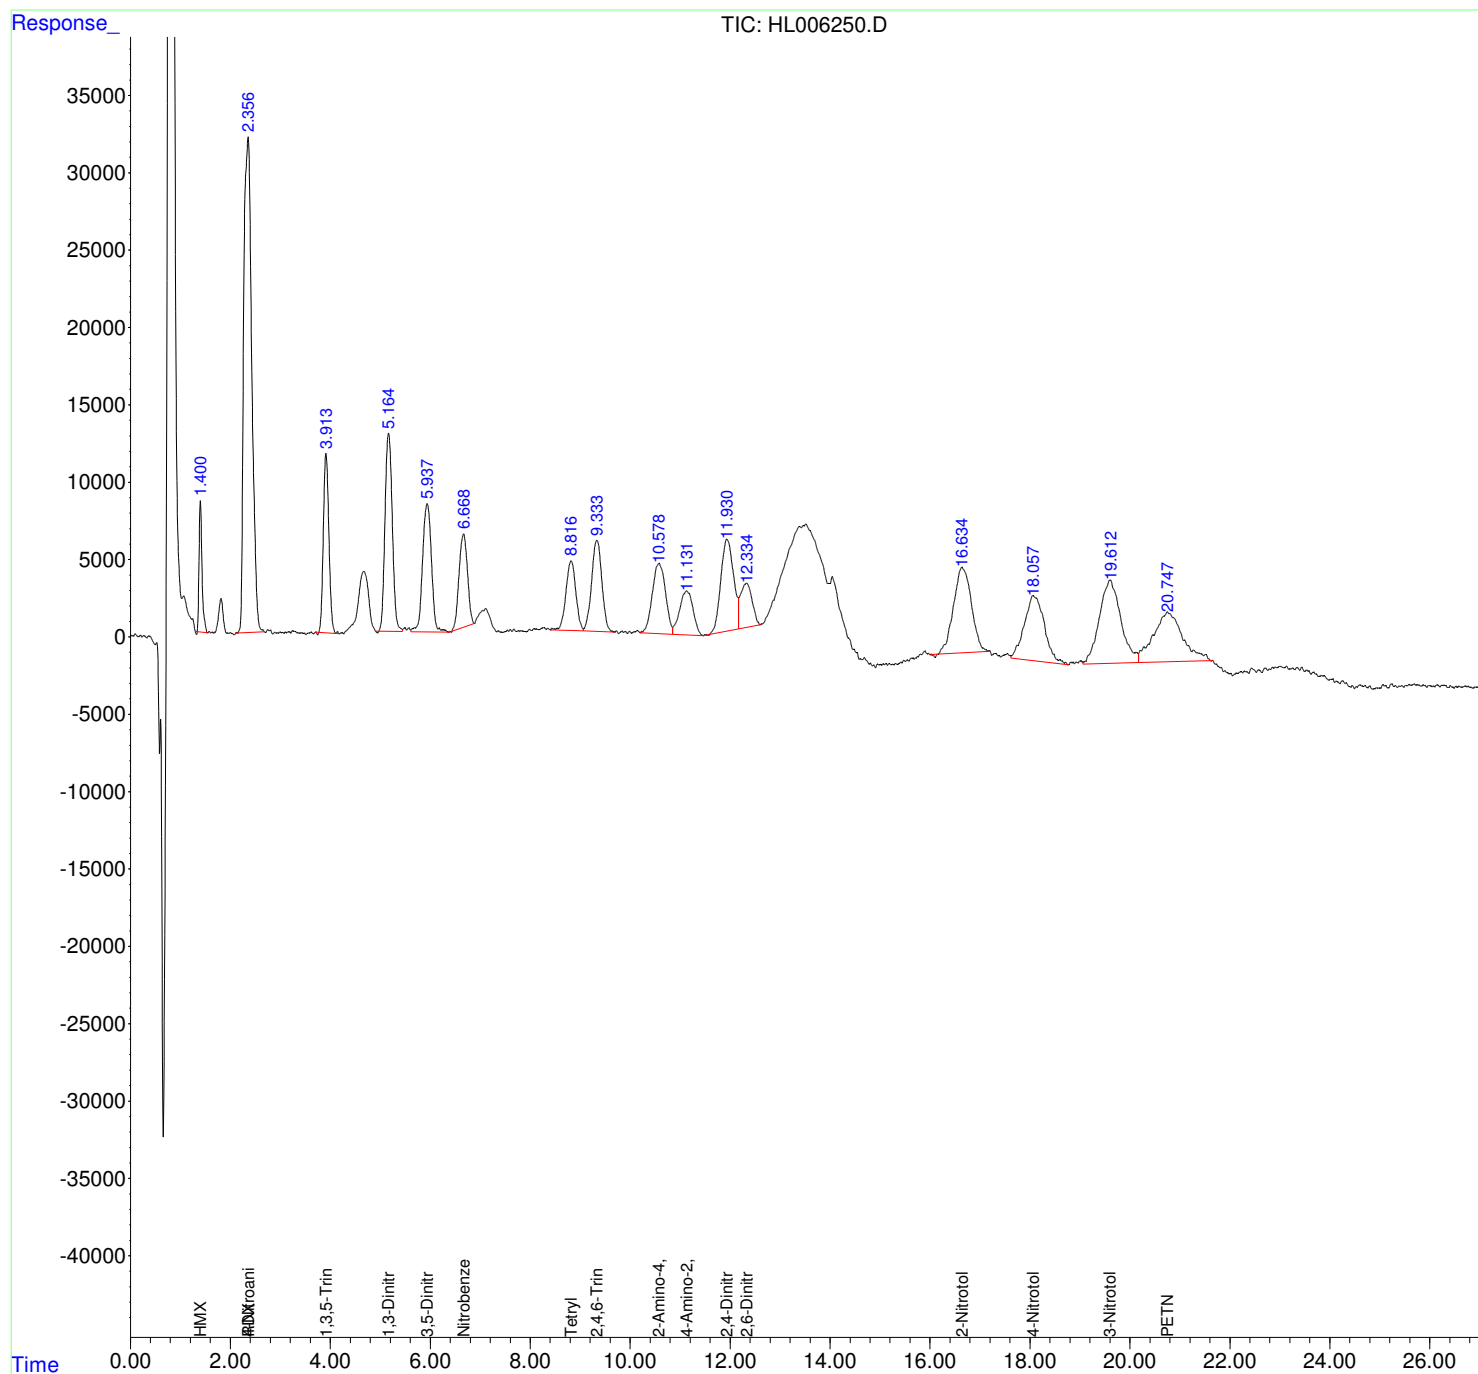


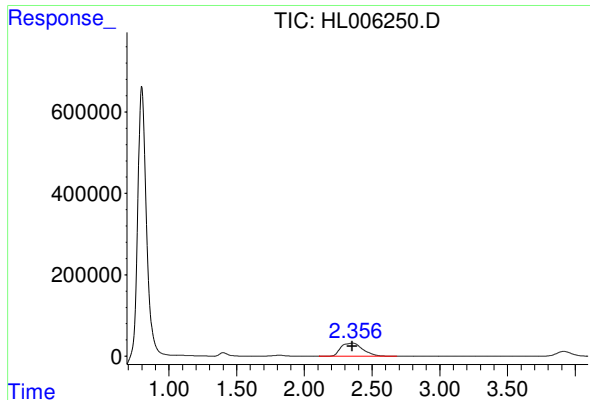

#1 4-Nitroaniline


R.T.: 2.354 min
Delta R.T.: 0.000 min
Response: 3583280
Conc: 256.44 ug/L

Instrument :
HPLC_L
ClientSampleId :

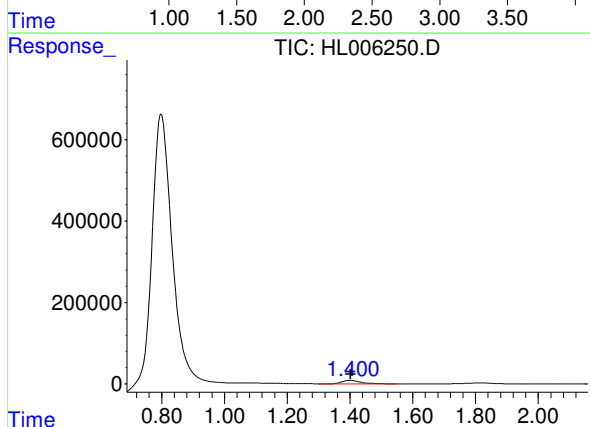


#2 HMX

R.T.: 1.403 min
Delta R.T.: 0.000 min
Response: 352072
Conc: 54.76 ug/L

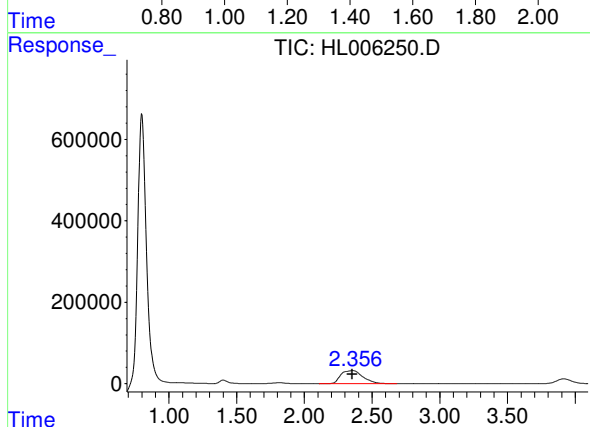


#3 RDX

R.T.: 2.354 min
Delta R.T.: 0.000 min
Response: 3583280
Conc: 256.44 ug/L

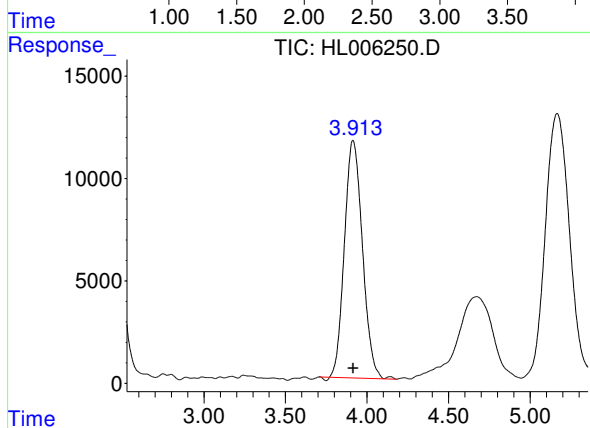

#4 1,3,5-Trinitrobenzene


R.T.: 3.915 min
Delta R.T.: 0.000 min
Response: 890281
Conc: 55.02 ug/L

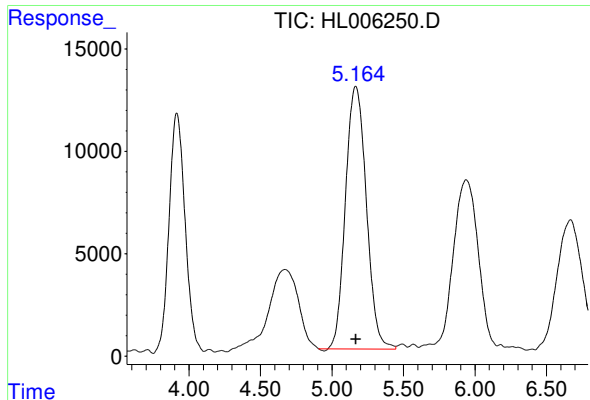

#5 1,3-Dinitrobenzene


R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 1298721
Conc: 53.77 ng/ml

Instrument :
HPLC_L
ClientSampleId :

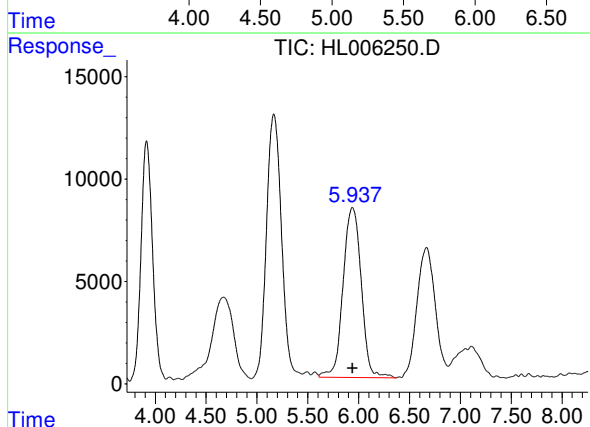


#6 3,5-Dinitroaniline

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 1028571
Conc: 55.08 ug/L

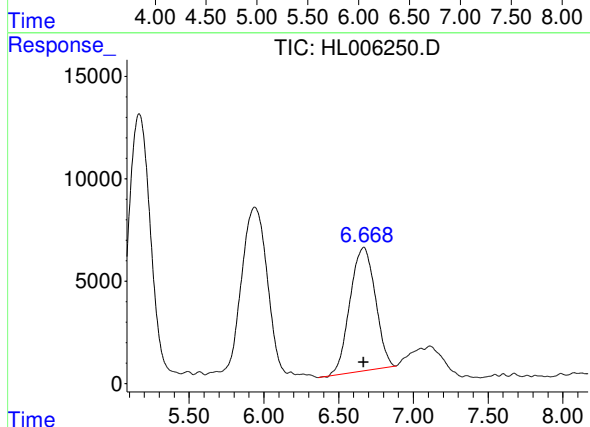


#7 Nitrobenzene

R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 708500
Conc: 51.33 ug/L

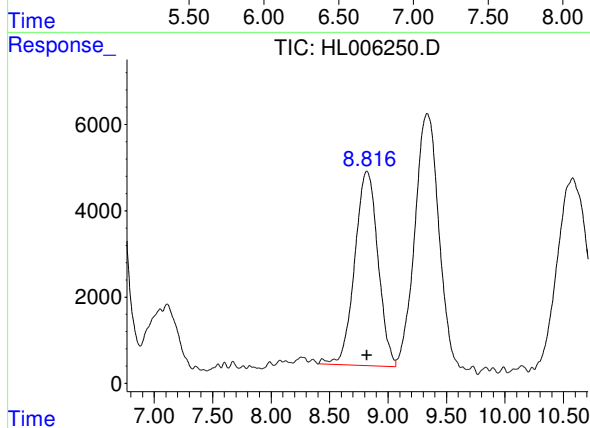

#8 Tetryl


R.T.: 8.819 min
Delta R.T.: 0.000 min
Response: 622395
Conc: 57.16 ug/L

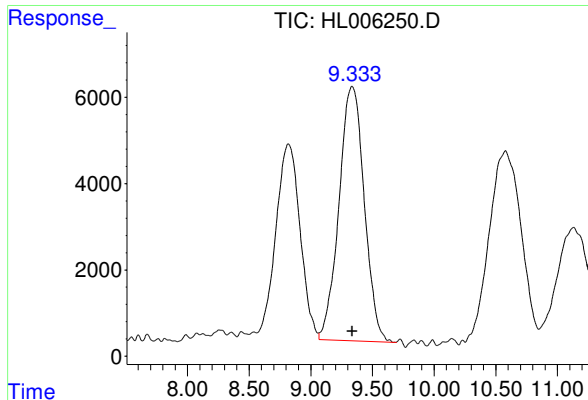

#9 2,4,6-Trinitrotoluene


R.T.: 9.335 min
Delta R.T.: 0.000 min
Response: 839548
Conc: 49.86 ug/L

Instrument :
HPLC_L
ClientSampleId :

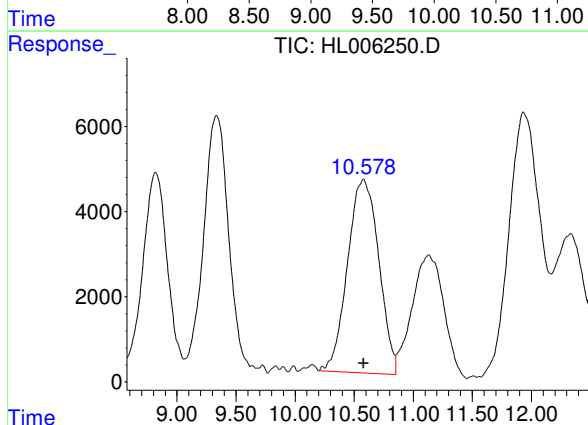


#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.578 min
Delta R.T.: 0.000 min
Response: 834335
Conc: 4.63 ug/L

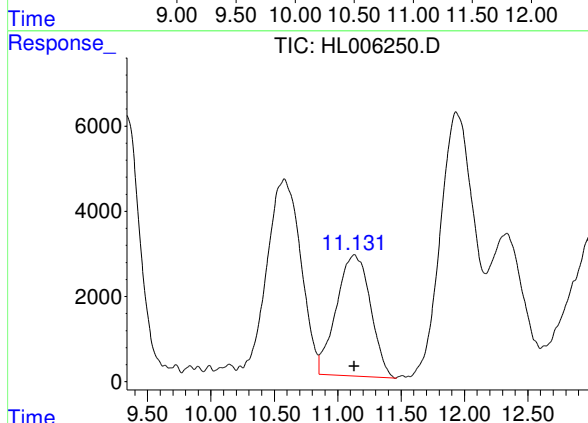


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.130 min
Delta R.T.: 0.000 min
Response: 532533
Conc: 48.84 ug/L

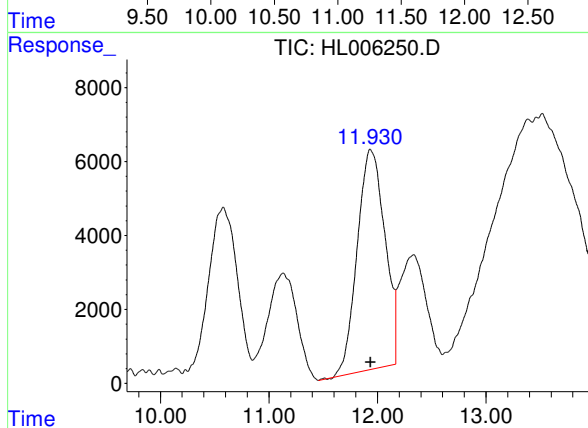

#12 2,4-Dinitrotoluene


R.T.: 11.936 min
Delta R.T.: 0.000 min
Response: 1051166
Conc: 46.71 ug/L

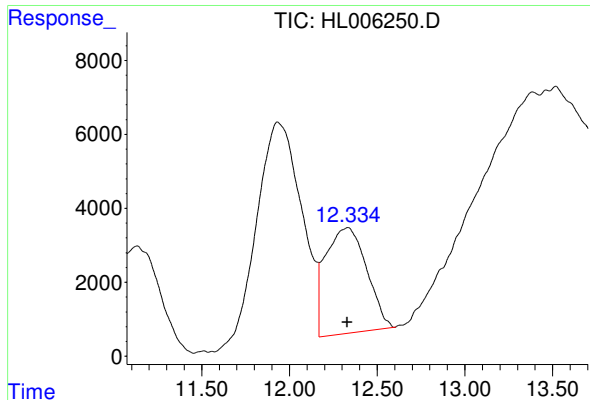

#13 2,6-Dinitrotoluene


R.T.: 12.329 min
Delta R.T.: 0.000 min
Response: 465067
Conc: 42.16 ug/L

Instrument :
HPLC_L
ClientSampleId :

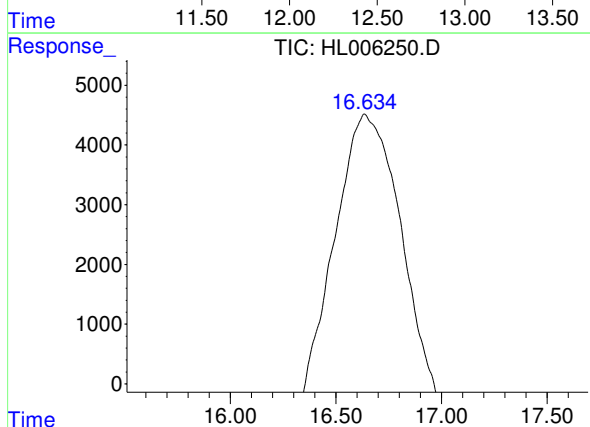


#14 2-Nitrotoluene

R.T.: 16.639 min
Delta R.T.: 0.000 min
Response: 1368952
Conc: 52.57 ug/L

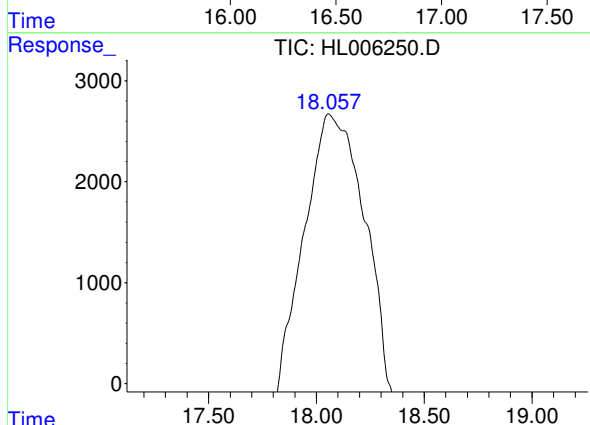


#15 4-Nitrotoluene

R.T.: 18.063 min
Delta R.T.: 0.000 min
Response: 1174283
Conc: 53.02 ug/L

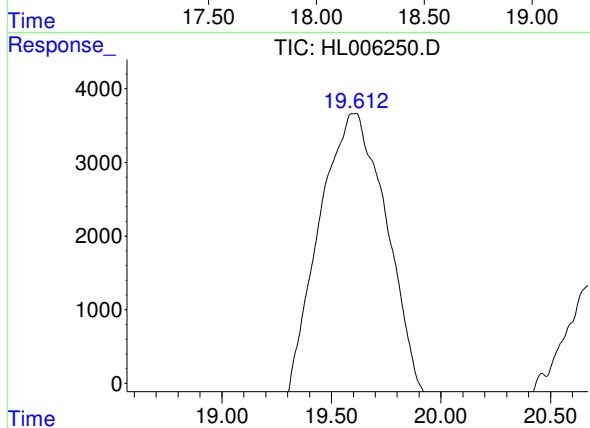

#16 3-Nitrotoluene

R.T.: 19.603 min
Delta R.T.: 0.000 min
Response: 1612202
Conc: 54.30 ug/L

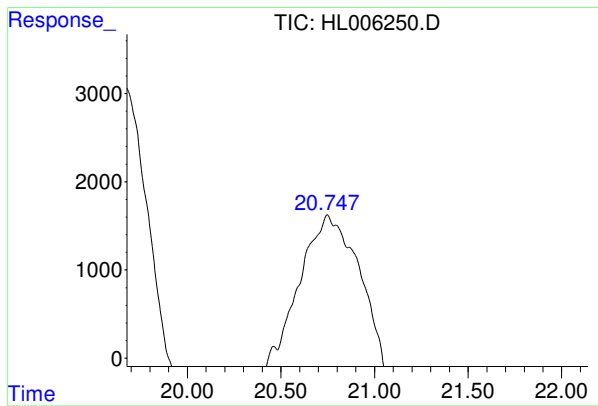

#17 PETN

R.T.: 20.751 min
Delta R.T.: 0.000 min
Response: 1301755
Conc: 99.12 ug/L

Instrument :
HPLC_L
ClientSampleId :