

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
 Data File : HL006251.D
 Signal(s) : vwd1A.ch
 Acq On : 24-Jun-2015, 22:16
 Operator : TP/IZ
 Sample : G2653-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :

Integration File: AUTOINT1.E
 Quant Time: Jun 25 08:06:11 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
 Quant Title :
 QLast Update : Thu Jun 25 08:06:05 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.371	4614991	330.280 ug/L
Target Compounds			
2) T HMX	1.382	1269733	197.472 ug/L
3) T RDX	2.371	4614991	330.280 ug/L
4) T 1,3,5-Trinitrobenzene	3.878	3232288	199.752 ug/L
5) T 1,3-Dinitrobenzene	5.123	4769032	197.432 ng/ml
6) T 3,5-Dinitroaniline	5.895	3603898	192.997 ug/L
7) T Nitrobenzene	6.615	2742356	198.676 ug/L
8) T Tetryl	8.768	2255460	207.134 ug/L
9) T 2,4,6-Trinitrotoluene	9.283	3066893	182.148 ug/L
10) T 2-Amino-4,6-dinitroto...	10.524	2971892	149.120 ug/L
11) T 4-Amino-2,6-dinitroto...	11.075	1930472	177.063 ug/L
12) T 2,4-Dinitrotoluene	11.882	4208412	187.025 ug/L
13) T 2,6-Dinitrotoluene	12.259	1966763	178.302 ug/L
14) T 2-Nitrotoluene	16.589	5233496	200.980 ug/L
15) T 4-Nitrotoluene	18.019	4100518	185.134 ug/L
16) T 3-Nitrotoluene	19.523	5574264	187.753 ug/L
17) T PETN	20.742	2731264	207.959 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
Data File : HL006251.D
Signal(s) : vwd1A.ch
Acq On : 24-Jun-2015, 22:16
Operator : TP/IZ
Sample : G2653-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: AUTOINT1.E
Quant Time: Jun 25 08:06:11 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
Quant Title :
QLast Update : Thu Jun 25 08:06:05 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

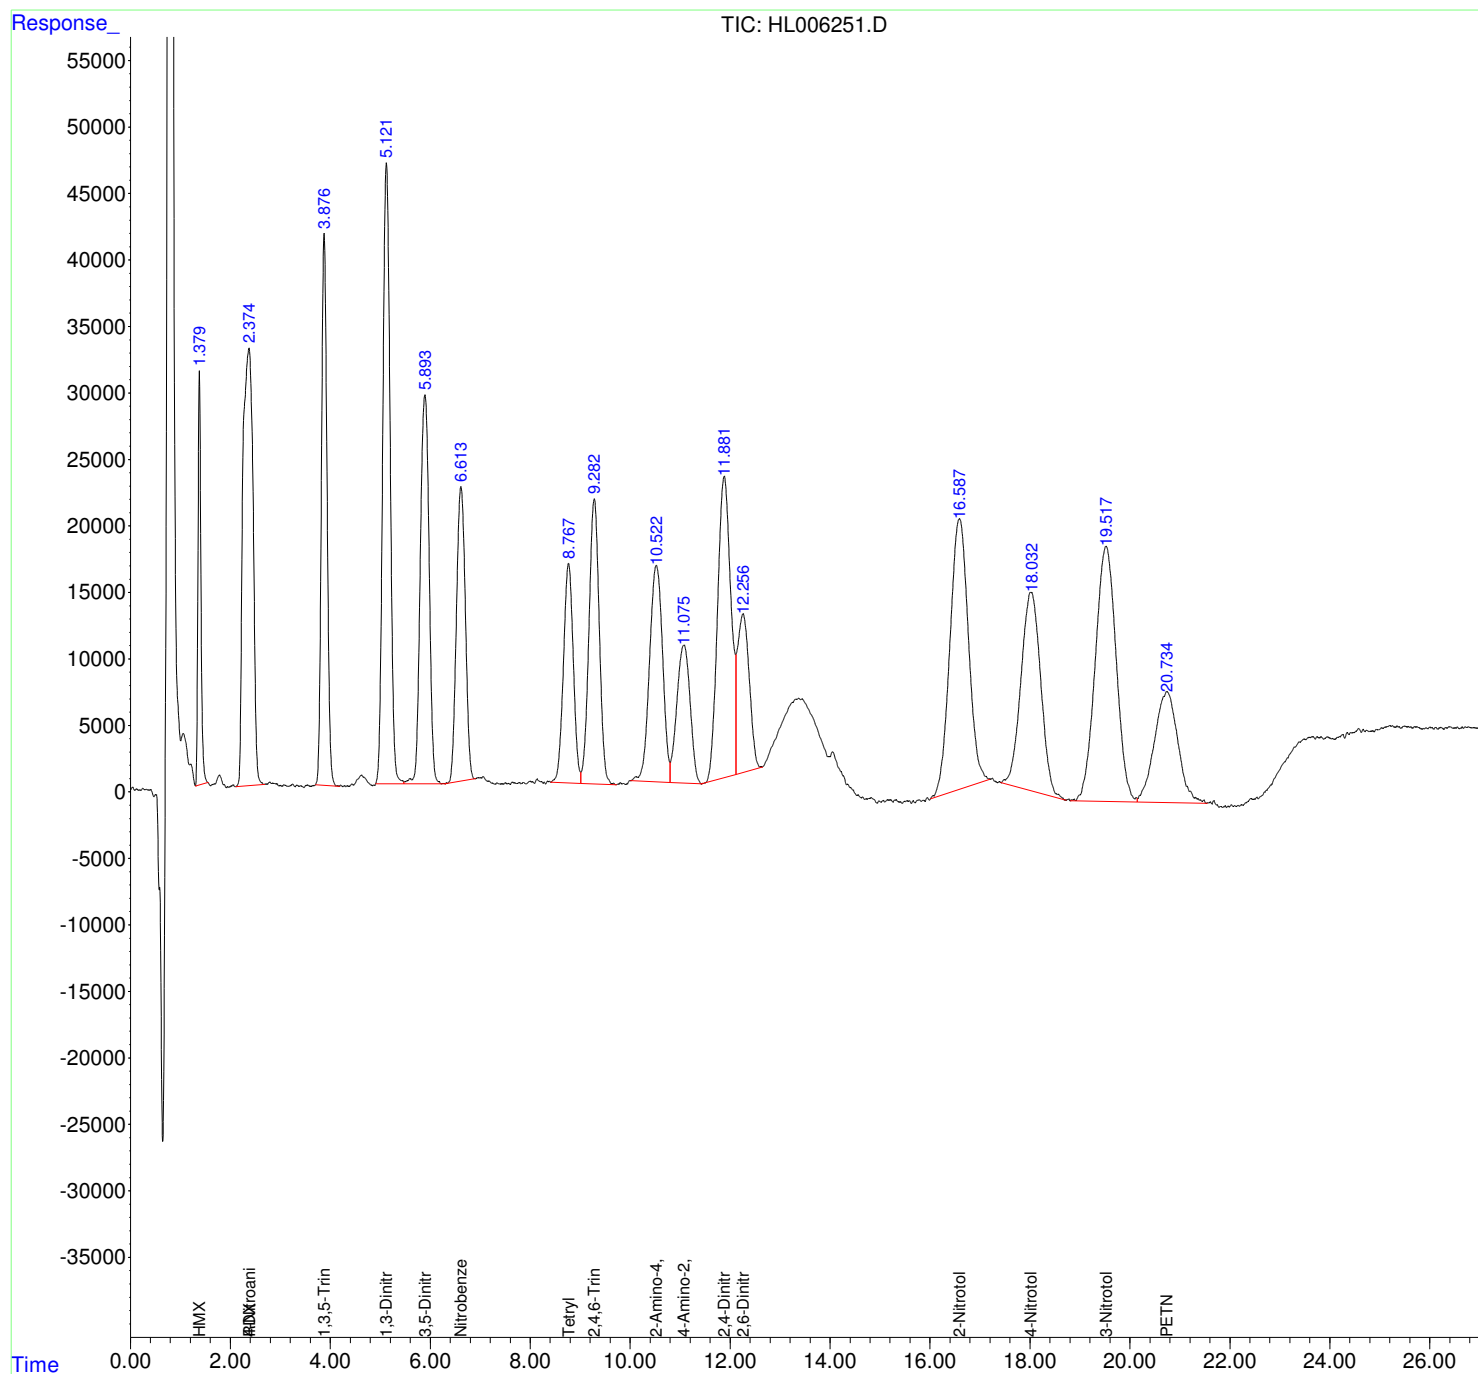


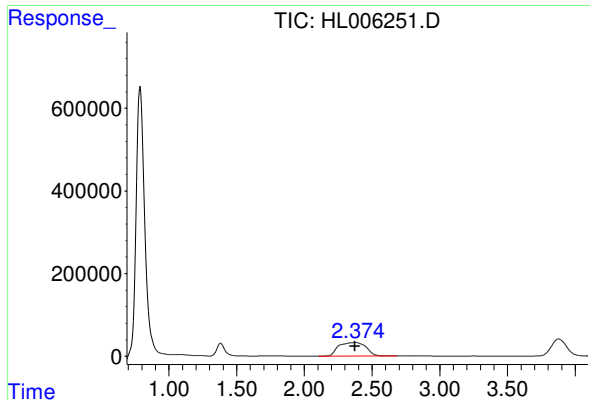

#1 4-Nitroaniline


R.T.: 2.371 min
Delta R.T.: 0.000 min
Response: 4614991
Conc: 330.28 ug/L

Instrument :
HPLC_L
ClientSampleId :

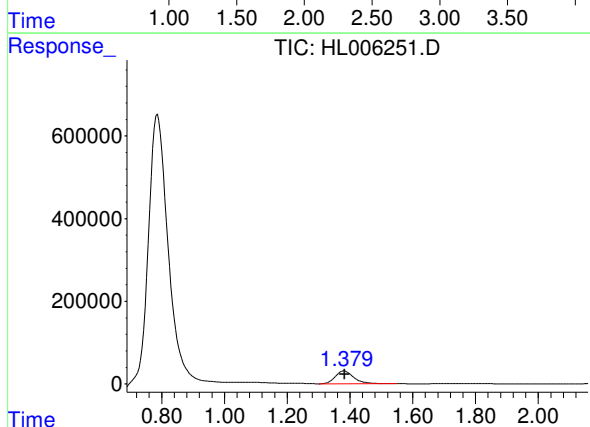


#2 HMX

R.T.: 1.382 min
Delta R.T.: 0.000 min
Response: 1269733
Conc: 197.47 ug/L

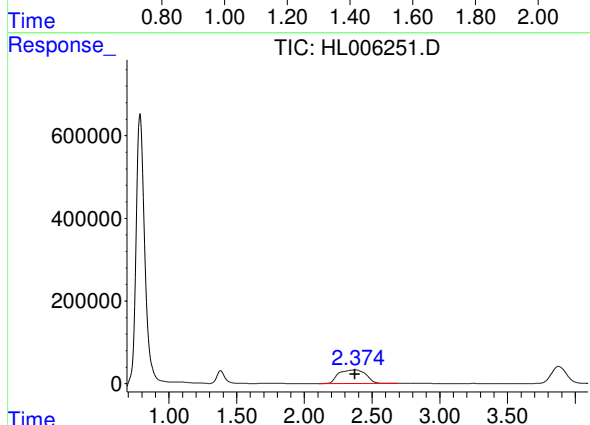


#3 RDX

R.T.: 2.371 min
Delta R.T.: 0.000 min
Response: 4614991
Conc: 330.28 ug/L

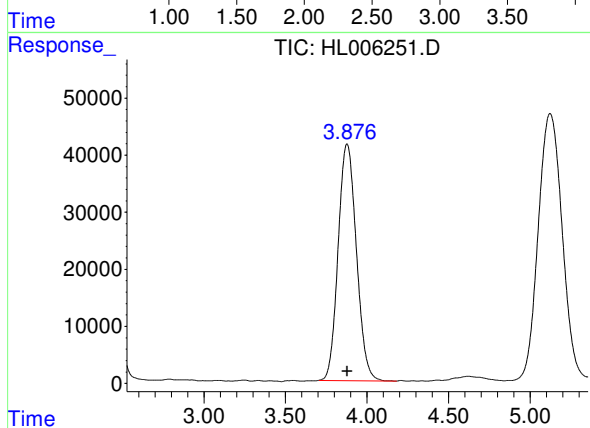

#4 1,3,5-Trinitrobenzene


R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 3232288
Conc: 199.75 ug/L

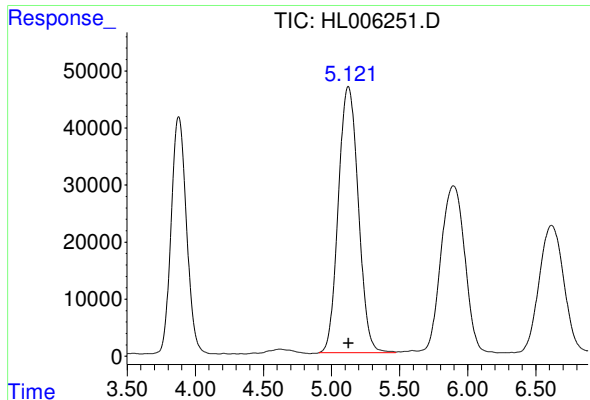

#5 1,3-Dinitrobenzene


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 4769032
Conc: 197.43 ng/ml

Instrument :
HPLC_L
ClientSampleId :

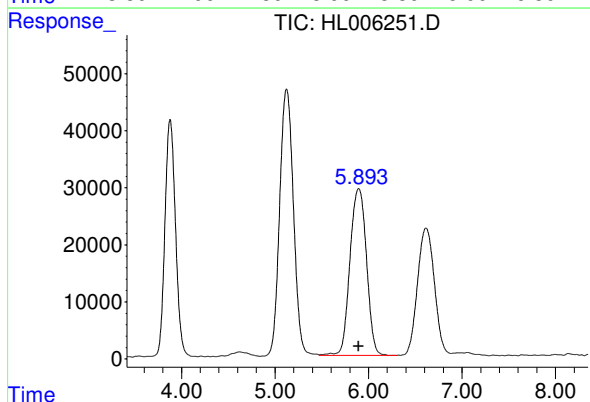


#6 3,5-Dinitroaniline

R.T.: 5.895 min
Delta R.T.: 0.000 min
Response: 3603898
Conc: 193.00 ug/L

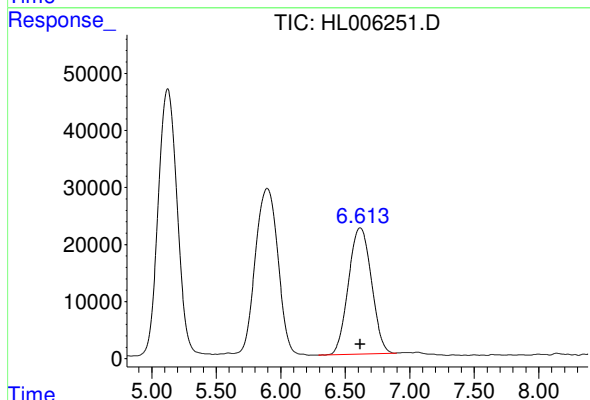


#7 Nitrobenzene

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 2742356
Conc: 198.68 ug/L

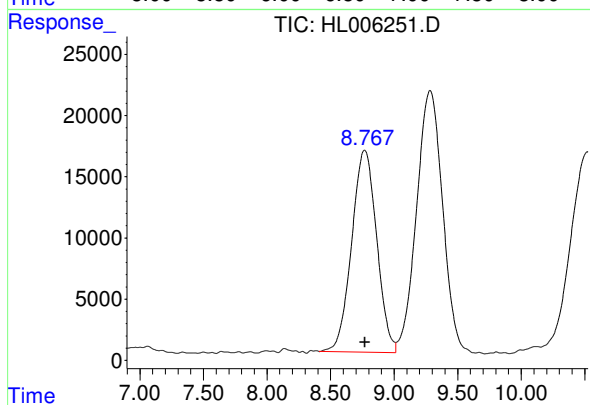

#8 Tetryl


R.T.: 8.768 min
Delta R.T.: 0.000 min
Response: 2255460
Conc: 207.13 ug/L

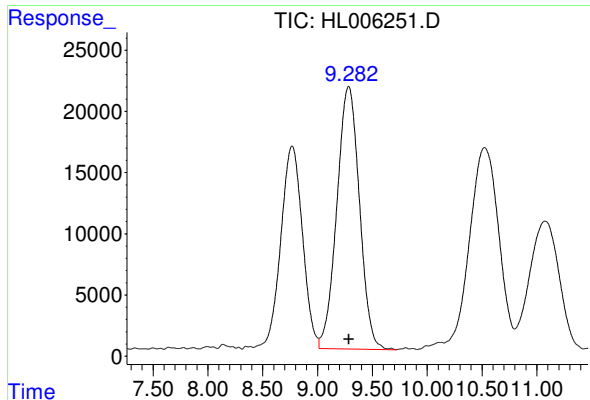

#9 2,4,6-Trinitrotoluene


R.T.: 9.283 min
Delta R.T.: 0.000 min
Response: 3066893
Conc: 182.15 ug/L

Instrument :
HPLC_L
ClientSampleId :

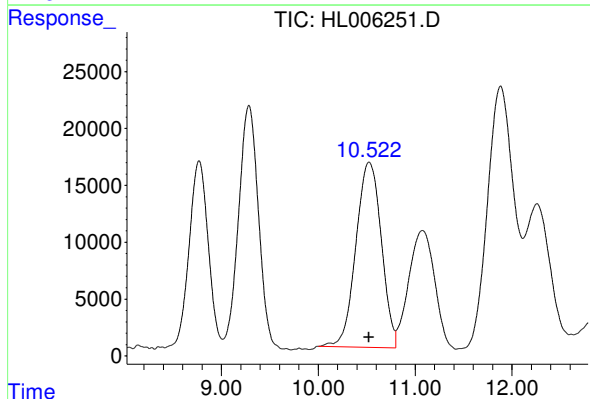


#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.524 min
Delta R.T.: 0.000 min
Response: 2971892
Conc: 149.12 ug/L

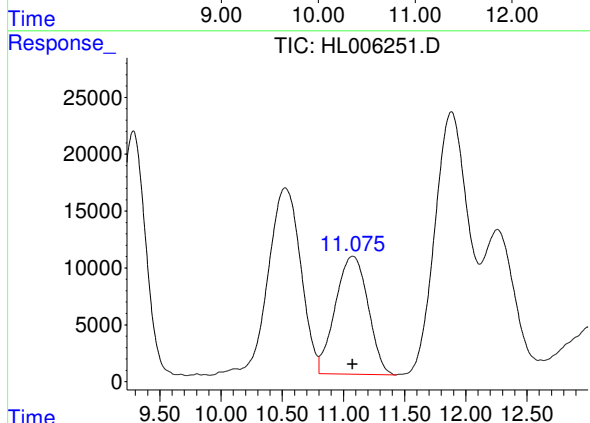


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.075 min
Delta R.T.: 0.000 min
Response: 1930472
Conc: 177.06 ug/L

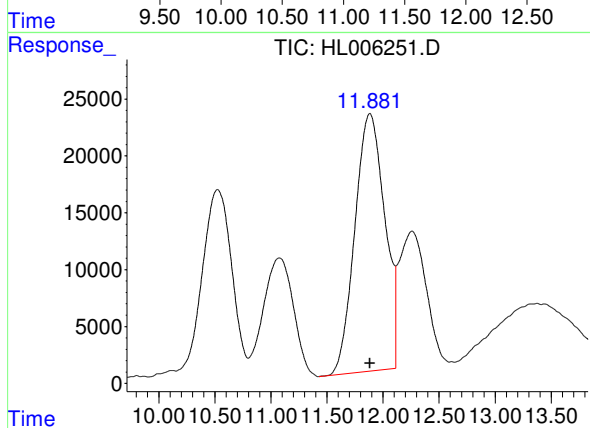

#12 2,4-Dinitrotoluene


R.T.: 11.882 min
Delta R.T.: 0.000 min
Response: 4208412
Conc: 187.02 ug/L

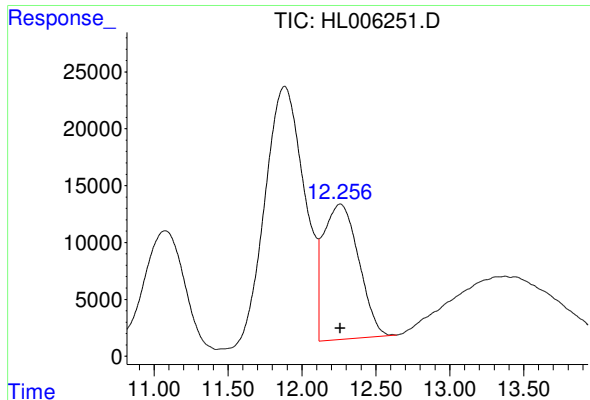

#13 2,6-Dinitrotoluene


R.T.: 12.259 min
Delta R.T.: 0.002 min
Response: 1966763
Conc: 178.30 ug/L

Instrument :
HPLC_L
ClientSampleId :

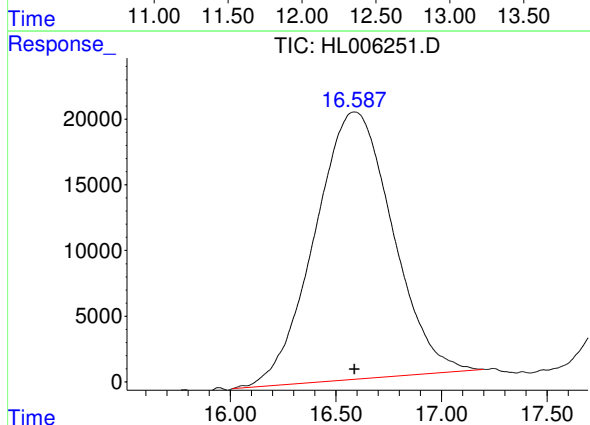


#14 2-Nitrotoluene

R.T.: 16.589 min
Delta R.T.: 0.000 min
Response: 5233496
Conc: 200.98 ug/L

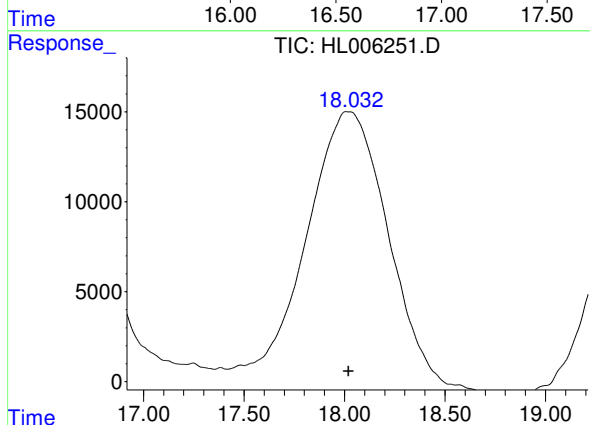


#15 4-Nitrotoluene

R.T.: 18.019 min
Delta R.T.: 0.000 min
Response: 4100518
Conc: 185.13 ug/L

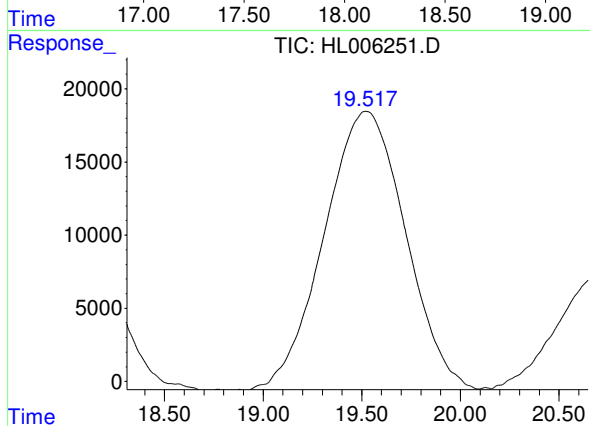

#16 3-Nitrotoluene

R.T.: 19.523 min
Delta R.T.: 0.006 min
Response: 5574264
Conc: 187.75 ug/L

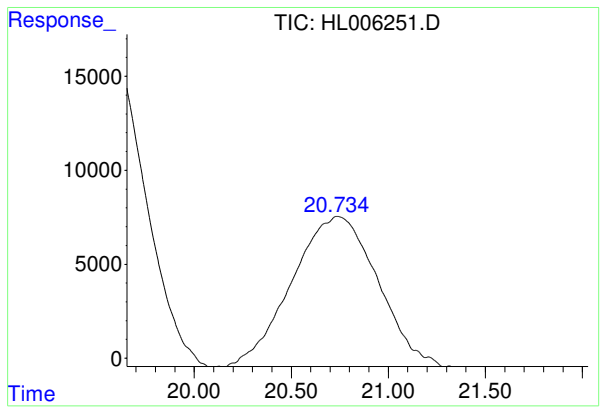

#17 PETN

R.T.: 20.742 min
Delta R.T.: 0.000 min
Response: 2731264
Conc: 207.96 ug/L

Instrument :
HPLC_L
ClientSampleId :