

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
 Data File : HL006252.D
 Signal(s) : vwd1A.ch
 Acq On : 24-Jun-2015, 22:44
 Operator : TP/IZ
 Sample : SSTDCCC0500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :

Integration File: AUTOINT1.E
 Quant Time: Jun 25 08:08:31 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
 Quant Title :
 QLast Update : Thu Jun 25 08:08:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	2.423	6644112	475.497 ug/L
Target Compounds				
2) T	HMX	1.389	3027303	470.813 ug/L
3) T	RDX	2.423	6644112	475.497 ug/L
4) T	1,3,5-Trinitrobenzene	3.888	7717538	476.936 ug/L
5) T	1,3-Dinitrobenzene	5.132	11432168	473.277 ng/ml
6) T	3,5-Dinitroaniline	5.905	8861835	474.571 ug/L
7) T	Nitrobenzene	6.620	6620707	479.653 ug/L
8) T	Tetryl	8.773	5511200	506.131 ug/L
9) T	2,4,6-Trinitrotoluene	9.286	7418419	440.593 ug/L
10) T	2-Amino-4,6-dinitroto...	10.531	7323502	443.267 ug/L
11) T	4-Amino-2,6-dinitroto...	11.075	4811943	441.351 ug/L
12) T	2,4-Dinitrotoluene	11.881	10622372	472.066 ug/L
13) T	2,6-Dinitrotoluene	12.252	5258554	476.729 ug/L
14) T	2-Nitrotoluene	16.576	12340252	473.898 ug/L
15) T	4-Nitrotoluene	18.010	9933584	448.491 ug/L
16) T	3-Nitrotoluene	19.504	13762080	463.536 ug/L
17) T	PETN	20.667	6455133	491.494 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
Data File : HL006252.D
Signal(s) : vwd1A.ch
Acq On : 24-Jun-2015, 22:44
Operator : TP/IZ
Sample : SSTDC00500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: AUTOINT1.E
Quant Time: Jun 25 08:08:31 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
Quant Title :
QLast Update : Thu Jun 25 08:08:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

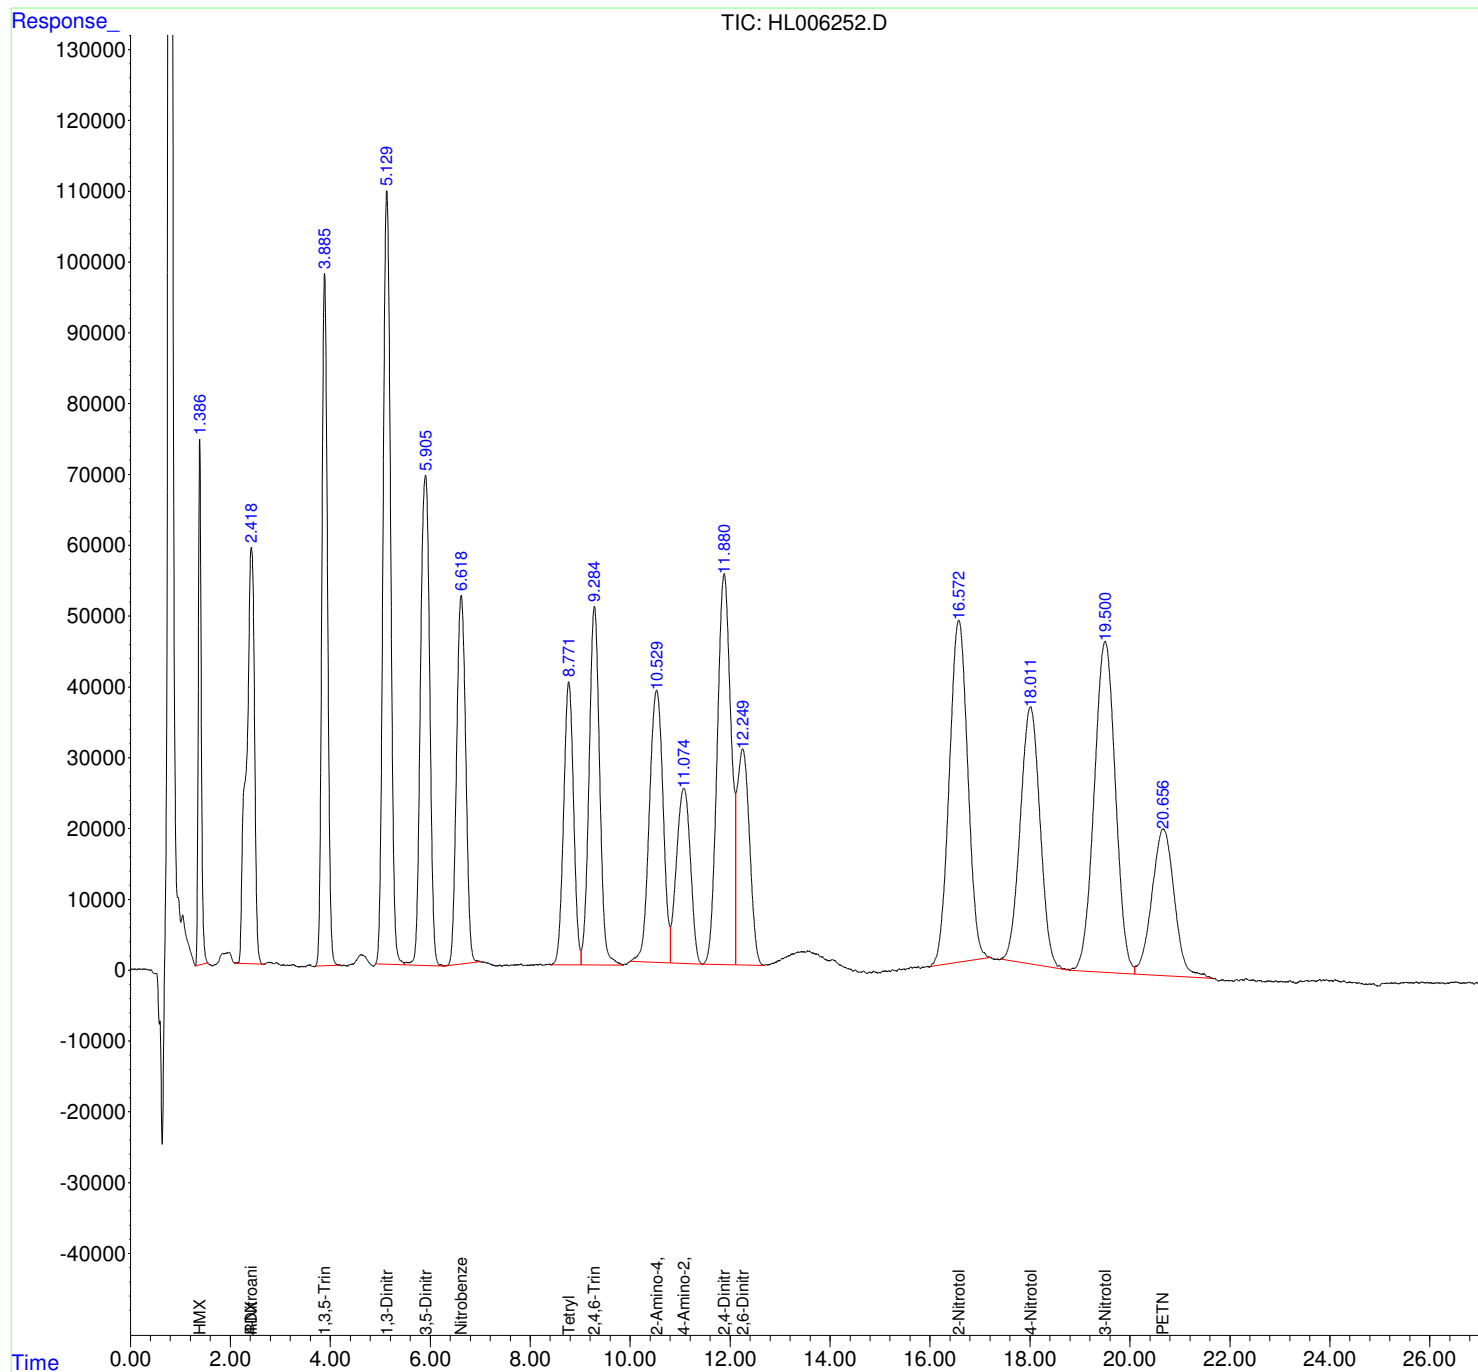


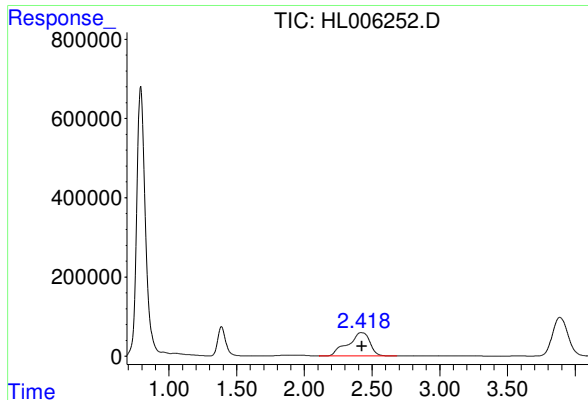

#1 4-Nitroaniline


R.T.: 2.423 min
Delta R.T.: 0.000 min
Response: 6644112
Conc: 475.50 ug/L

Instrument :
HPLC_L
ClientSampleId :

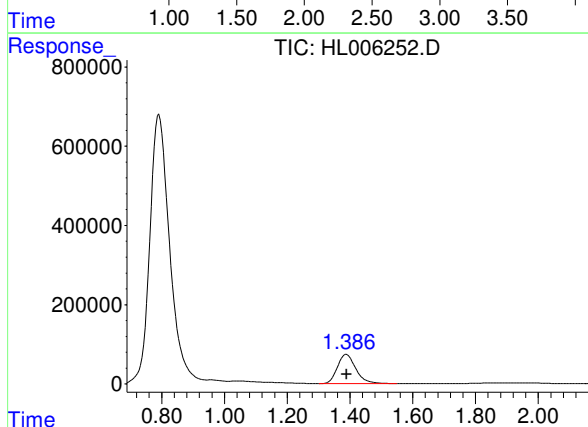


#2 HMX

R.T.: 1.389 min
Delta R.T.: 0.000 min
Response: 3027303
Conc: 470.81 ug/L

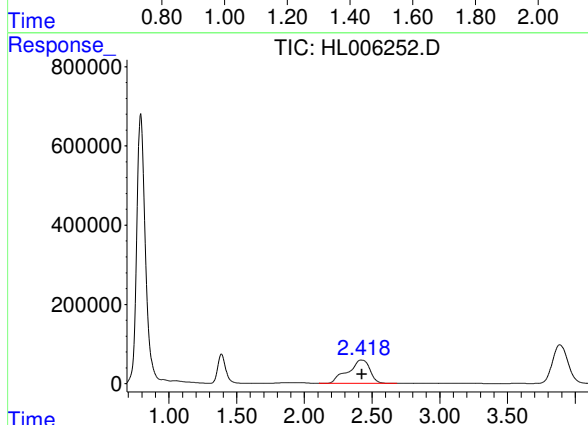


#3 RDX

R.T.: 2.423 min
Delta R.T.: 0.000 min
Response: 6644112
Conc: 475.50 ug/L

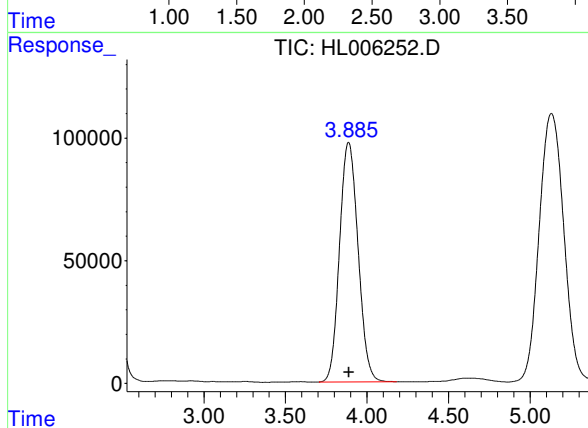

#4 1,3,5-Trinitrobenzene


R.T.: 3.888 min
Delta R.T.: 0.000 min
Response: 7717538
Conc: 476.94 ug/L

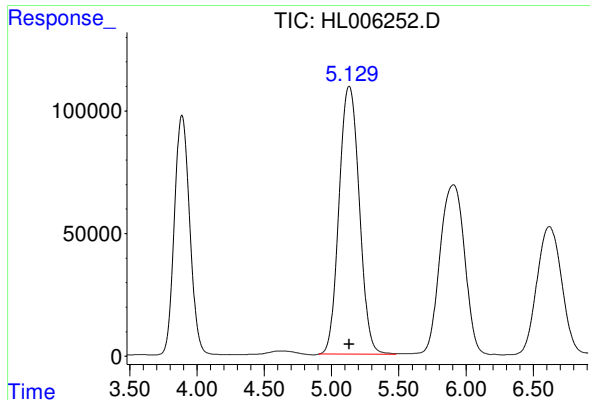

#5 1,3-Dinitrobenzene


R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 11432168
Conc: 473.28 ng/ml

Instrument :
HPLC_L
ClientSampleId :

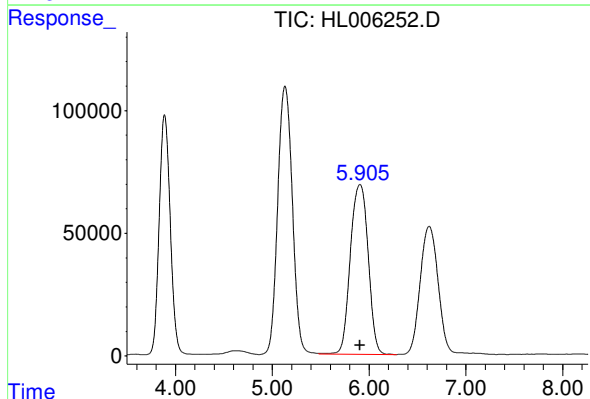


#6 3,5-Dinitroaniline

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 8861835
Conc: 474.57 ug/L

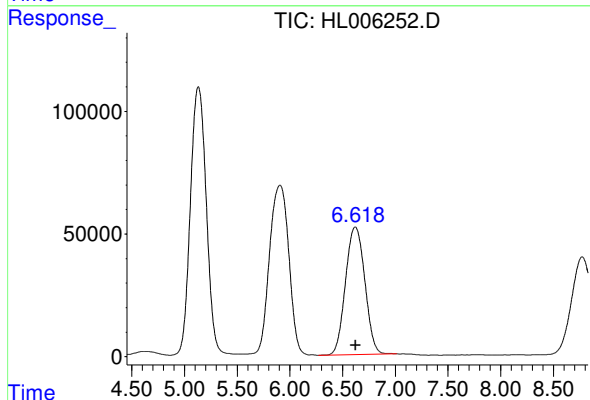


#7 Nitrobenzene

R.T.: 6.620 min
Delta R.T.: 0.000 min
Response: 6620707
Conc: 479.65 ug/L

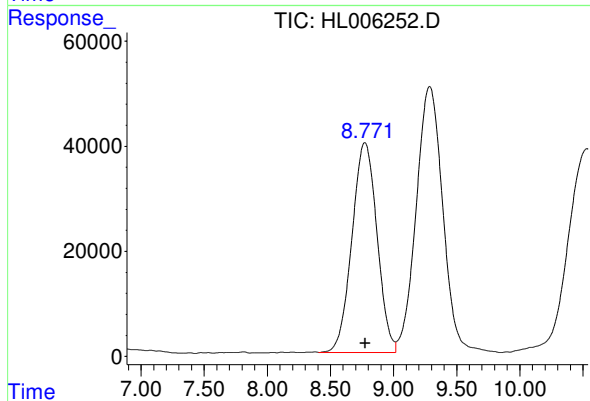

#8 Tetryl


R.T.: 8.773 min
Delta R.T.: 0.000 min
Response: 5511200
Conc: 506.13 ug/L

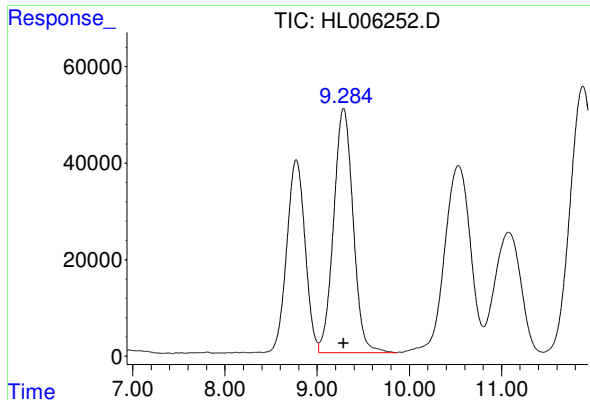

#9 2,4,6-Trinitrotoluene


R.T.: 9.286 min
Delta R.T.: 0.000 min
Response: 7418419
Conc: 440.59 ug/L

Instrument :
HPLC_L
ClientSampleId :

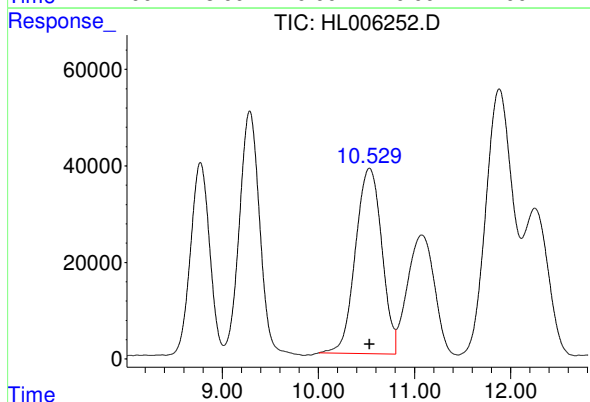


#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.531 min
Delta R.T.: 0.000 min
Response: 7323502
Conc: 443.27 ug/L

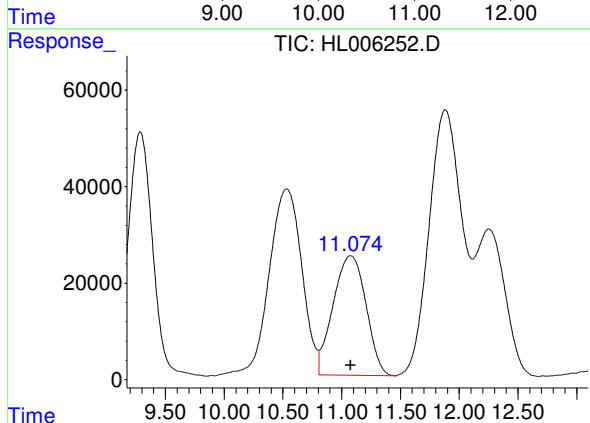


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.075 min
Delta R.T.: 0.000 min
Response: 4811943
Conc: 441.35 ug/L

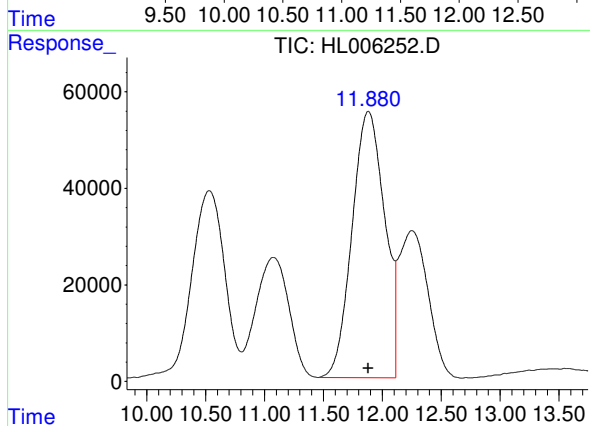

#12 2,4-Dinitrotoluene


R.T.: 11.881 min
Delta R.T.: 0.000 min
Response: 10622372
Conc: 472.07 ug/L

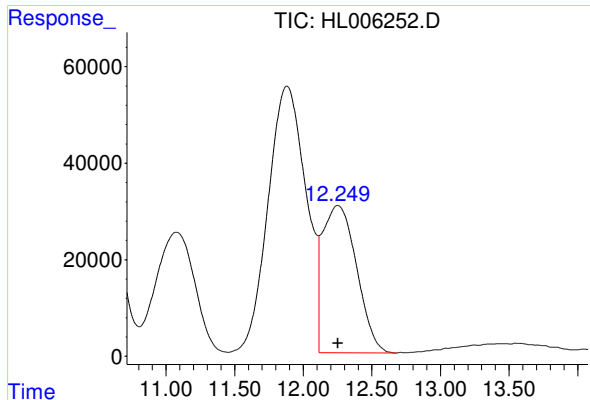

#13 2,6-Dinitrotoluene


R.T.: 12.252 min
Delta R.T.: 0.000 min
Response: 5258554
Conc: 476.73 ug/L

Instrument :
HPLC_L
ClientSampleId :

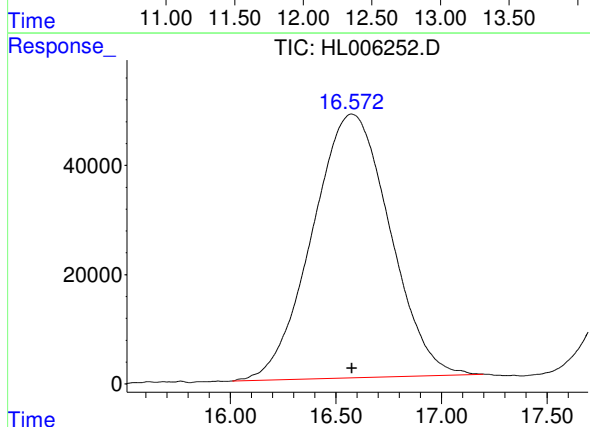


#14 2-Nitrotoluene

R.T.: 16.576 min
Delta R.T.: 0.000 min
Response: 12340252
Conc: 473.90 ug/L

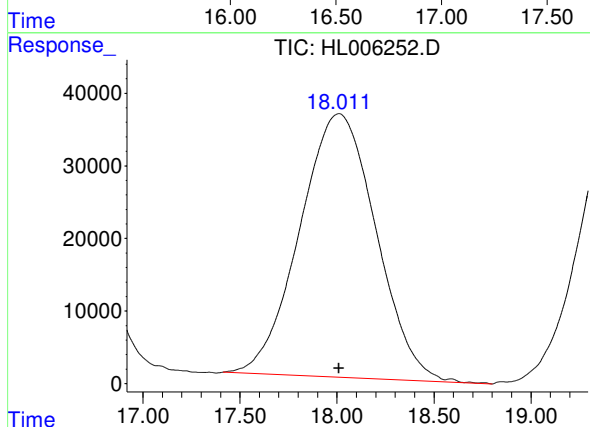


#15 4-Nitrotoluene

R.T.: 18.010 min
Delta R.T.: 0.000 min
Response: 9933584
Conc: 448.49 ug/L

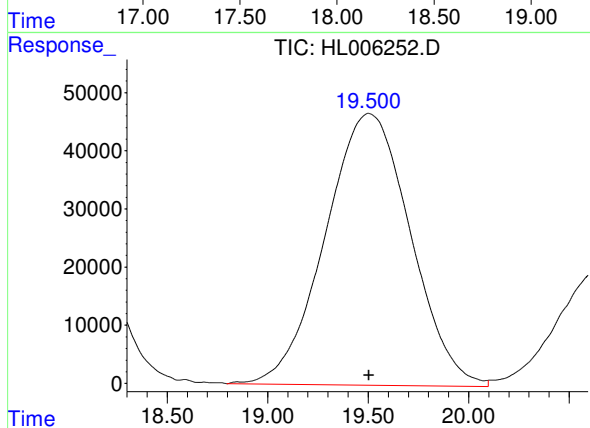

#16 3-Nitrotoluene

R.T.: 19.504 min
Delta R.T.: 0.000 min
Response: 13762080
Conc: 463.54 ug/L

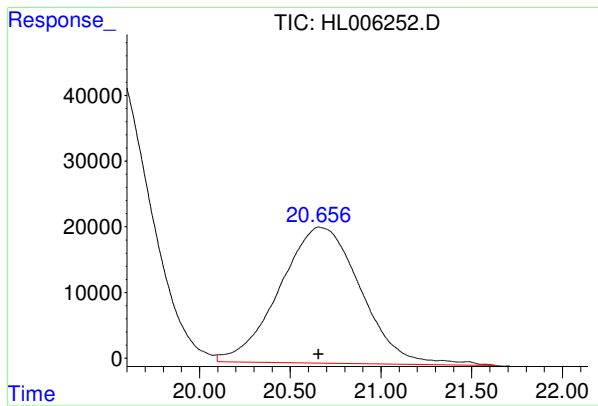

#17 PETN

R.T.: 20.667 min
Delta R.T.: 0.012 min
Response: 6455133
Conc: 491.49 ug/L

Instrument :
HPLC_L
ClientSampleId :