

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
 Data File : HL006244.D
 Signal(s) : vwd1A.ch
 Acq On : 24-Jun-2015, 18:57
 Operator : TP/IZ
 Sample : SSTDICC2000
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 SSTDICC2000

Integration File: AUTOINT1.E
 Quant Time: Jul 10 08:08:28 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
 Quant Title :
 QLast Update : Fri Jul 10 08:08:15 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.289	3546905	1765.665 ug/L m
Target Compounds			
2) T HMX	1.397	12306170	1968.292 ug/L
3) T RDX	2.418	23068050	1903.837 ug/L m
4) T 1,3,5-Trinitrobenzene	3.921	31281879	1932.348 ug/L
5) T 1,3-Dinitrobenzene	5.180	47198617	1948.027 ng/ml
6) T 3,5-Dinitroaniline	5.967	36171991	1935.149 ug/L
7) T Nitrobenzene	6.688	27044580	1959.834 ug/L
8) T Tetryl	8.862	19588225	1775.071 ug/L
9) T 2,4,6-Trinitrotoluene	9.387	30007167	1793.892 ug/L
10) T 2-Amino-4,6-dinitroto...	10.645	30393107	1744.731 ug/L
11) T 4-Amino-2,6-dinitroto...	11.196	19695756	1805.661 ug/L
12) T 2,4-Dinitrotoluene	12.016	44579530	1981.146 ug/L
13) T 2,6-Dinitrotoluene	12.389	20664232	1873.373 ug/L
14) T 2-Nitrotoluene	16.772	50587523	1975.220 ug/L
15) T 4-Nitrotoluene	18.228	40919076	1901.145 ug/L
16) T 3-Nitrotoluene	19.744	56478715	1936.264 ug/L
17) T PETN	20.944	25153102	1947.044 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL062415\
Data File : HL006244.D
Signal(s) : vwd1A.ch
Acq On : 24-Jun-2015, 18:57
Operator : TP/IZ
Sample : SSTDICC2000
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

Integration File: AUTOINT1.E
Quant Time: Jul 10 08:08:28 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL062415.M
Quant Title :
QLast Update : Fri Jul 10 08:08:15 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

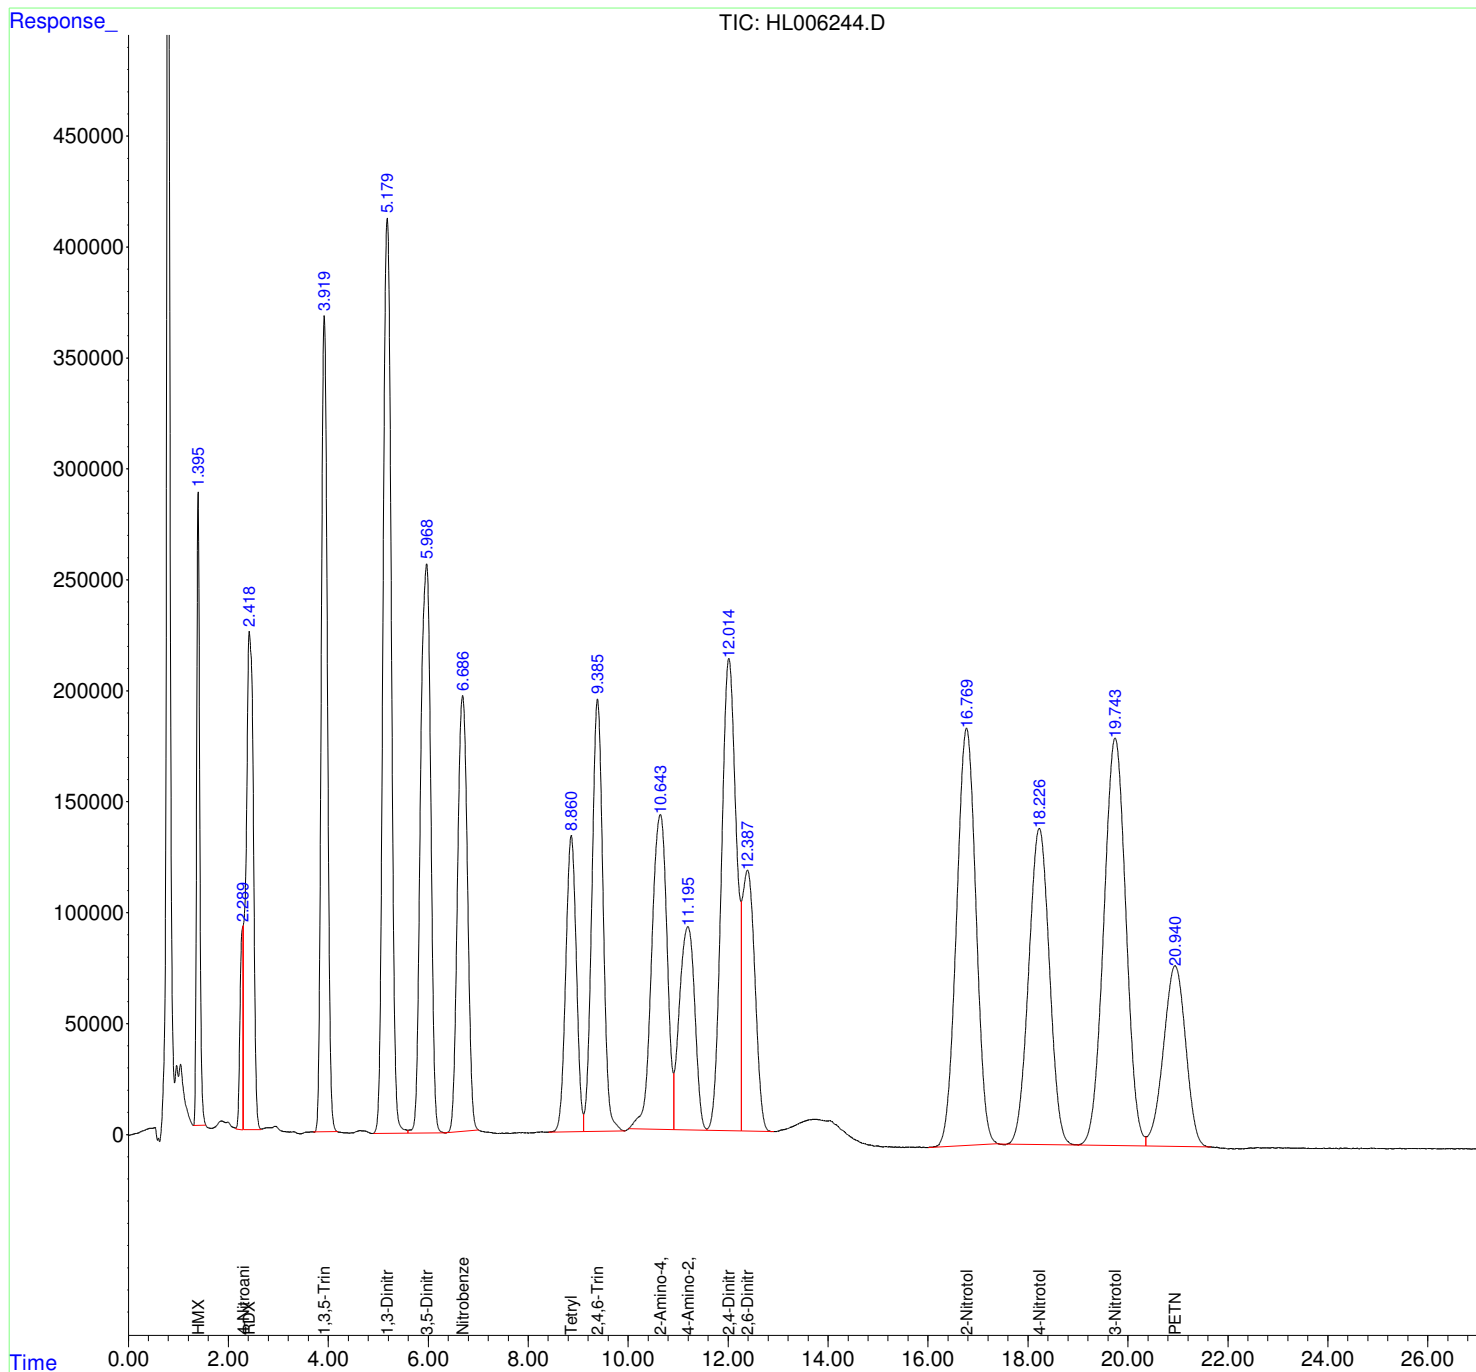


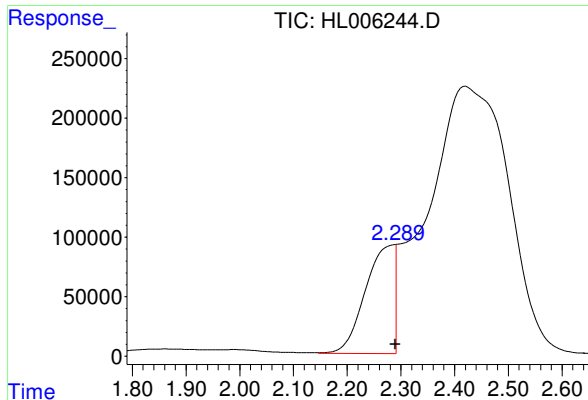

#1 4-Nitroaniline


R.T.: 2.289 min
Delta R.T.: 0.000 min
Response: 3546905
Conc: 1765.67 ug/L m

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

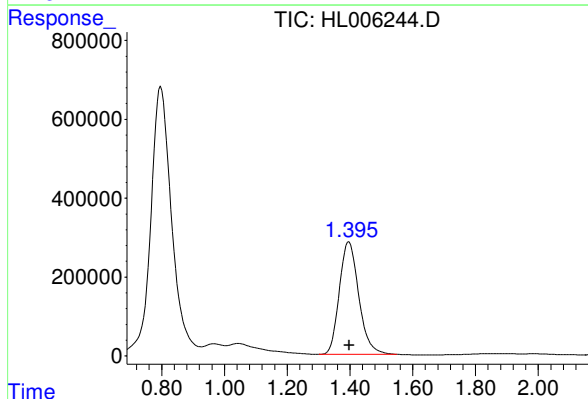


#2 HMX

R.T.: 1.397 min
Delta R.T.: 0.000 min
Response: 12306170
Conc: 1968.29 ug/L

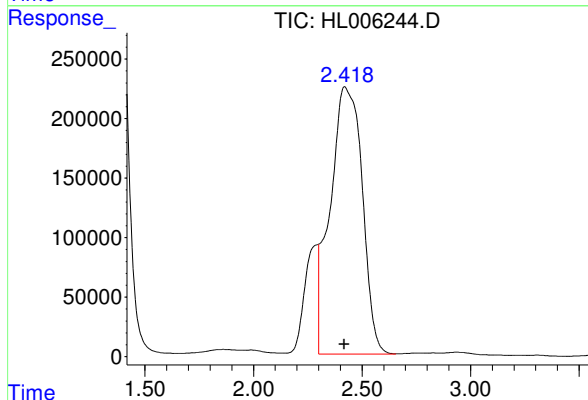


#3 RDX

R.T.: 2.418 min
Delta R.T.: 0.000 min
Response: 23068050
Conc: 1903.84 ug/L m

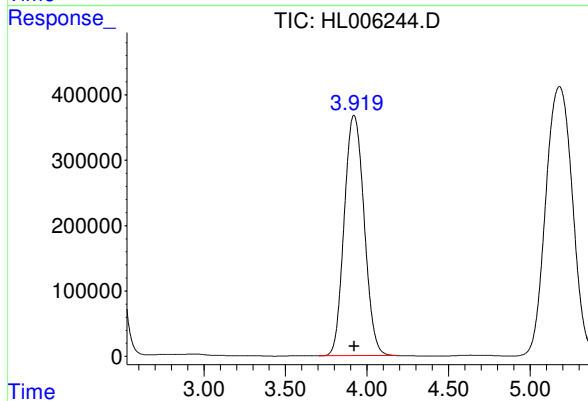

#4 1,3,5-Trinitrobenzene


R.T.: 3.921 min
Delta R.T.: 0.000 min
Response: 31281879
Conc: 1932.35 ug/L

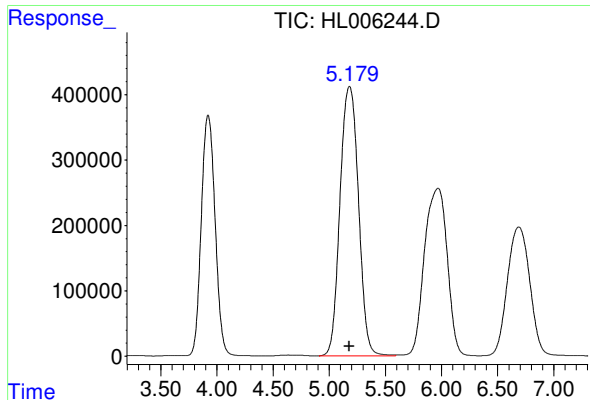

#5 1,3-Dinitrobenzene


R.T.: 5.180 min
Delta R.T.: 0.000 min
Response: 47198617
Conc: 1948.03 ng/ml

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

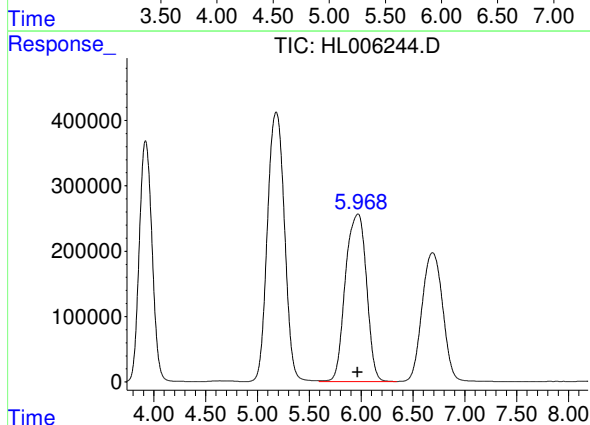


#6 3,5-Dinitroaniline

R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 36171991
Conc: 1935.15 ug/L

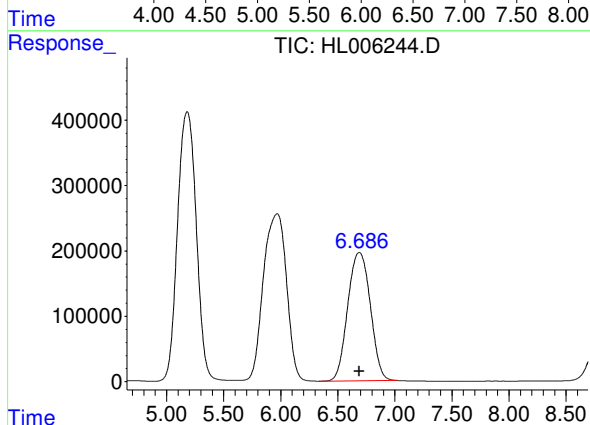


#7 Nitrobenzene

R.T.: 6.688 min
Delta R.T.: 0.000 min
Response: 27044580
Conc: 1959.83 ug/L

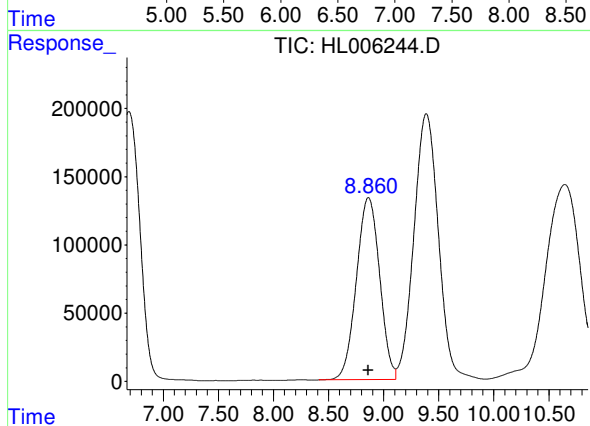

#8 Tetryl


R.T.: 8.862 min
Delta R.T.: 0.000 min
Response: 19588225
Conc: 1775.07 ug/L

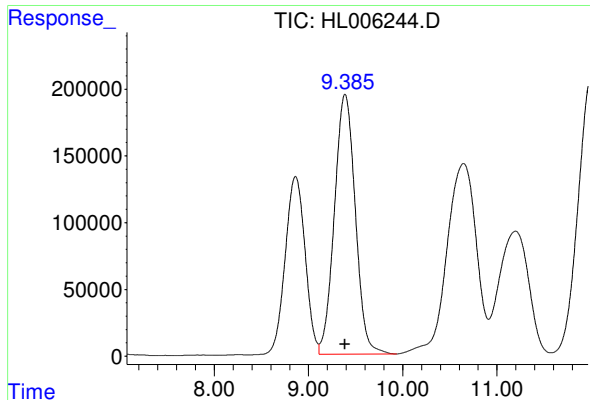

#9 2,4,6-Trinitrotoluene


R.T.: 9.387 min
Delta R.T.: 0.000 min
Response: 30007167
Conc: 1793.89 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

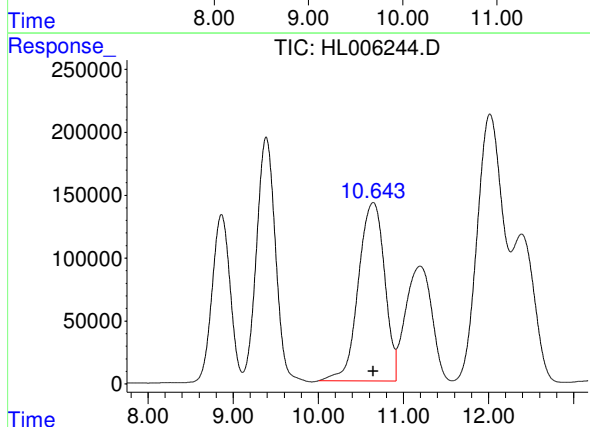


#10 2-Amino-4,6-dinitrotoluene

R.T.: 10.645 min
Delta R.T.: 0.000 min
Response: 30393107
Conc: 1744.73 ug/L

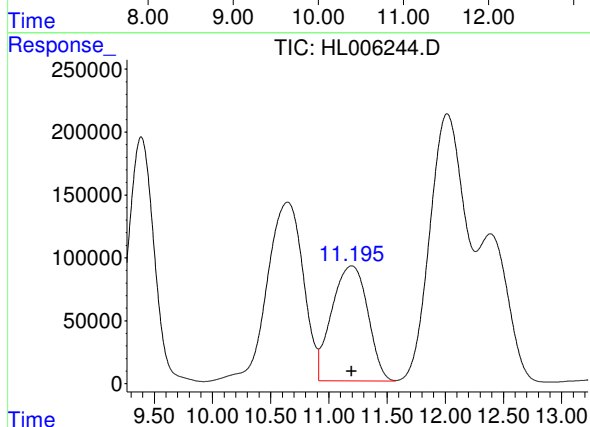


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.196 min
Delta R.T.: 0.000 min
Response: 19695756
Conc: 1805.66 ug/L

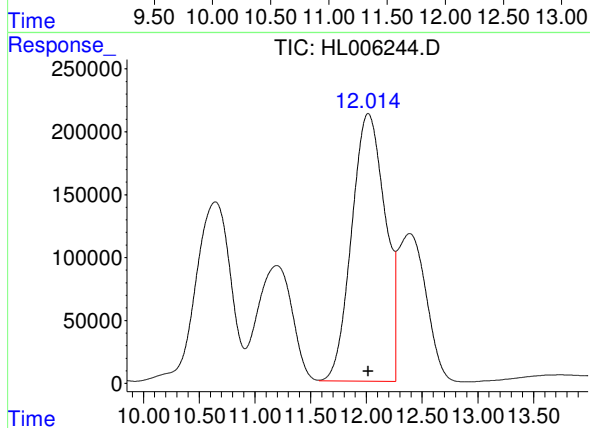

#12 2,4-Dinitrotoluene


R.T.: 12.016 min
Delta R.T.: 0.000 min
Response: 44579530
Conc: 1981.15 ug/L

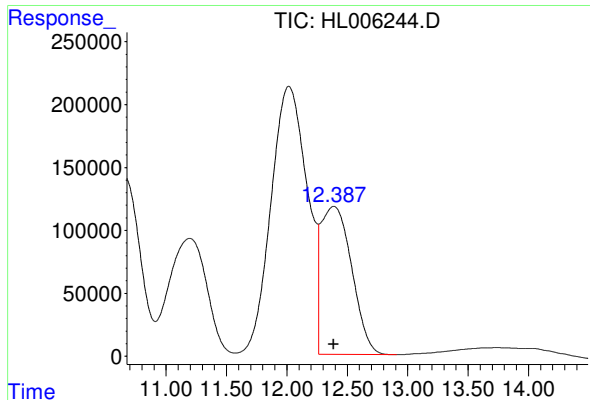

#13 2,6-Dinitrotoluene


R.T.: 12.389 min
Delta R.T.: 0.000 min
Response: 20664232
Conc: 1873.37 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

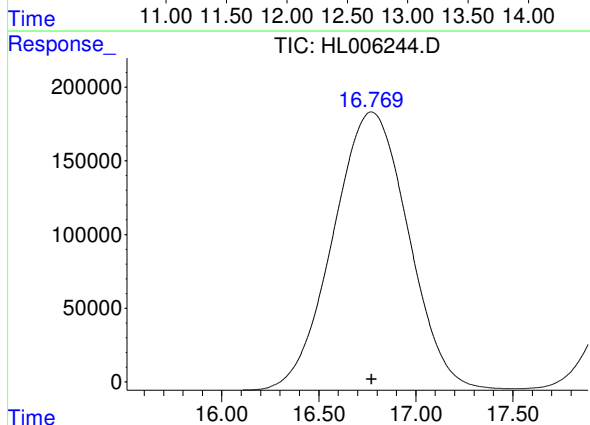


#14 2-Nitrotoluene

R.T.: 16.772 min
Delta R.T.: 0.000 min
Response: 50587523
Conc: 1975.22 ug/L

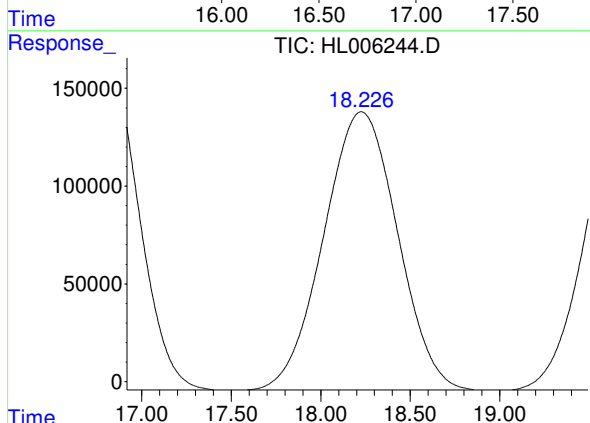


#15 4-Nitrotoluene

R.T.: 18.228 min
Delta R.T.: 0.000 min
Response: 40919076
Conc: 1901.15 ug/L

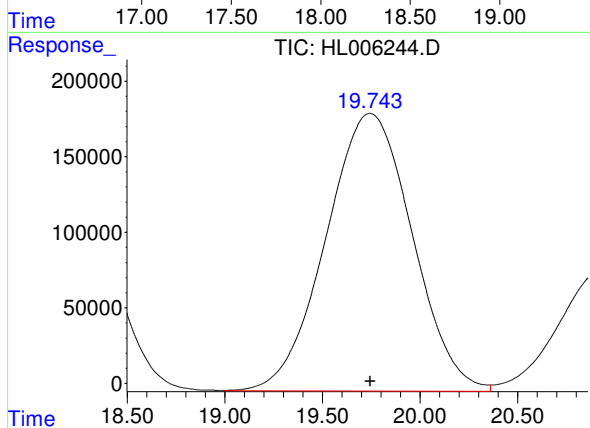

#16 3-Nitrotoluene

R.T.: 19.744 min
Delta R.T.: 0.000 min
Response: 56478715
Conc: 1936.26 ug/L

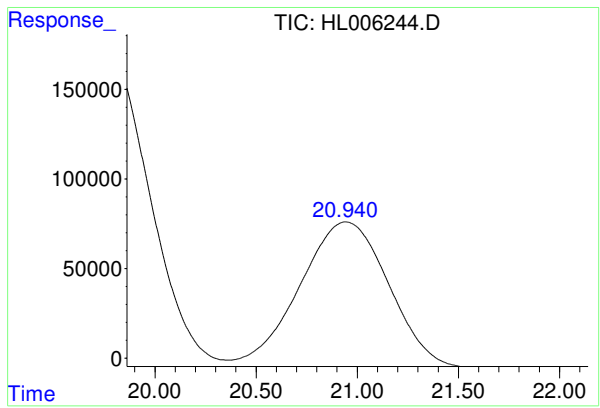

#17 PETN

R.T.: 20.944 min
Delta R.T.: 0.000 min
Response: 25153102
Conc: 1947.04 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000