

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL070213\HL005489.D Vial: 20
Acq On : 03-Jul-2013, 03:29 Operator: QM
Sample : E2747-18 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 3 3:31 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT02-SS7-062613

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 17:40:52 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.34	733080	181.014 ug/L
Target Compounds			
17) T PETN	19.54	1847496	170.825 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005489.D HL070213.M

Wed Jul 03 03:31:53 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL070213\HL005489.D Vial: 20
Acq On : 03-Jul-2013, 03:29 Operator: QM
Sample : E2747-18 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 3 3:31 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT02-SS7-062613

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 17:40:52 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

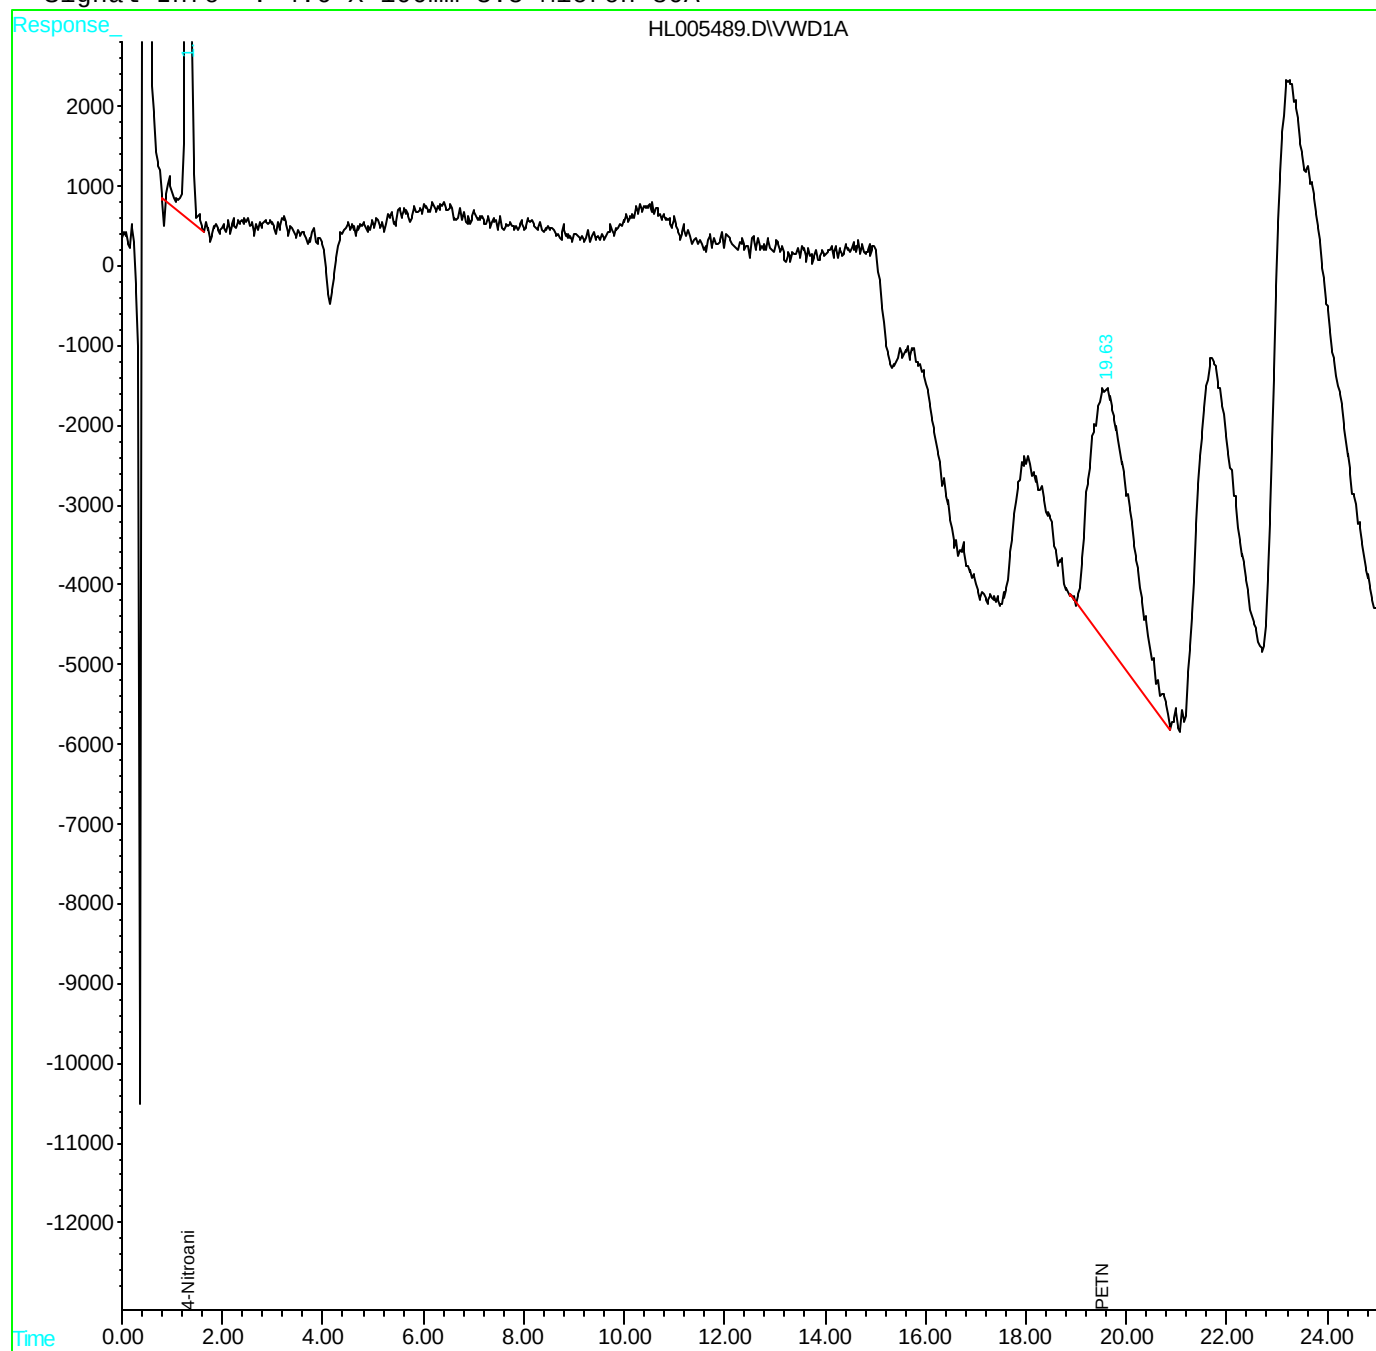


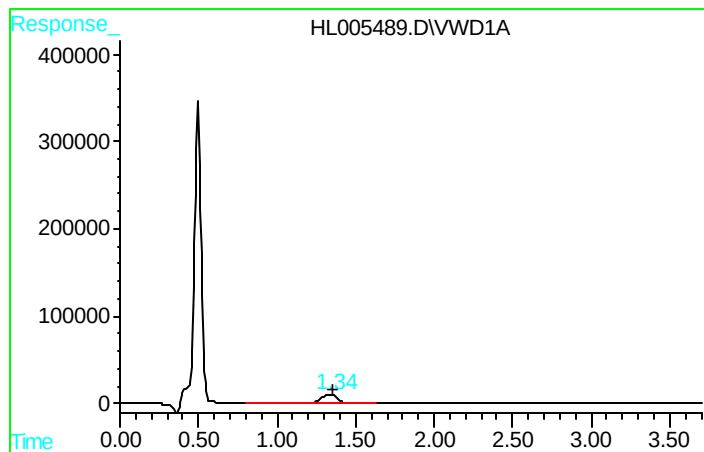

#1 4-Nitroaniline

R.T.: 1.339 min
Delta R.T.: -0.013 min
Response: 733080
Conc: 181.01 ug/L

Instrument :
HPLC_L
ClientSampleId :
POLJAT02-SS7-062613

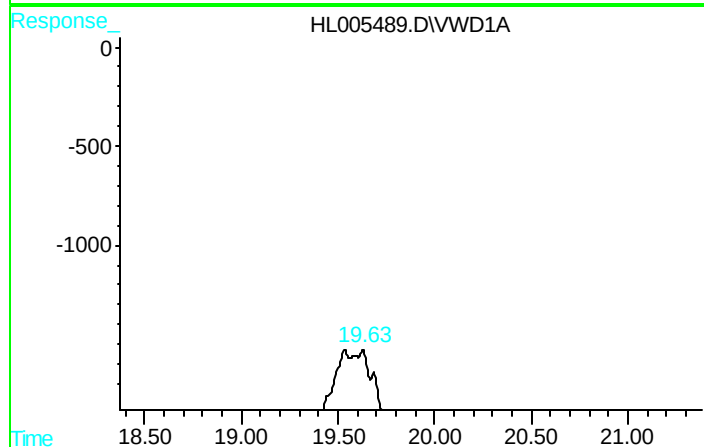

#17 PETN

R.T.: 19.540 min
Delta R.T.: -0.060 min
Response: 1847496
Conc: 170.83 ug/L